

Comparative Analysis for Peak Detection Techniques for Signal Processing

ASSESSMENT II

**Marta Alberola Martín,
Ravneet-Rahul Sandhu,
Roger Puig i Arxer**

Master in Health Data Science — MHEDAS

January 14, 2025



Co-funded by the
European Union



UNIVERSITAT ROVIRA I VIRGILI



BIOINFORMATICS
BARCELONA



Universitat Autònoma
de Barcelona



UNIVERSITAT DE
BARCELONA



Universitat
de Lleida



UNIVERSITAT POLITÈCNICA
DE CATALUNYA
BARCELONATECH



UNIVERSITAT DE VIC
UNIVERSITAT CENTRAL
DE CATALUNYA



Universitat
de Girona



Université
Grenoble Alpes

Table of Contents

1. Challenge	3
2. Methods	4
Scipy	4
Hybrid	7
Custom	10
3. Conclusions	13

- **Material:**
 - 25 noisy synthetic signals + Ground truth signals
 - Sampling frequency: 10 Hz
 - One example of a clean peak of intensity one

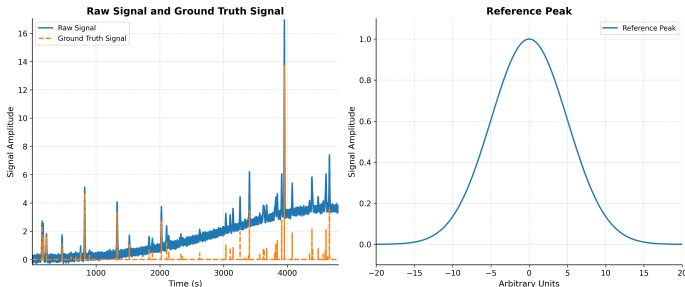


Figure: Noisy signal with ground truth peaks alongside the reference peak of intensity one.


```
scipy_method(sig, t, gt_sig, fs=10, win_dur=500, th1=0.25, th2=0.15)
```

- **Parameters:**

- **sig, t:** Input signal and time vector.
- **gt_sig:** Ground truth signal for peak detection.
- **fs:** Sampling frequency (Hz).
- **win_dur:** Window duration in seconds.
- **th1:** Threshold factor for peak height.
- **th2:** Threshold factor for peak prominence.

- **Windowed approach:**

- **No ground truth peaks:** Skip the window.
- **One ground truth peak:** height = 25% max value, prominence = 15% max value.
- **Multiple ground truth peaks:** height = 25% max value, distance = average ground truth spacing $\times$ fs, prominence = 15% max value.

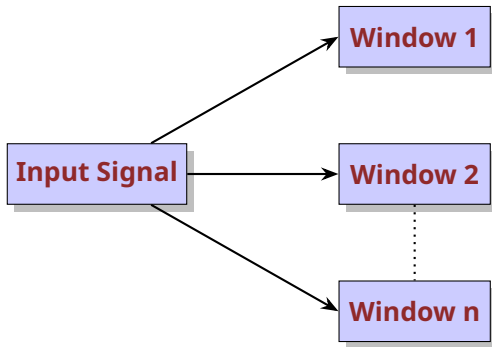

find_peaks(window_1, params)*

find_peaks(window_2, params)*

⋮

find_peaks(window_n, params)*

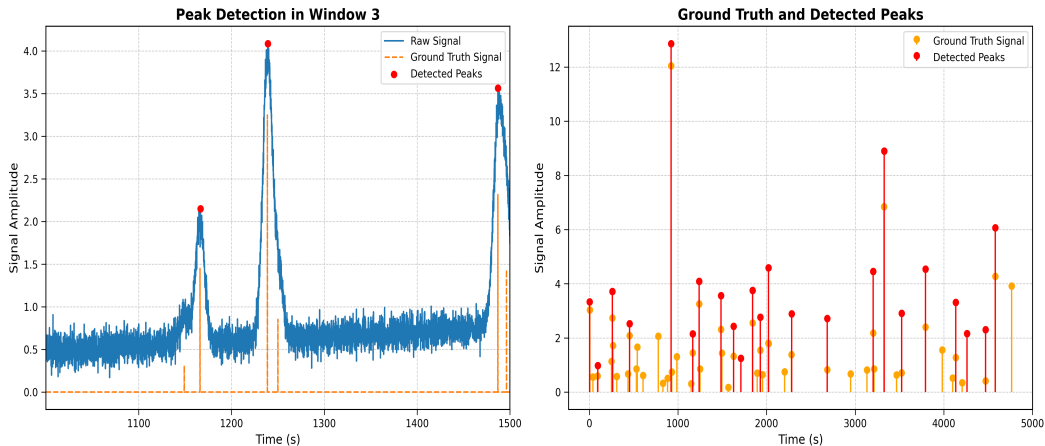
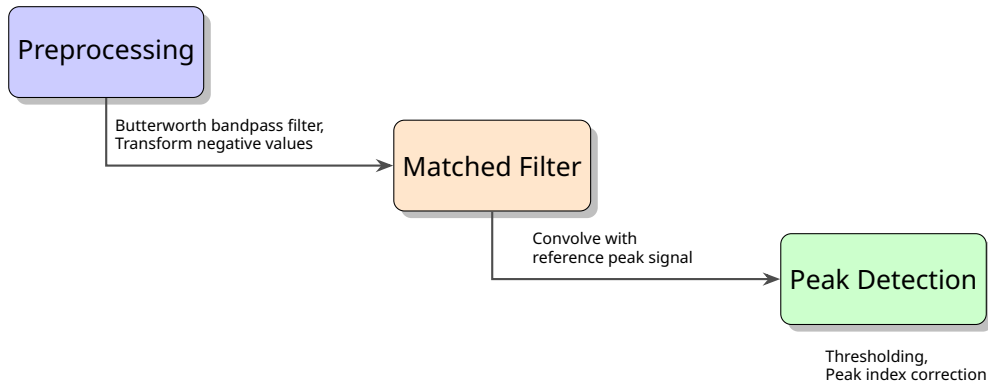


Figure: Peak detection process for a single window, along with the comparison of all detected peaks to ground truth peaks using the SciPy method.

```
hybrid_method(sig, t, ref, fs=10, order=1, lc=0.01, hc=0.1, th=0.01)
```

- **Parameters:**

- **sig, t:** Input signal and time vector.
- **ref:** Reference peak window for matched filtering.
- **fs:** Sampling frequency (Hz).
- **order, lc, hc:** Filter order, low cutoff frequency, and high cutoff frequency for the band-pass filter.
- **th:** Threshold factor to determine the peak detection threshold.



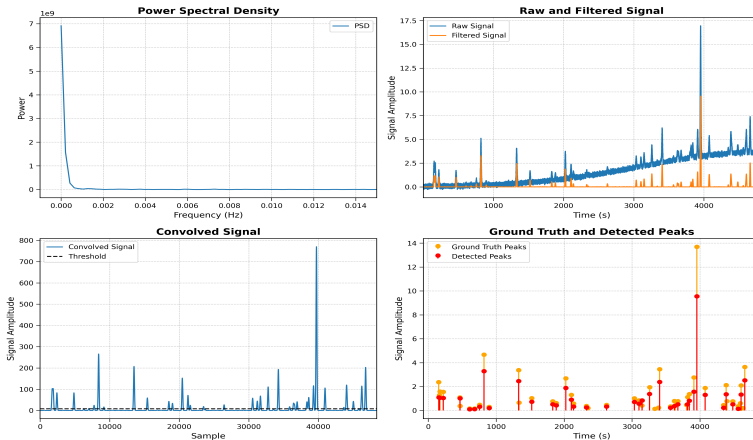
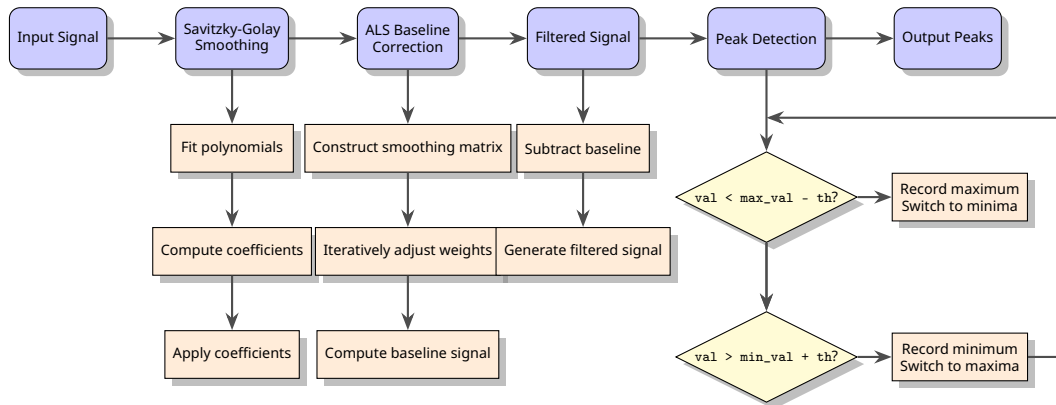


Figure: Representation of the power spectral density (PSD), raw signal, filtered signal, convolved signal, and the alignment of ground truth peaks with detected peaks using the hybrid method.

```
custom_method(sig, t, win_len=151, poly_order=3, lam=1e8, pen=0.001,  
              max_iter=50, th=0.1)
```

- **Parameters:**

- `sig`, `t`: Input signal and time vector.
- `win_len`: Window length for Savitzky-Golay smoothing.
- `poly_order`: Polynomial order for smoothing.
- `lam`: Smoothing parameter for ALS baseline removal.
- `pen`: Penalty parameter for ALS baseline removal.
- `max_iter`: Maximum iterations for ALS baseline removal.
- `th`: Threshold for peak detection.



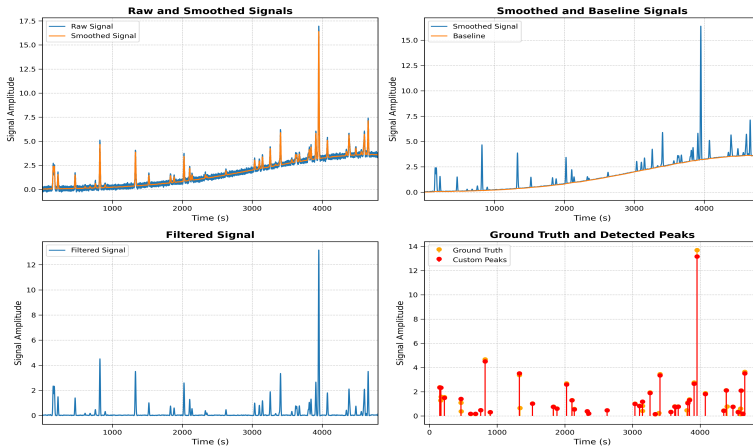


Figure: Raw, smoothed, baseline, and filtered signals processed using the custom method, along with detected peaks and ground truth peaks for comparison.

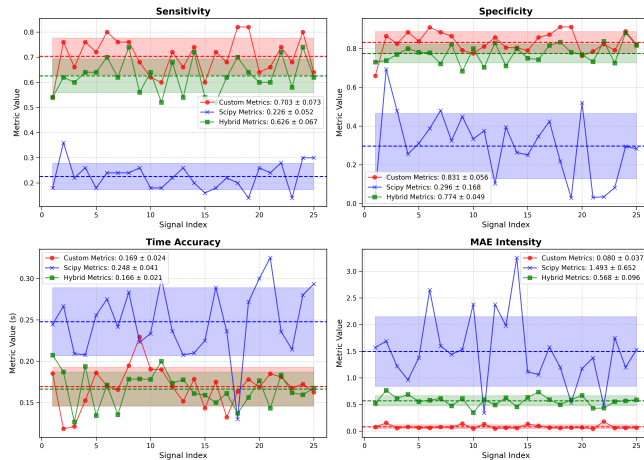


Figure: Performance comparison of all methods (tolerance = 500 ms).

Comparative Analysis for Peak Detection Techniques for Signal Processing

ASSESSMENT II

**Marta Alberola Martín,
Ravneet-Rahul Sandhu,
Roger Puig i Arxer**

Master in Health Data Science — MHEDAS

January 14, 2025



Co-funded by the
European Union



UNIVERSITAT ROVIRA I VIRGILI

