

1 Results from the Tritiated Methane Calibration

1.1 Tritium as a Calibration Source

Due to the self shielding properties of liquid xenon it is practically impossible to perform a low energy electronic recoil (ER) calibration within the fiducial volume of a +100 kg detector using an external source. The fiducial volume of the LUX detector is surrounded by more than 6 cm of liquid xenon providing excellent shielding from both external backgrounds and calibration sources. For example, a 100 keV gamma has a mean free path of about 2 mm in liquid xenon and would require thirty mean free paths to penetrate into the fiducial volume. A higher energy source such as ^{137}Cs (662 keV) has a longer mean free path of 4 cm however, the probability of a low energy deposit from forward scattering is greatly suppressed. Further, calibrating within the fiducial volume by relying on gammas from an external source to forward scatter brings along systematic uncertainties from high energy deposits near the edge, DAQ rate and having to use multi scatter event selection instead of a standard set of single scatter WIMP search cuts. An ideal ER calibration source for current and next generation noble gas detectors should consist of single scatter events depositing sub 10 keV energies uniformly distributed in the fiducial region. These requirements are all satisfied by tritium beta decay. Tritium has a Q value of 18.6 keV [1], a mean beta energy of 5.6 keV [2] and a mode of 3 keV [3] making it an ideal low energy internal calibration source, so long as it can be removed after calibration. The half-life of tritium is 12.3 years [4] thus it is not practical to wait for the activity to decay away as with other internal calibration sources, the tritium must be removed after the calibration is complete. To mitigate the effect of hydrogen diffusion into plastics, [link], we use tritiated methane instead of just tritium. The tritium atom is bound to the methane molecule lessening its diffusion into detector internals [described in sections, cite that Japanese paper] also, the molecular bond to the methane molecule does not impact the nuclear physics of the tritium beta decay. We have studied the removal of methane by the commonly used SAES heated zirconium getter and found that significant amounts of methane can be removed from xenon at flow rates commonly employed in large scale liquid xenon experiments [5][6].

In an experimental setup at UMD it was demonstrated that tritiated methane can be injected directly into a liquid xenon vessel containing plastics and removed [link section in this paper]. Before injecting tritiated methane into the LUX detector we first demonstrated the removal of natural methane to five orders of magnitude using an integrated xenon gas sampling system developed for LUX to track krypton, [7] [8]. Methane is chemically identical to tritiated methane and having the ability to sample the gas allowed us to infer that nothing was missed in the outgassing and absorption of methane by plastic components in LUX 2. At the end of the science run two tritiated methane injections were conducted at the end of the LUX science run in August 2013. An absolute activity of 20 mBq of tritiated methane was injected into the liquid volume at the purifier's outlet while circulating. A methane removal time constant of 6.7 hours was observed, consistent with the natural methane purification rate measured by the sampling system, 3 and 2. After a day of circulating through the getter the tritium rate had fallen below levels confirming the effective removal of the tritiated methane with the getter. A second, larger injection of 800 mBq was performed a week later yielding a similar removal time constant. The second injection produced 20,000 beta decays in the LUX detector before being completely removed, 7000 of those decays were in the fiducial volume and could be used to calibrate the ER band in the WIMP search region of 1-50 Phe (about 1-8 keVee). The CH_3T (tritiated methane) was injected at the getter output and had passed through a special methane purifier to remove O_2 , H_2O and other electronegative impurities that could cause a degradation in electron lifetime. The injections were performed while circulating and with the getter actively purifying in order to maintain detector purity and stability. Prior to LUX detector upgrades in December of 2013 a total of 10 Bq of tritiated methane was injected into the LUX detector and successfully removed providing over 150,000 beta decays within the fiducial volume. The new tritium calibration source provided an unprecedented low energy electronic recoil calibration for the LUX dark matter search [PRL Ref].

1.2 Mixing of Tritiated Methane in Liquid Xenon

Tritium events appear uniformly distributed in the liquid volume several minutes after injecting the tritiated methane inline with the xenon gas circulation path. Figure 1 shows the XY and Z distribution of tritium events thirty minutes after an injection. The events shown cover the region from the gate to the cathode and radially out to the edge of the detector. An additional cut requiring that the event be between $\pm 3\sigma$ of the ER mean was made to disregard residual alpha events from the walls and cathode, the event rate consisted overwhelmingly of tritium events. The tritiated methane dispersed uniformly throughout the liquid xenon illuminating all regions on the detector.

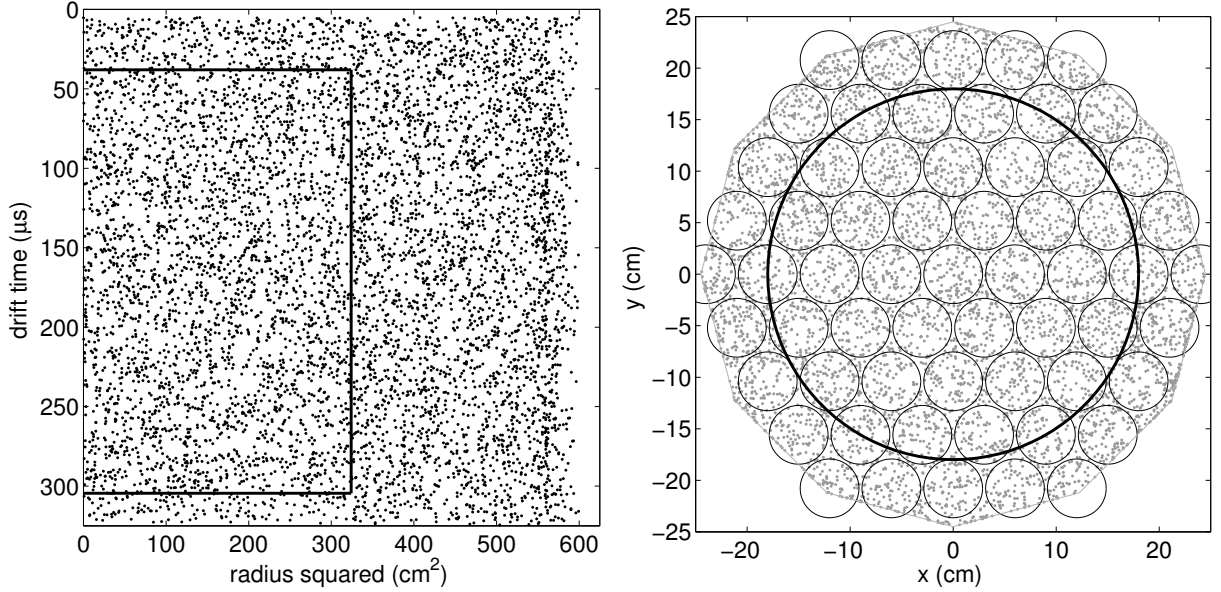


Figure 1: Left: The distribution of tritium events vs. detector radius squared. The solid black line represents the fiducial volume. Right: The distribution of tritium events vs. XY in the region between the gate and the cathode. The solid black line represents the fiducial volume and the black circles represent the locations of PMTs (photo multiplier tubes).

1.3 Definition of Electronic Recoil Band and Comparison with NEST Model

Using the tritium source we calibrated the electronic recoil band in the fiducial volume of the LUX detector to unprecedented accuracy. Figure 4 shows the mean of the ER band along with the 10-90% confidence bounds ($\pm 1.28\sigma$) obtained from the beta decay of tritium at a drift field of 180 V/cm. The results of the leakage fraction at 50% NR acceptance per each 1 Phe bins in S1 are shown in 5. The nuclear recoil band, in red, is defined by the NEST model along with AmBe and ^{252}Cf calibrations. Methane will not quench xenon scintillation [[9]] shows that if methane is introduced into the xenon at a relative concentration of a few percent, then the amount of scintillation produced by the mixture is reduced by a factor of two compared to pure xenon. But for our application we require a methane concentration of only one part in 10^{15} , and therefore our methane injection will not have any negative effects on scintillation production and transport.

WIMPs primarily interact with the atomic nuclei xenon atoms in LUX resulting in nuclear recoils whereas the vast majority of residual radioactivity within the detector are gammas which result in electronic recoils. Thus, knowing the separation of the ER from the NR band allows for a measure of the background rejection of a liquid xenon WIMP search experiment. We define the measure of background rejection as leakage fraction,

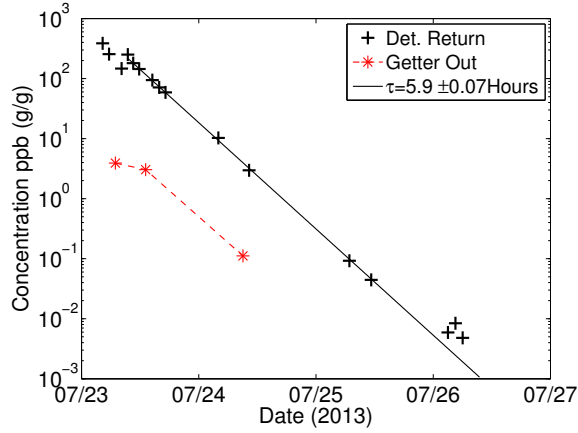


Figure 2: Removal of natural methane observed by the integrated xenon sampling system prior to the tritiated methane injections. The red points indicate xenon gas measurements at the getter outlet, we find a 97% one pass removal efficiency at a flow rate of 25 SLPM. $1 \cdot 10^{-3}$ ppb (g/g) is the limit of detection for methane using the LUX gas sampling system.

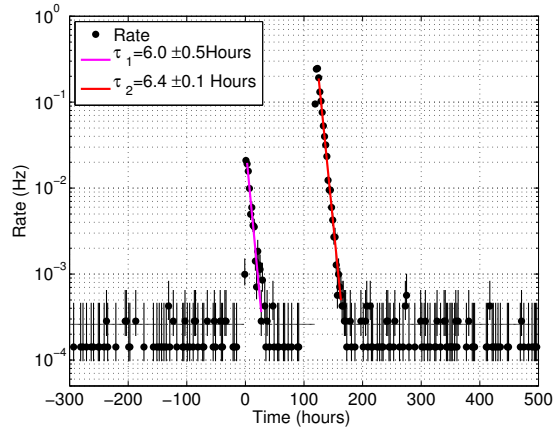


Figure 3: Left: Rate of single scatter events with S1 below 150 Phe in the fiducial volume. 150 Phe in S1 is about 18.6 keV_{ee}, the endpoint to the tritium beta spectrum. The magenta and red curves are fits to the first and second tritium injection's removal rate. Right: The rate of single scatter events with S1 below 150 for the whole detector volume. Note the removal of tritiated methane is consistent with the natural methane removal rate measured independently.

reported here as the fraction of events in the ER band that spill into the lower half of the NR band. Over 115,000 tritium decays were used for the ER band calibration, between 1-50 Phe in S1 (1-8 keV_{ee}), and were found using standard WIMP search cuts within the fiducial volume. A figure of merit for ER and NR discrimination is the leakage fraction defined as the number of tritium events populating the lower half of the NR band are compared to the total number of tritium events in the selected energy range. Figure 5 shows the leakage fraction per 1 Phe bins in S1. The mean leakage fraction in the region used for the LUX 2013 PRL results, between 1-30 Phe (1-5 keV_{ee}) in the fiducial, was found to be $0.42\% \pm 0.02\%$, see Figure 5. In the 40 hour time window in which the data was acquired less than three out of 115,000 events are expected

to be non tritium [BG paper reference]. The NR band used is from NEST version 0.98 and is vetted with AmBe, ^{252}Cf and DD neutron generator calibrations.

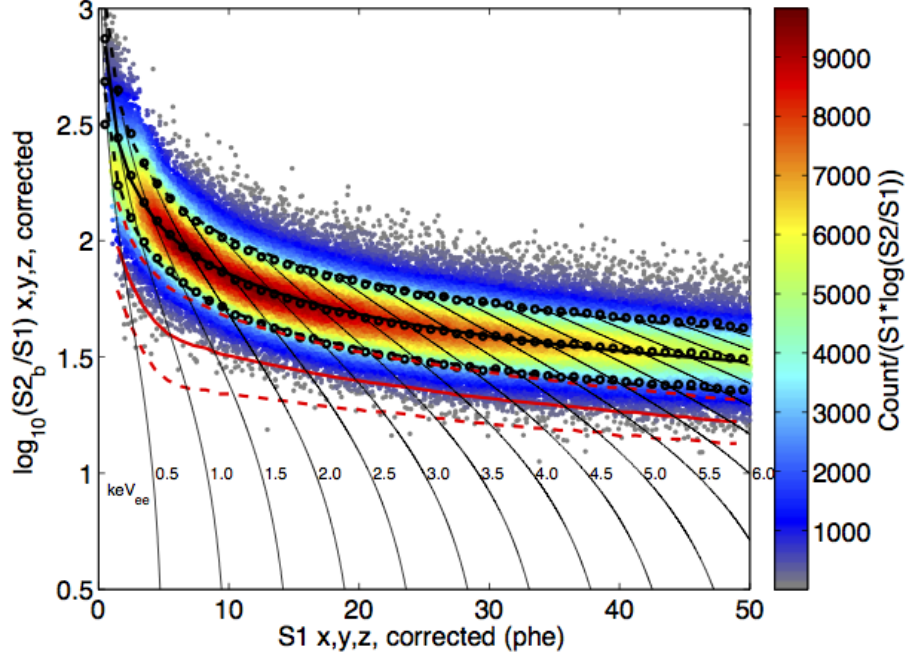


Figure 4: Discrimination vs. S1 using over 115,000 tritium beta decays between 1 and 50 Phe in S1 (about 1 – 8keV_{ee}). On average from 1 to 30 Phe the discrimination is 99.58%, defined by the fraction of events of events below the mean of the nuclear recoil band. The red band represents the NEST nuclear recoil band (version 0.98) vetted with an AmBe, ^{252}Cf and DD neutron generator calibration.

2 All the things we can do with Tritium

- Define the ER band.
- Binned leakage fraction, and potentially optimize for spacial dependent leakage fraction in XYZ plane.
- S1, S2 threshold. (Energy is a bit convoluted let's not go there). Requires NEST
- Combined energy calibration to about 0.5 keV_{ee}. Requires NEST
- Light Yield, Charge Yield. Requires some trivial smearing model, 10% effect.
- Fano-like factor vs. energy. Requires some trivial smearing model, sub 2% effect.
- Fiducial mass calculation, optimized for low energy S2s making it more WIMP like.
- g1 and g2 calculation by competing tritium spectrum with NEST, or multiple E fields
- ER band Gaussianity.
- ... anything else?

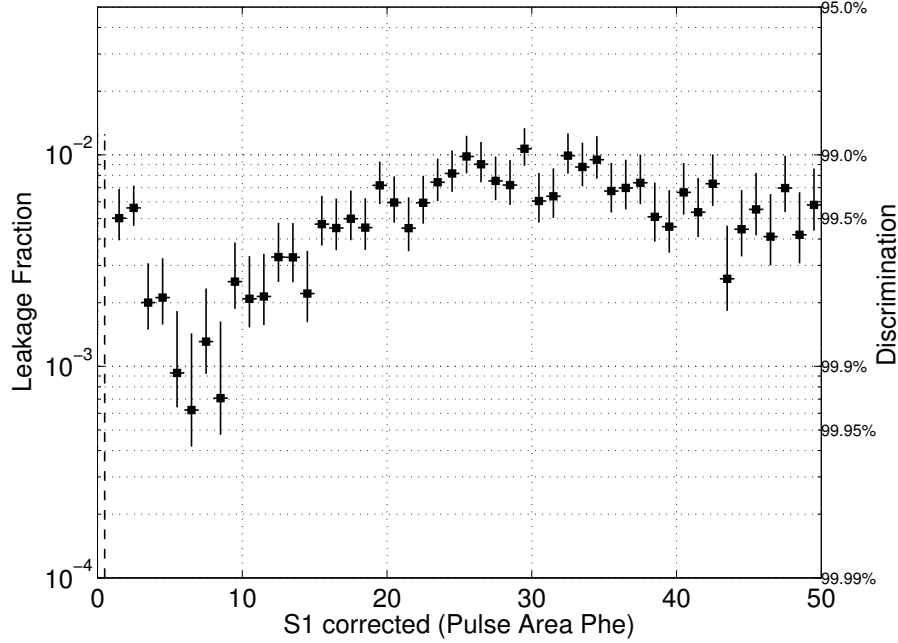


Figure 5: Discrimination vs. S1 using over 115,000 tritium beta decays between 1 and 50 Phe in S1 (about $1 - 8\text{keV}_{ee}$). On average from 1 to 30 Phe the discrimination is 99.58%, defined by the fraction of events of events below the mean of the nuclear recoil band. The red band represents the NEST nuclear recoil band (version 4c) vetted with an AmBe, ^{252}Cf and DD neutron generator calibration.

References

- [1] Sz. Nagy, T. Fritioff, M. Bjrkhage, I. Bergstrm, and R. Schuch. On the q -value of the tritium β -decay. *EPL (Europhysics Letters)*, 74(3):404, 2006.
- [2] D. P. Gregory and D. A. Landsman. Average decay energy of tritium. *Phys. Rev.*, 109:2091–2091, Mar 1958. doi:10.1103/PhysRev.109.2091.
- [3] P Venkataramaiah, K Gopala, A Basavaraju, S S Suryanarayana, and H Sanjeeviah. A simple relation for the fermi function. *Journal of Physics G: Nuclear Physics*, 11(3):359, 1985.
- [4] L. L. Lucas and M. P. Unterweger. Comprehensive review and critical evaluation of the half-life of tritium. *Journal of Research of NIST*, 105(4):541 – 551, 2000. ISSN 0883-2889. doi:http://dx.doi.org/10.6028/jres.105.043.
- [5] A. Dobi, et al. Study of a zirconium getter for purification of xenon gas. *Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment*, 620(23):594 – 598, 2010. ISSN 0168-9002. doi:http://dx.doi.org/10.1016/j.nima.2010.03.151.
- [6] D.S. Leonard, et al. A simple high-sensitivity technique for purity analysis of xenon gas. *Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment*, 621(1-3):678 – 684, 2010. ISSN 0168-9002. doi:DOI:10.1016/j.nima.2010.04.152.
- [7] Attila Dobi, et al. Detection of krypton in xenon for dark matter applications. *Nucl.Instrum.Meth.*, A665:1–6, 2011. doi:10.1016/j.nima.2011.11.043.

- [8] A. Dobi, et al. Xenon purity analysis for EXO-200 via mass spectrometry. *Nucl.Instrum.Meth.*, A675:40–46, 2012. doi:10.1016/j.nima.2012.01.066.
- [9] K. N. Pushkin, et al. Scintillation light, ionization yield and scintillation decay times in high pressure xenon and xenon methane. *Nuclear Science, IEEE Transactions on*, 54(3):744–750, June 2007. ISSN 0018-9499. doi:10.1109/TNS.2007.894815.