


Sample Name: MF744

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    5
Acq. Instrument : 6890 GC                     Location  : Vial  5
Injection Date  : 11/28/2016 7:13:50 PM      Inj       :    1
                                           Inj Volume: Manually
Sequence File   : C:\Chem32\1\DATA\Chelsea\MF742-781 2016-11-28 15-43-02\MF742-781.S
Method          : C:\CHEM32\1\DATA\CHELSEA\MF742-781 2016-11-28 15-43-02\HEADSPACE SAGEBRUSH_
                  2013.M (Sequence Method)
Last changed    : 11/28/2016 3:43:03 PM by SYSTEM
Method Info     : FID for Sagebrush samples using headspace sampler
=====

```

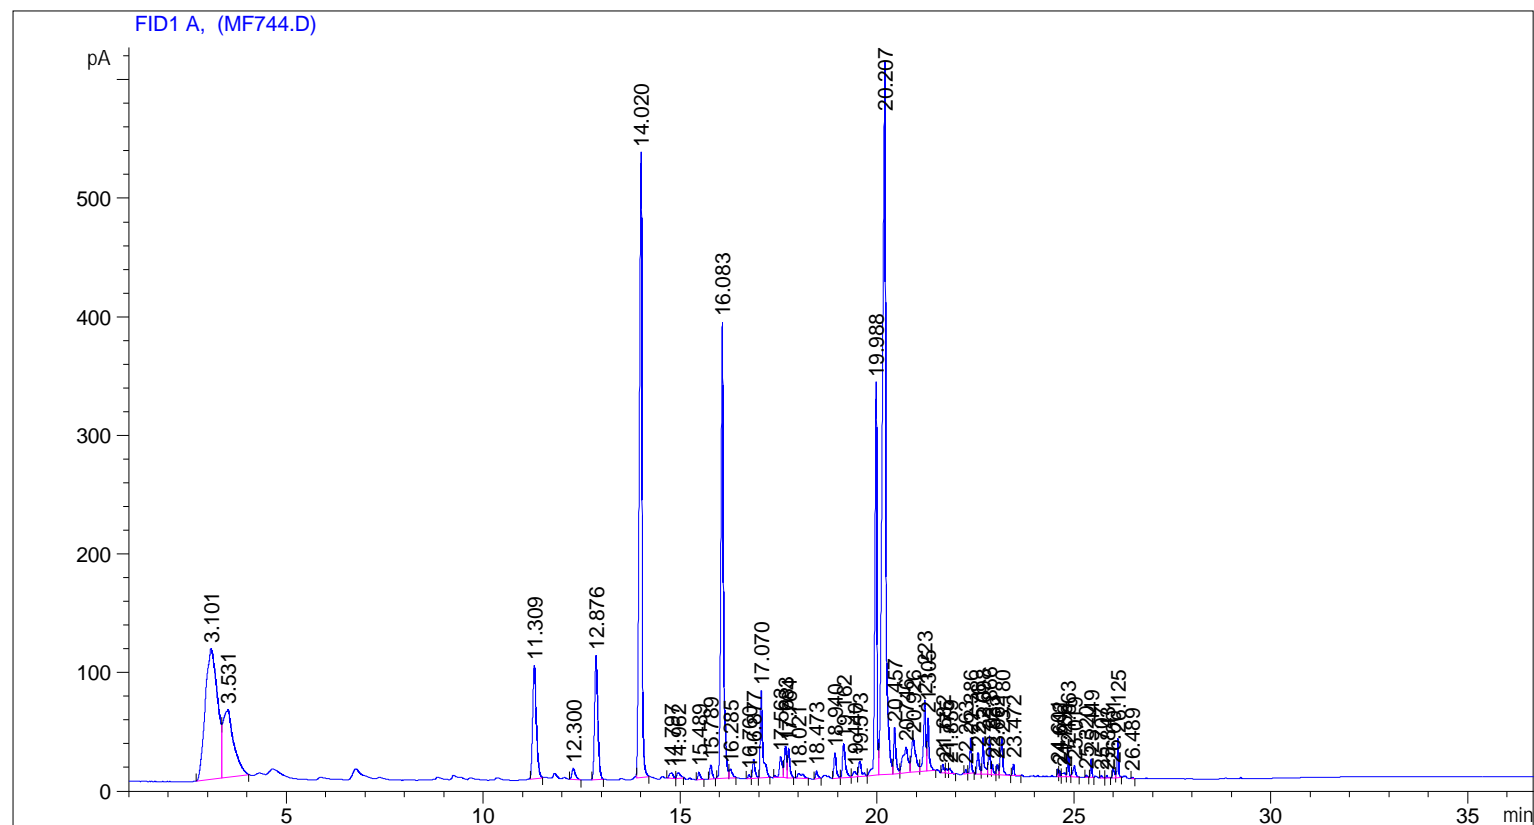

```

=====
                        Area Percent Report
=====

```

```

Sorted By           :      Signal
Calib. Data Modified :      Wednesday, May 18, 2011 10:54:12 AM
Multiplier          :      1.0000
Dilution            :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	3.101	BV	0.2762	2377.08057	14.04095	?
2	3.531	VB	0.2366	1104.51636	6.52416	?
3	11.309	BB	0.0901	615.69073	3.63676	?
4	12.300	BB	0.0903	56.99836	0.33668	?
5	12.876	BB	0.0854	593.87915	3.50793	?
6	14.020	BB	0.0705	2511.21509	14.83325	?

Sample Name: MF744

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
7	14.797	BV	0.0859	29.13912	0.17212	?
8	14.962	VB	0.0889	28.64383	0.16919	?
9	15.489	BB	0.0648	25.33917	0.14967	?
10	15.789	BB	0.0655	49.46070	0.29215	?
11	16.083	BV	0.0637	1738.22290	10.26734	?
12	16.285	VB	0.0807	43.27050	0.25559	?
13	16.760	BV	0.0573	11.34937	0.06704	?
14	16.877	VB	0.0609	65.25550	0.38545	?
15	17.070	BB	0.0659	331.42554	1.95767	?
16	17.563	BV	0.0759	92.20842	0.54466	?
17	17.683	VV	0.0586	102.27797	0.60414	?
18	17.764	VB	0.0588	100.38351	0.59295	?
19	18.021	BB	0.1232	36.33869	0.21465	?
20	18.473	BB	0.0571	23.34285	0.13788	?
21	18.940	BB	0.0623	87.49044	0.51679	?
22	19.162	BB	0.0738	144.96367	0.85627	?
23	19.440	BV	0.0897	25.36399	0.14982	?
24	19.573	VV	0.0790	68.19263	0.40280	?
25	19.988	VV	0.0553	1174.50916	6.93759	?
26	20.207	VV	0.0799	3599.88281	21.26380	?
27	20.457	VV	0.0601	160.69009	0.94916	?
28	20.746	VV	0.1207	197.61534	1.16727	?
29	20.926	VV	0.1090	218.75615	1.29215	?
30	21.223	VV	0.0594	244.41122	1.44369	?
31	21.305	VB	0.0495	154.43973	0.91224	?
32	21.682	BV	0.0492	25.64920	0.15150	?
33	21.775	VV	0.0545	14.26675	0.08427	?
34	21.859	VB	0.0567	17.00839	0.10047	?
35	22.263	BV	0.0428	9.61465	0.05679	?
36	22.386	VB	0.0403	79.39866	0.46899	?
37	22.576	BV	0.0609	72.69293	0.42938	?
38	22.698	VV	0.0459	96.56286	0.57038	?
39	22.866	VV	0.0426	96.24632	0.56851	?
40	22.933	VV	0.0435	26.74788	0.15799	?
41	23.062	VV	0.0434	25.97570	0.15343	?
42	23.180	VB	0.0596	131.65567	0.77766	?
43	23.472	BB	0.0321	17.68093	0.10444	?
44	24.601	BV	0.0286	11.93424	0.07049	?
45	24.642	VV	0.0285	9.64041	0.05694	?
46	24.766	VV	0.0816	21.30959	0.12587	?
47	24.863	VB	0.0350	52.87433	0.31232	?
48	25.019	BB	0.0694	45.12497	0.26654	?
49	25.320	BB	0.0371	4.90834	0.02899	?
50	25.449	BB	0.0343	35.07893	0.20720	?
51	25.707	BB	0.0502	8.34542	0.04929	?
52	25.843	BB	0.0428	7.42750	0.04387	?
53	26.001	BV	0.0446	27.67526	0.16347	?
54	26.125	VB	0.0353	76.85061	0.45394	?
55	26.489	BB	0.0304	2.61060	0.01542	?

Total s : 1.69296e4

Signal 2: FID1 B, not found

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	3.156		0.0000	0.00000	0.00000	
2	3.415		0.0000	0.00000	0.00000	Methacrolein
3	13.763		0.0000	0.00000	0.00000	alpha-Pinene
4	14.362		0.0000	0.00000	0.00000	Camphene
5	15.480		0.0000	0.00000	0.00000	beta-Pinene
6	16.958		0.0000	0.00000	0.00000	1,4-Cineole
7	17.306		0.0000	0.00000	0.00000	Cymene
8	17.587		0.0000	0.00000	0.00000	1,8-Cineole
9	21.577		0.0000	0.00000	0.00000	Camphor
10	22.670		0.0000	0.00000	0.00000	Terpineol
11	22.818		0.0000	0.00000	0.00000	

Totals : 0.00000

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

*** End of Report ***