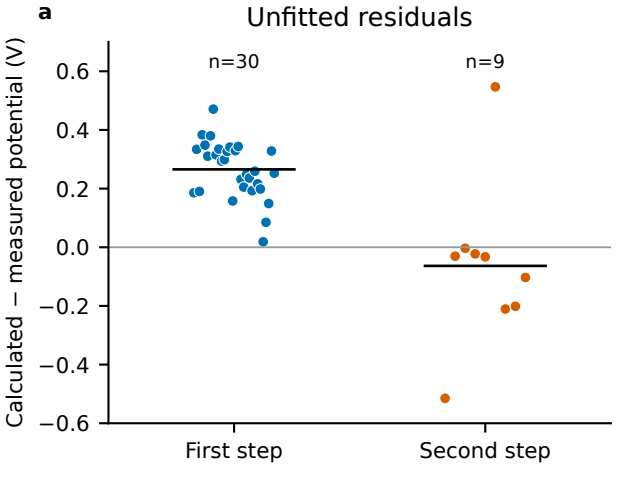
a
Unfitted residuals
n=30
n=9
Calculated − measured potential (V)
0.6
0.4
0.2
0.0
−0.2
−0.4
−0.6
First step
Second step

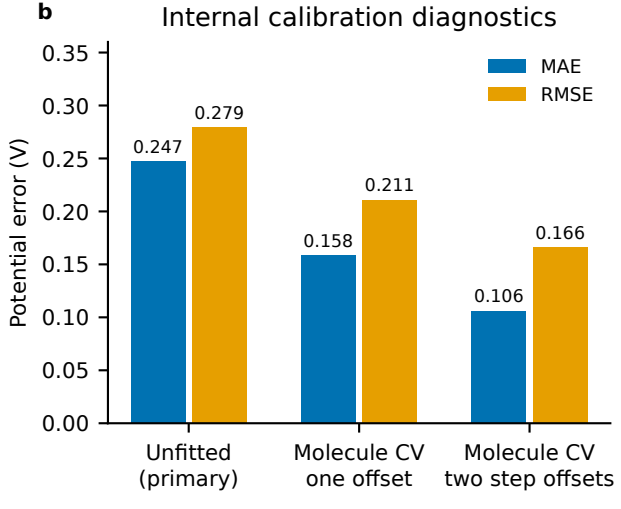
b
Internal calibration diagnostics
MAE
RMSE
Potential error (V)
0.35
0.30
0.25
0.20
0.15
0.10
0.05
0.00
0.247
0.279
0.158
0.211
0.106
0.166
Unfitted
(primary)
Molecule CV
one offset
Molecule CV
two step offsets