Both-input exact panel contrasts · EXP-impact-paired-001

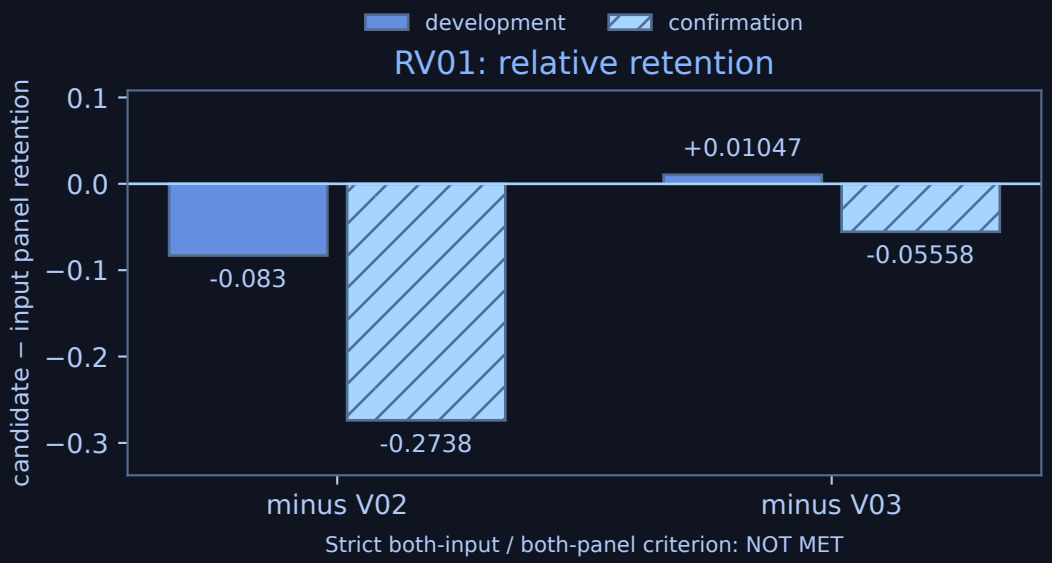

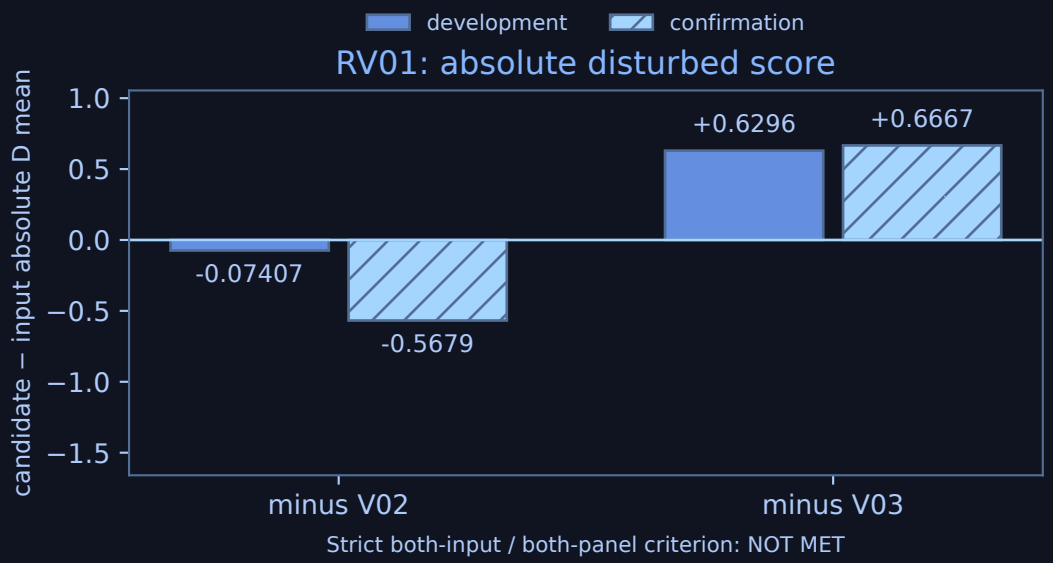

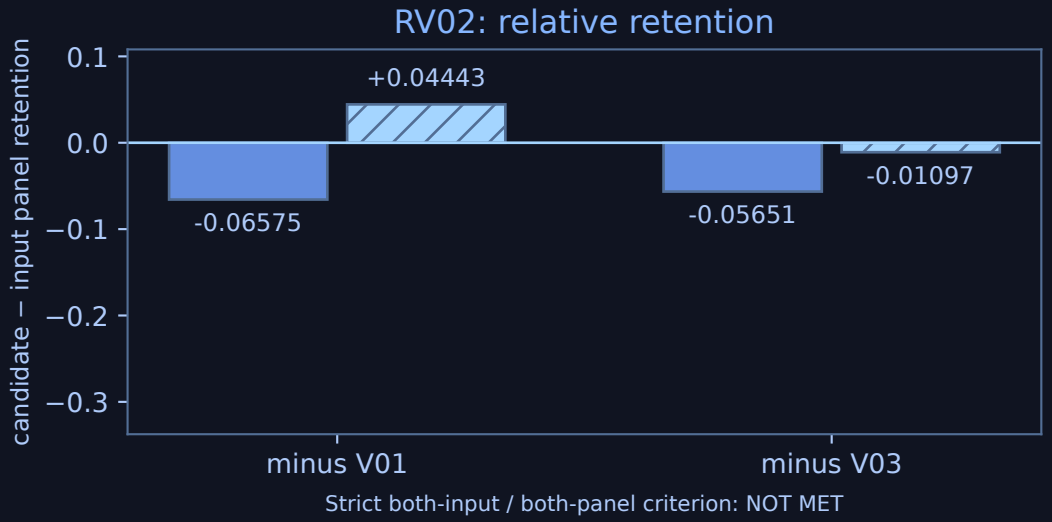

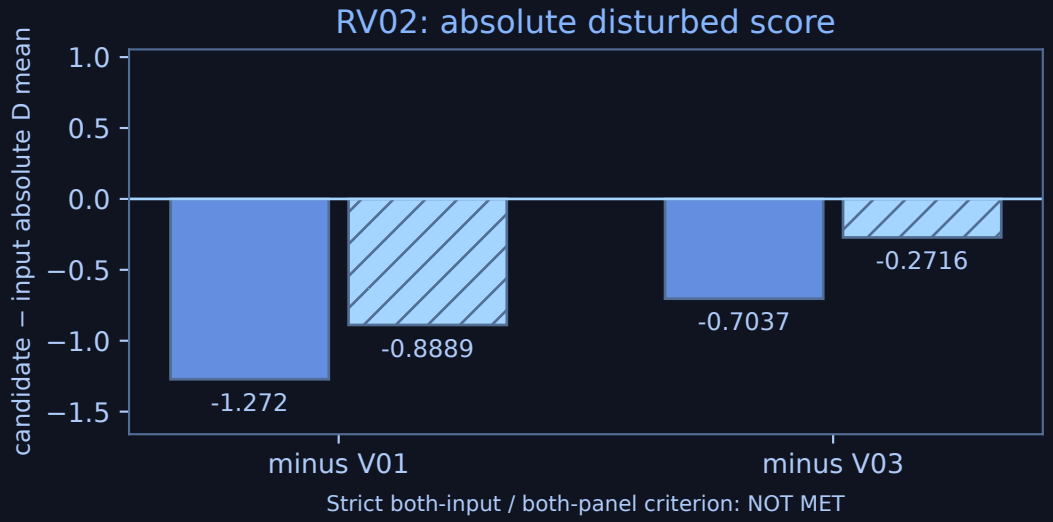

RV01: JOINT NOT MET; RV02: JOINT NOT MET. Calibration: PASSED.
Panel retention = arithmetic mean of two exact D/U fractions, not pooled D/U. Absolute D panel means use 162 samples.
Exact strict signs determine criteria; ties fail. Joint requires relative + absolute advantage and passed recovery/exposure/non-equivalence.
Conditional structural population performance, not evolvability. Genetic ancestry ambiguous; finite deterministic contrasts, no confidence intervals.