



Republic of the Philippines
Department of Health
National Capital Regional Office
VALENZUELA MEDICAL CENTER

Padrigal St., Karuhatan, Valenzuela City
Tel. No. 294-6711 to 16, Telefax 291-4259
Email address: valgen_hosp@yahoo.com



MINUTES OF THE PRE-BID CONFERENCE

11 January 2024

Public Bidding VMC No. 2023-041

Supply and Delivery of Various Medical Equipment – Batch 3

Present during the meeting were as follows:

BIDS & AWARDS COMMITTEE:

Ms. Ruby S. Gurrea - Chairperson
Engr. Zoraida S. Cuadra - Vice Chairperson
Mr. Rolando N. Saoi - BAC Member
Dr. Maria Concepcion Isberto - BAC Member
Dr. Edilberto V. Cavaneyro - Provisional Member
Mr. Eric Jose Pajarillo - Provisional Member
Ms. Mary Grace Santillan - Provisional Member
Dr. Joyce Ancheta-Bismonte - Provisional Member

BAC SECRETARIAT:

Ms. Ligaya Ubalde - Head - In-charge
Mr. Rannier John C. Fajardo
Ms. Angelita B. Dayego
Ms. Kristine Joy R. Manuel
Ms. Aileen C. Pacheco
Ms. Maiko Janzel M. Dizon
Mr. Lester John Jake R. Divino

TWG, END-USERS & OBSERVERS:

Dr. Rowena Helena Evangelista - TWG
Dr. Derrick Mendoza - TWG
Engr. Reynato Pascual - TWG
Dr. Cyril Joseph Corpuz - TWG
Ms. Melissa Austria - TWG
Ms. Avigail B. Ching - TWG
Mr. Percieval Mariano - End-user, OR
Mr. Mark Joshua Cruz - End-user, Pulmo
Ms. Shirlene V. Vianzon - Observer, CAO
Ms. Rufina Vadil - Observer, Budget Section
Mr. Raymund Joe B. Macuana - Observer, Accountant III

Ms. Almira Satumba - Observer, OIC-FMO II
Ms. Catherine F. Sofia - Observer, MMS
Mr. Billy T. Lucena - Observer, IMISS
Mr. Renato Acordo - Observer, IMISS
Engr. Gerardo E. Lingat - Engineer III
Mr. Joy Lariosa - EFMS, MET III
Mr. Dennis Santillan - EFMS, MET I
Mr. Roderick R. Balagtas - Observer, Proc.
Ms. Emelyn C. Sison - Support Staff

PROSPECTIVE BIDDER/S:

Ms. Jennifer A. Telen - United Medical Supply
Ms. Neshly H. Torino - Rainphil Inc.
Ms. Rose Sua rez - Patient Care Car Corp.
Ms. Chona Belo - Elan Vita Diagnostic Solutions
Ms. Zola Galicia - Quicklink Consumer Goods Trading
Mr. Jordan Catolico - One Top Medical Systems Resources
Mr. Gu Capon - RSM
Mr. John Alfie Sumulong - BHCI
Ms. Nikki Ramirez - Quicklink Trading
Mr. Reinhold Gonzales - Respicare Enterprises Inc.
Ms. Maicah Bayo - Healthrush Enterprises
Ms. Aya Jawod - Sunfu Solutions Inc.
Ms. Charmaine Mooasa - R&A
Ms. Jenny Rose Veluz - Rite-Tech Medical Inc.
Ms. Jessica Mamposte - RBGM Medical Express
Ms. Camila Urano - Grandline Medical Equipment Corp.

The conference started at 10:00am and was presided by **Ms. Ruby S. Gurrea**, Chairperson of Bids & Awards Committee (BAC), held at the BAC Office, 2nd Floor, Admin Building, Valenzuela Medical Center, Padrigal St., Karuhatan, Valenzuela City. She acknowledged the presence of all representatives of each prospective bidder, the members of the BAC, BAC Secretariat, TWG as well as the invited observers. She reminded everyone that the Committee strictly adheres to Republic Act No. 9184 or the Government Procurement Act and the Standard Public Bidding Documents.


BUSINESS MATTERS:

- In accomplishing the Technical Specifications and Schedule of Requirements, state only the item that will be bid.

- Bid Security will be forfeited if withdrawn during the validity period.
- Notice of Award will be faxed to winning bidders. The following day will be counted as 1st day of receipt.
- CTC of documents by the bidder itself are acceptable provided that the bidder will submit the Omnibus Sworn Statement. (Note: State CTC based on original, photocopy, etc.)
- Any document or certification issued outside Philippines should be accompanied by the official red ribbon (authentication) by the Philippine Consular Office/Embassy where the subject document or certification is issued.
- Modification of Bid is strictly prohibited. The description stated in the bid offer will be followed and cannot be amended

PRESENTATION OF BIDS:

- Bidders shall submit their bids through their duly authorized representatives using the forms specified in the Bidding Documents in two (2) separate sealed envelopes, which shall be submitted simultaneously.
- Bidders shall enclose the "Original" and "Copy 1" of their Eligibility and Technical Documents in a separate envelope marked ELIGIBILITY and TECHNICAL COMPONENTS. The "Original" and "Copy 1" of their Financial Documents (Bid Form, Bid Offer & others) shall be enclosed in a separate envelope marked FINANCIAL COMPONENTS.
- These 2 envelopes shall be enclosed in any sealed box (preferably Data File Box) with a cover.
- No color preference for the Folders and Boxes.
- All documents to be submitted as part of the Bid should be arranged in chronological order based in the Checklist provided by the BAC. Further, all bid proposals should be ring bound and tabulated in words. Failure to follow instructions will mean disqualification.

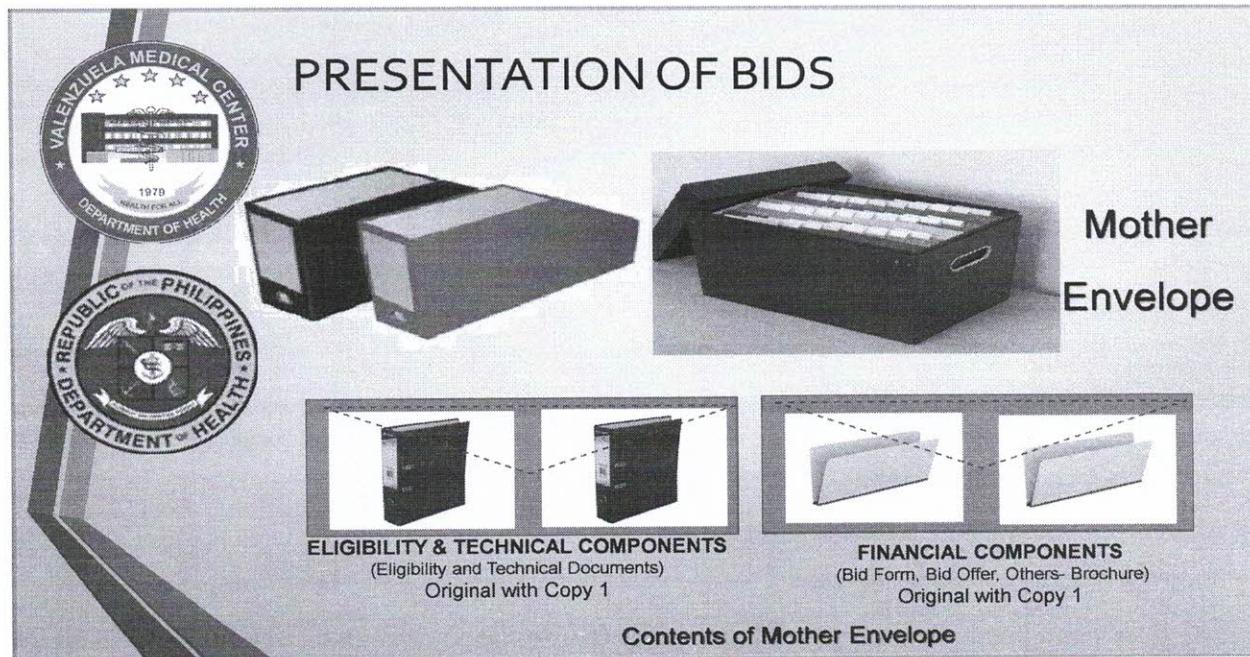

➤ **Documents Comprising the Bid: Eligibility and Technical Components – 1st Envelope**

(A) Eligibility Documents

Class "A" Documents:

(i)

- a. Valid PhilGEPS Registration Certificate (Platinum Membership) (all pages) in accordance with Section 8.5.2 of the IRR;

(ii)

- b. Statement of the prospective bidder of ALL its ongoing Government and Private Contracts including contracts awarded but not yet started, if any, whether similar or not similar in nature and complexity to the contract to be bid;
- c. Statement of the bidder's Single Largest Completed Contract (SLCC) similar to the contract to be bid, except under conditions provided for in Sections 23.4.1.3 and 23.4.2.4 of the 2016 revised IRR of RA No. 9184, within the last three (3) years as provided in the Bidding Documents;

- Amount of the completed contract should be fifty (50%) of the ABC to be bid

- d. Original copy of Bid Security. If in the form of a surety Bond, submit also a certification issued by the Insurance Commission or an Original copy of the Notarized Bid Securing Declaration
- e. Conformity with the Technical Specifications, which may include production/delivery schedule, manpower requirements, and/or after-sales/parts, if applicable; and
- f. Original duly signed Omnibus Sworn Statement (OSS);
Original Notarized Secretary's Certificate in case of a corporation, partnership, or cooperative; or Original Special Power of Attorney of all members of the joint venture giving full power and authority to its officer to sign the OSS and do acts to represent the Bidder.

Financial Documents

- g. The prospective bidder's computation of its Net Financial Contracting Capacity (NFCC); or A committed Line of Credit from a Universal or Commercial Bank in lieu of its NFCC computation.

Class "B" Documents

- h. If applicable, a duly signed joint venture agreement (JVA) in case the joint venture is already in existence or duly notarized statements from all the potential joint venture partners stating that they will enter into and abide by the provisions of the JVA in the instance that the bid is successful.

➤ **FINANCIAL COMPONENT ENVELOPE – 2nd Envelope**

The second envelope shall contain the financial information/documents as specified in the PBDs

- i. Original of duly signed and accomplished Financial Bid Form;
- j. Original of duly signed and accomplished Price Schedule(s).
- k. Original Brochure

Other documentary requirements under RA No. 9184 (as applicable)

- (l) [For foreign bidders claiming by reason of their country's extension of reciprocal rights to Filipinos] Certification from the relevant government office of their country stating that Filipinos are allowed to participate in government procurement activities for the same item or product.
- (m) Certification from the DTI if the Bidder claims preference as a Domestic Bidder or Domestic Entity.

ADDITIONAL REQUIRED DOCUMENTS (to be submitted during Post-Qualification)

1. Bidding Documents duly signed/initialed by the authorized representative of the prospective bidder (each page). Attach Official Receipt as proof of payment of bidding documents
2. Bid Bulletin/s, if any
3. Document Request List (DRL) - Optional
4. Registration certificate from the Securities and Exchange Commission (SEC), Department of Trade and Industry (DTI) for a sole proprietorship, or Cooperative Development Authority (CDA) for cooperatives or its equivalent document.
5. Mayors or Business permits issued by the city or municipality where the principal place of business of the prospective bidder is located, or the equivalent document for Exclusive Economic Zones or Areas. Please
6. Updated tax clearance per E.O. No. 398, s. 2005, as finally reviewed and approved by the Bureau of Internal Revenue (BIR).
7. The Supplier's audited financial statements, showing, among others, the Supplier's total and current assets and liabilities, stamped "received" by the BIR with 2022 ITR or its duly accredited and authorized institutions, for the preceding calendar year which should not be earlier than two (2) years from the date of bid submission
8. Certificate of **Good Performance** from at least two (2) Government or Private Hospital/Agency similar to the contract to be bid (CY 2022 to present)
9. Special Power of Attorney – If a single proprietorship
10. For SLCC - Proof of evidence for Single Largest Completed Contract (SLCC) – Purchase Order or Notice of Award or Contract Agreement.
11. Notarized Certificate of Stocks Availability.

12. Certificate from the manufacturer to distribute their products or Exclusive Distributorship or any equivalent documents.
13. License to Operate (LTO)

REVIEW OF TECHNICAL SPECIFICATIONS:

ITEM NO.	QTY	UOM	SPECIFICATIONS	ABC	TOTAL ABC		
			<u>EMERGENCY DEPARTMENT</u>				
1	2	unit	3-CHANNEL ECG MACHINE	106,666.67	213,333.34		
			-Proposed location: Emergency Department (Clean & Tent)				
			- Voltage input: 100 to 240 VAC ±10%				
			- Built-in rechargeable lithium battery for 2hrs continuous work				
			- One (1) year on parts and service of machine, one (1) year preventive maintenance service included				
			2 extra patient cable				
			Specifications:				
			- Compact and Portable Design				
			- 5-inch diagonal, 15:16:9 Aspect Ratio, TFT LCD with LED Graphics Backlit				
			- Weight: 1.1-1.2kgs (without AC adapter, battery and recording paper)				
			- Peripheral Ports: USB, LAN port				
			- 6 Hours of Continuous Operation without Recording				
			- 5, 12.5, 25, 50mm/s Recording Speed				
			- Records and Prints 12-Lead Resting ECG with 10-second Duration				
			- Complete digital filters and self-adapting filtering				
			- Up to 300 seconds of rhythm analysis for easier in arrhythmia locating or its equivalent				
			- "One-touch" functional shortcut keys				
			- Onscreen operation guide to check the ECG procedure				
			- Multi language voice reminder and visual alarming for lead-off, low battery and no paper				
			- Support general settings according to different situations for physicians and patients				
			- 3 report formats: simple report, median beat report and manual report				
			- Massive local storage capacity up to 1500 files or with copying/saving data thru flash drive				
			OTHER REQUIREMENTS:				
			Report and Certificates.				
			- With Certificate of availability of spare parts within five (5) years				
			- With Certification of Calibration and Quarterly Preventive Maintenance				
			- With uptime and downtime certificate (95%-98%)				
			DELIVERY SCHEDULE: 90 calendar days				

<u>LABORATORY DEPARTMENT</u>					
2	1	unit	INCUBATOR (FOR MICROBIOLOGY)	200,000.00	200,000.00
			Specification:		
			*Interior Chamber Volume: at least 5.9 cu. ft / 166 L		
			*Interior Dimensions (w x d x h): at least 19.5 x 20.0 x 26.0 in /495 x 508 x 660 mm		
			*Exterior Dimensions (w x d x h): at least 25.3 x 27.3 x 38.0 in 643 x 693 x 965 mm		
			*Temperature Range: Ambient + 8°C to 70°C		
			*Temperature Stability:(+/-) 0.05°C - 0.1°C @ 37°C		
			*Temperature Uniformity:(+/-) 0.5°C - 1°C @ 37°C		
			*Amperage: at least 6.0 Amps / 4.0 Amps		
			*Shelves: at least 3 Standard, 12 Total		
			*Touch Screen Controller Features: Large, easy-to-read display screen • Data export via USB • Stores up to 5 years of log data • Password locking capabilities • Data logged once per minute • Export in .CSV file • Smart alarm: accounts for door openings and temperature set point changes before alarm • Temperature deviation alarm * with UPS/AVR or equivalent functions		
			• with 5 years preventive maintenance quotation of labor and services after warranty period		
			OTHER REQUIREMENTS: - With Certificate of availability of spare parts within five (5) years - With Certification of Calibration and Quarterly Preventive Maintenance - With uptime and downtime certificate (95%-98%)		
			*with 3 years warranty on parts and services		
			*Training for operation, maintenance and repair for medical equipment technician of VMC.		
			DELIVERY SCHEDULE: 90 calendar days		
3	1	unit	TRANSPORT BOX WITH DATA LOGGER	250,000.00	250,000.00
			Specification :		
			Cooling :Passive		
			Gross volume: 44 Liters		
			*Storage capacity, blood bags /approx. 26 Blood Bags (450ml)		
			*External dimensions (H x W x D)at least 499 x 710 x 550 mm		
			* Inner dimensions (H x W x D): at least 264 x 496 x 334 mm		
			*Dimensions of interior container (H x W x D): at least 192 x 390 x 237 mm		
			Net weight (empty): at least 17 kg		
			Gross weight (fully stocked) : at least 40 kg		
			Outer material / interior material: Polyethylene		
			Material of Interior container :Stainless steel		

		Insulation: Polyurethane		
		Insulation Thickness: 90-105 mm		
		Accessories (standard): 24 cooling elements at 0.6 l each 1 stainless steel interior container (with Lid) Securing frame for interior container		
		Cold Life at +32°C: up to 109.08 h		
		*with Temperature data logger		
		<ul style="list-style-type: none"> • For continuous, tamper-proof temperature recording • New, easy to read LCD display with 30 days summary • Interchangeable external probe with high quality gold plated connector and built-in audible alarm • Temperature range -40°C to +99°C (measurement range from an external probe) • Standard battery (3V CR2032) replaceable by user 		
		• with 3 years warranty on parts and services		
		• with 5 years preventive maintenance quotation of labor and services		
		• with training on operation, maintenance and repair for Medical Equipment Technician and end-user.		
		with UPS and AVR		
		OTHER REQUIREMENTS:		
		- With Certificate of availability of spare parts within five (5) years		
		- With Certification of Calibration and Quarterly Preventive Maintenance		
		- With uptime and downtime certificate (95%-98%)		
		DELIVERY SCHEDULE: 90 calendar days		
4	2	unit	ELECTROSURGICAL UNIT	999,263.50
		Accessories:		
		-1 unit cart/table with brakes		
		-1 unit Monopolar footswitch with cable		
		-1 pc disposable hand control pencil		
		-1 pc reusable grounding pad/plate		
		-1 set bipolar footswitch, cable & forceps		
		-2 pc bipolar cable and forceps		
		-1 pc adapter		
		TECHNICAL SPECIFICATIONS:		
		-With isolated output electrosurgical energy system		
		-With at least 15.7 cm LCD touchscreen or LED numerical display		
		-Should be sturdy and can be placed on the table top		
		-must have the following settings: cut, coag, bipolar and shared coag or its equivalent		
		-Monopolar cutting modes: pure cut, blended cut or its equivalent		
		-Monopolar coagulation modes: spray, standard and pinpoint		

		-Bipolar modes: micro and macro, with 90 watts maximum power output		
		-bipolar output meter with alarm or audible feedback to surgeon during procedure		
		-Must have at least two (2) monopolar		
		-General mode for general procedures		
		-Laparoscopic mode and fluid mode		
		-Must have technology that insulates the system from interference from the other electrical equipment		
		-must be capable of two (2) simultaneous monopolar coagulation (one hand control and 1 foot control)		
		- Must be supplied with foot pedals: 1 for monopolar (cut and coag) and 1 for independent bipolar only use. Splash proof and with low voltage, and medical grade design		
		Integrated interface for activation of smoke evacuators and other devices		
		-Auto voltage ranged from 100 volts to 240 volts at 50/60 Hz.		
		-Radio frequency (RF) isolated and independent outputs		
		ADDITIONAL REQUIREMENTS:		
		- Voltage preferably: 100 to 250V, 60Hz or auto volt		
		DELIVERY SCHEDULE: 90 calendar days		
5	2	unit	PORTABLE TRANSPORT MECHANICAL VENTILATOR	1,167,000.00
		>portable ventilator can be used in hospital, aeromedical (optional) and ground transport		
		>Able to ventilate adult and pediatric patients (at least 0.5kgs of body weight)		
		>Modes of ventilation		
		a. Basic modes of ventilation		
		> With High and Low Alarm limits		
		> Approximately weight <10lbs(4.5 kgs for easy transport)		
		>Altitude compensation from (-1000ft to 30,000ft)		
		>Operating temperature range for external conditions (-10C + 50C)		
		>Pneumatically driven		
		>Spare consumables filter, vent valve, battery		
		>Warranty period for 3 years		
		> User and technical manual (2 copies)		
		>Availability of spare parts 10 years from the date of purchase		
		>Certificate of availability of spare parts from manufacturer		
		>Authorized distributorship from manufacturer		
		>Quarterly Preventive maintenance and calibration during warranty period		
		>With uptime 95-98% and downtime 2-5%		

			>Inclusion of training for End Users and Biomed		
			>Provision for loaner unit when equipment is under repair during warranty period		
			INSTALLATIONS: 5 LOCAL INSTALLATIONS OF THE SAME BRAND and/or MODEL from GOVERNMENT AND/OR PRIVATE HOSPITALS		
			Certificate of Good Performance from at least three (3) Government or Private Hospital/Agency similar to the contract to be bid (CY 2022 to present)		
			DELIVERY SCHEDULE: 90 calendar days		
6	2	unit	INFANT INCUBATOR	2,123,333.00	4,246,666.00
			Specifications:		
			- Dual LCD screen, with 7-12.1-inch colored LCD color touch screen and 5.6-inch LCD color screen can be achieved by simple click		
			Three control modes: -air mode -baby mode -family care mode servo control or equivalent (optional)		
			- Trend display		
			- Dovetail shape guiderail to install small medical devices		
			- Electronic bassinet tilting mechanism, adjust the angle more gently		
			- >37 degrees Celsius temperature set function		
			- The height of whole unit can be adjusted		
			-Double wall hood, automatic air curtain to reduce heat loss and keep the air temperature constant		
			- Independent over-temperature protection system, multiple failure alarm indications to provide multiple safety protection		
			- RS-232 connector to support data transmission		
			- Low noise DC motor		
			- Newborn special monitoring module: VITAL SIGNS: HR and O2 SAT		
			- Preferably Masimo Blood oxygen technology and/or Melcor technology to effectively eliminate motion disturbance and improve the measurement performance of weak perfusion		
			- Air temperature control range: 20-37 degrees Celsius (override mode 37.1-39 degrees Celsius		
			- Baby temperature control range: 20-37 degrees Celsius (override mode 37.1-39 degrees Celsius		
			- Temperature sensor display range: 17-50 degrees Celsius		
			- Warm-up time: at least 40 minutes		
			- The temperature fluctuation range between incubator temperature and average incubator temperature (under stable temperature condition): </=0.5 degrees Celsius		
			- Difference between the average air temperature and the control temperature:</+1.0 degrees		

		Celsius		
		-Temperature overshoot in Air control mode:</=1.0 degrees Celsius		
		-Temperature uniformity:</=0.8 degrees Celsius (matress horizontally placed)		
		- Accuracy of skin temperature sensor: +-0.2 – 0.3 degrees Celsius		
		- Electronic Inclination of the bassinet: no less than +-12 degrees Celsius		
		- Precision of tilt Angle display for crib equipped with electric and/or mechanical adjustment		
		- Mattress size: at least 630mm x 340mm x 30mm		
		- Accuracy of humidity display and control:+- 5%RH		
		-Control range of oxygen concentration: 20%~65%O2		
		-Accuracy of oxygen display		
		concentration:		
		+2%O2 (oxygen concentration sets <25%)		
		+3%O2 (oxygen concentration sets >25%)		
		- Weighing Range: 100~999g		
		Standard Configuration		
		- Main unit (including infant compartment, machine case, controller, I.V. pole and tray), sensor box, humidity control system, VHA stand oxygen concentration control system, skin temperature sensor.		
		- Weighing system, Observation Lamp (optional), SpO2, Camera, Panel Damping System and Hands-free Alarm Silence		
		- Power requirement: AC220-240V, 50/60HZ, 1300VA		
		OTHER REQUIREMENTS:		
		- With Certificate of Calibration		
		- With Certificate of availability of spare parts within five (5) years		
		- With Quarterly Preventive Maintenance		
		- With uptime and downtime certificate (95%-98%)		
		WARRANTY: 3 YEARS ON PARTS AND SERVICES		
		DELIVERY SCHEDULE: 60CD		
		EMERGENCY ROOM		
		3-CHANNEL ECG MACHINE		
		-Proposed location: Emergency Department (Clean & Tent)		
		- Voltage input: 100 to 240 VAC ±10%		
		- Built-in rechargeable lithium battery for 2hrs continuous work		
		- One (1) year on parts and service of machine, one (1) year preventive maintenance service included		
		2 extra patient cable		

		Specifications:		
		- Compact and Portable Design		
		- 5-inch diagonal, 16:9 Aspect Ratio, TFT LCD with LED Graphics Backlit		
		- Weight: 1.1kg (without AC adapter, battery and recording paper)		
		- Peripheral Ports: USB, LAN port		
		- 6 Hours of Continuous Operation without Recording		
		- 5, 12.5, 25, 50mm/s Recording Speed		
		- Records and Prints 12-Lead Resting ECG with 10-second Duration		
		- Complete digital filters and self-adapting filtering		
		- Up to 300 seconds of rhythm analysis for easier in arrhythmia locating		
		- "One-touch" functional shortcut keys		
		- Onscreen operation guide to check the ECG procedure		
		- Multi language voice reminder and visual alarming for lead-off, low battery and no paper		
		- Support general settings according to different situations for physicians and patients		
		- 3 report formats: simple report, median beat report and manual report		
		- Massive local storage capacity up to 1500 files		
		OTHER REQUIREMENTS:		
		Report and Certificates.		
		- With Certificate of availability of spare parts within five (5) years		
		- With Certification of Calibration and Quarterly Preventive Maintenance		
		- With uptime and downtime certificate (95%-98%)		
		DELIVERY SCHEDULE: 90 calendar days		
7	1	unit	STATIONARY CEILING MOUNTED DIGITAL X-RAY MACHINE	23,666,666.00
		A ceiling mounted general radiography system that is design to perform various radiologic exposures of the whole body with flexibility and agility.		
		Flexible operation with a floating tabletop with electromagnetic lock and a 3D hanging track rotates freely in any direction, convenient for all clinical application.		
		The system shall use 17x17 and 14x17 WIFI detector are available in the cassette, it could optimize the diagnosis accuracy by the excellent image quality with fast acquiring speed and unlock the value of existed general x-ray system, by working with other x-ray system.		
		Automatic Image Viewing Field Tracking System, which allows ceiling tube to move synchronized with wall detector movement. Outstanding electric machine works little noise and stable		

		performance.		
		The system shall have a wide range of image processing and enhancing functions for better image quality.		
		A central console with integrated xray generation techniques and parameters setting, image acquisition settings and processing and RIS-PACS data handling workflow.		
		The system shall have RIS-PACS interfacing and connectivity capability.		
		The voltage and current can be set at the computer unit, console set and X-ray tube receiver set for convenience		
		STATIC WIFI FLAT PANEL DETECTOR		
		Quantity: 2 pieces (17x17) and 2 pcs (14x17) with 2 batteries and 1 extra battery		
		Detector technology: Wireless detector with Cesium iodide (CsI)scintillator coupled to TFT matrix with amorphous silicon technology		
		Image Size: 35x43 cm (14x17 inch) and 43x43cm (17x17 inch)		
		Pixel Matrix: minimum 2350x3072		
		Pixel Pitch 100 – 150 µm		
		A/D Conversion: 16 bits		
		DQE: 2µGy at 0 lp/mm 65%		
		Spatial Resolution: 3.3 - 3.6 LP/mm		
		Image Acquisition Time: maximum 2s		
		Image Processing Time: maximum 3s		
		Recommended cycle time: maximum 10s		
		X-ray Voltage Range: 40-150 KV		
		Data Interface: GigE /802.11ac		
		Power Dissipation: 20 W Adapter Input: AC 100-240V,50-60Hz		
		Adapter Output: DC 24V, 60W		
		Dimensions: 38x46x1.5 cm		
		Max. load capacity 100 to 150kg with patient lying on it; 10 to 150 kg with patient standing		
		Battery: Lithium ion, build in, rechargeable, at least 3200mAh 2 pieces		
		Charging time: 180 to 240 minutes for 100 % battery capacity		
		Battery Standby Time: 6 to 10 hours		
		Housing Material: Carbon, Alloy or its equivalent		
		Water Tightness: IPX3		
		Operating Environment: 5-35 °C/10-75%		
		DXRAY DIAGNOSTIC WORKSTATION		
		CPU: i7 12th gen or latest version		
		Image Capture Memory: 16GB, Hard Drive: 1 TB SSD		
		Monitor: 24inch, Resolution: 1920*1080 pixels,		

		medical grade		
		CD/DVD recording/burning Case management		
		Case management function: including the management of patient information, exam information and images.		
		Worklist enquiry service following standard DICOM3.0 may inquiry from HIS/PACS and download case information. Image acquisition		
		Acquisition system: positive and negative film image capture can be configured		
		Real time automatic window width level adjustment		
		Real time ROI (region of interests) clipping		
		Real time enhancement		
		Selecting image and rotation according to different body postures;		
		Displaying patient information, examination information, device information and image information Image processing		
		Adjustment of window width, window level, Gamma, and LUT curve.		
		Positive and negative film switchover, image zoom, translation, mirror image, rotation, magnified display; Image enhancement, noise reduction: Scheme and level of image enhancement and noise reduction can be adjusted according to different body postures.		
		Image labeling function: including drawing straight line, rectangle, polygon, arrow and text;		
		Real time reminding the free space of image disk of the system.		
		RT prompt system can be used for store size of the disk space of image. Image output		
		Sending SCU with DICOM: support sending image to any PACS and workstations following Standard DICOM3.0		
		Receiving SCP server with DICOM: support receiving image following Standard DICOM3.0 from any workstation.		
		Image Stitching. It is of great clinical significance for orthopedic department to obtain important diagnostic basis before clinical operation and provide accurate reference for postoperative evaluation.		
		Advanced Feature:		
		1. Emergency mode: it can supply emergency exposure without registration		
		2. Check-up mode: it can import and register patient information by excel		
		3. Reject analysis: Image cancel / delete image / Statistic of use		
		HIGH FREQUENCY GENERATOR (80KW)		
		Nominal supply voltage(50/60Hz): 3-phase AC:380/400/415		
		Nominal Electric Power: 80KW (130KV,500ma,0.1s)		

		Short time rating: 150kV@500mA,130kV@500mA,80kV@1000mA		
		Voltage: 40 to 150kv, 1kv step		
		Tube Current Range: 10 to 1000ma		
		mAs: 0.1 to 1000mAs		
		Time range: 1ms-10000ms		
		X-RAY TUBE		
		Target Material: Lawrencium-tungsten Molybdenum Target angle:12°		
		Focal Spot Sizes: 0.6 / 1.2 mm		
		Permanent filtration: 1- 2.5mmAl/75kw		
		Max Output Voltage: 150KV		
		Power: 20KW/50KW		
		Anode heat storage: 210kJ to 300 kJ / 300KHU to 350KHU		
		Max. heat content of Assembly: 900 kJ to 1000 kj (1250 KHU to 1350 KHU)		
		Max. anode heat dissipation rate: 750W (1050 HU/s)		
		Anode rotation: 2800 min. -1 at 50Hz		
		Touch screen display: at least 10 inch wide which displays console software and rotation angle.		
		COLLIMATOR		
		Max. operating voltage of X-ray tube: 150kV		
		Irradiation field (SID=100cm): 430mm×430mm		
		Power supply: 24VAC 6A Average illumination (at SID=100cm): 160 lx or more		
		Illumination duration: Continuously for 30seconds (automatically turn off)		
		Light source time limit: 30s±5s		
		Attached filter (70kV): 0.5 /1.0/1.5mm Al (switch inside) Distance from focal spot to installation surface: 60m		
		3D CEILING SUSPENSION SYSTEM		
		Ceiling Suspended System		
		Move the wall detector and automatic tracking for tube side.		
		X-ray tube support horizontal travel range Longitudinal: 2600mm, manual with EM lock		
		X-ray tube support transverse travel range with tube trolley: 1800mm, manual with EM lock		
		X-ray tube support vertical travel range 1500mm, manual with EM lock and motorized with speed in the z-axis Up to max. 60mm/s		
		Mini distance between tube focus to the ceiling: 1225mm Tube Rotation angle around vertical axis: ±180°, manual		
		Tube Rotation angle around horizontal axis: ±90°, manual		
		Ceiling Rails Dimension: 3200x610x100(upper);3200x1554x100mm(lower)		
		Ceiling Rails Weight: 65kg Ceiling Tube support Dimension: 1000x650x1250mm		

		Ceiling Tube support Weight: 200kg		
		Vertical Detector Stand (LZ-1)		
		Vertical Moving Range: 1400mm (353-1753 floor to focus), manual with EM lock		
		Available for movable grid		
		Wall Bucky Dimension:615.5x370x2240mm		
		Wall Bucky Weight:120kg		
		Floating Diagnosis Table (6 Way)		
		Table size: 2100x800x500mm		
		Table load for the patient: 250 to 300 KG		
		Tabletop floating range: ±500mm*±130mm		
		Cassette longitudinal movement under table: ±250mm		
		Tabletop vertical movement range: 500-850mm, motorized.		
		Grid Ratio: 10:1		
		Grid Focus: 1000mm		
		INCLUSIONS:		
		Wireless Detector Flat Panels		
		a. 17x17 and 14x17, 4 pieces with 2 rechargeable batteries and 1 extra		
		DIGITAL PRINTER		
		Desktop for Image Suite PC with UPS and AVR (1 Unit)		
		Radiologist work station (1 PC Desktop with Medical Grade 32-inch Monitor and UPS and AVR)		
		1 set Lead Gown and Thyroid shield		
		Infrastructure: (Electrical and Civil Works)		
		Full renovation of the existing xray room		
		a. FDA required radiation protection shielding		
		b. Control room with lead glass		
		c. Two (2) comfort rooms (1 for patient / 1 for staff)		
		d. Cabinets		
		e. Electrical Lightings and outlets		
		Installation of new air-conditioned units		
		a. 2 units 3-tonne for main xray room		
		b. 1 unit 2.5-HP for control room		
		Transient Voltage Surge Suppressor (TVSS) Installation		
		Warranty:		
		5 years warranty of parts and service. Not covered in the warranty are the materials and items subject to wear and tear, damages resulting from accidents, misuse and abuse, failure to follow operating instructions and unauthorized alterations,		
		Warranty certificate includes: Availability of spare parts within 10 years. With uptime and down time certificate (95-98%)		
		Delivery Period: 90 calendar days only upon the receipt of Purchase Order and / or Notice to		

		Proceed		
		Deliver, Installation, Calibration and Training shall be free of charge. Training, familiarization and proper usage of the machine should be done for at least 7 working days by the vendor.		
		Availability of Field Service Engineers should be 24/7 to address all the product related concerns.		
		Provision of Preventive Maintenance Service (Quarterly) during warranty period. Calibration of Equipment with certificate during warranty. Operation Manual (end User and METS copy)		
		OTHER REQUIREMENTS:		
		-With uptime and downtime certificate (95%-98%)		
		- Manufacturing date: 2022 onwards		
		DELIVERY SCHEDULE: 90 calendar days		
			TOTAL:	32,909,192.34

Other Concerns:

- Schedule of Requirements: Items to be bid only.
- Post-Qualification Evaluation: Technical Working Group (TWG) may ask for additional documents from supplier for validation.
- Minutes of the Pre-Bid and Bid Bulletin will be posted in the Philgeps and VMC Website (<https://vmc.doh.gov.ph/>)
- **ALL UNITS** will be subject for evaluation.
- All documents to be submitted as part of the Bid should be arranged in chronological order based in the Checklist provided by the BAC. Further, all bid proposals should be ring bound and tabulated in words. Failure to follow instructions will mean disqualification.

A. Template in the Goods Offered in the Philippines and/or Abroad

- Column 1 – Should be in accordance with VMC's item number.
- Column 2 - Indicate the **item description of your offer** with BRAND. If no BRAND indicates **GENERIC OR NO BRAND**.
- **Column 3** – Country of Origin
- The Price Schedule should be filled completely or put zero if not applicable.
- The final unit price should be stated.
- In the Price Schedule, "*For Goods Offered from Abroad Form*" will be used **if the origin of the item** is from abroad, if manufactured in the Philippines, "*For Goods Offered from Within the Philippines Form*" shall be used. (Please use the attached Form/Template)

B. BID Opening will be on January 23, 2024, at 10:00 AM

The pre-bidding conference was adjourned at 2:00 pm.

Prepared by:


LIGAYA E. UBALDE, MPA
BAC Secretariat

Noted by:


RUBY S. GURREA, RN, MAN
Chairperson, BAC

Bid Form for the Procurement of Goods
[shall be submitted with the Bid]

BID FORM

Date : _____

Project Identification No. : _____

To: [name and address of Procuring Entity]

Having examined the Philippine Bidding Documents (PBDs) including the Supplemental or Bid Bulletin Numbers [insert numbers], the receipt of which is hereby duly acknowledged, we, the undersigned, offer to [supply/deliver/perform] [description of the Goods] in conformity with the said PBDs for the sum of [total Bid amount in words and figures] or the total calculated bid price, as evaluated and corrected for computational errors, and other bid modifications in accordance with the Price Schedules attached herewith and made part of this Bid. The total bid price includes the cost of all taxes, such as, but not limited to: [specify the applicable taxes, e.g. (i) value added tax (VAT), (ii) income tax, (iii) local taxes, and (iv) other fiscal levies and duties], which are itemized herein or in the Price Schedules,

If our Bid is accepted, we undertake:

- a. to deliver the goods in accordance with the delivery schedule specified in the Schedule of Requirements of the Philippine Bidding Documents (PBDs);
- b. to provide a performance security in the form, amounts, and within the times prescribed in the PBDs;
- c. to abide by the Bid Validity Period specified in the PBDs and it shall remain binding upon us at any time before the expiration of that period.

[Insert this paragraph if Foreign-Assisted Project with the Development Partner:]

Commissions or gratuities, if any, paid or to be paid by us to agents relating to this Bid, and to contract execution if we are awarded the contract, are listed below:

Name and address Amount and Purpose of
of agentCurrencyCommission or gratuity

(if none, state "None")]

Until a formal Contract is prepared and executed, this Bid, together with your written acceptance thereof and your Notice of Award, shall be binding upon us.

We understand that you are not bound to accept the Lowest Calculated Bid or any Bid you may receive.

We certify/confirm that we comply with the eligibility requirements pursuant to the PBDs.

The undersigned is authorized to submit the bid on behalf of [name of the bidder] as evidenced by the attached [state the written authority].

We acknowledge that failure to sign each and every page of this Bid Form, including the attached Schedule of Prices, shall be a ground for the rejection of our bid.

Name: _____

Legal capacity: _____

Signature: _____

Duly authorized to sign the Bid for and behalf of: _____

Date: _____

Bid Securing Declaration Form

[shall be submitted with the Bid if bidder opts to provide this form of bid security]

REPUBLIC OF THE PHILIPPINES)
CITY OF _____) S.S.

BID SECURING DECLARATION Project Identification No.: *[Insert number]*

To: *[Insert name and address of the Procuring Entity]*

I/We, the undersigned, declare that:

1. I/We understand that, according to your conditions, bids must be supported by a Bid Security, which may be in the form of a Bid Securing Declaration.
2. I/We accept that: (a) I/we will be automatically disqualified from bidding for any procurement contract with any procuring entity for a period of two (2) years upon receipt of your Blacklisting Order; and, (b) I/we will pay the applicable fine provided under Section 6 of the Guidelines on the Use of Bid Securing Declaration, within fifteen (15) days from receipt of the written demand by the procuring entity for the commission of acts resulting to the enforcement of the bid securing declaration under Sections 23.1(b), 34.2, 40.1 and 69.1, except 69.1(f), of the IRR of RA No. 9184; without prejudice to other legal action the government may undertake.
3. I/We understand that this Bid Securing Declaration shall cease to be valid on the following circumstances:
 - a. Upon expiration of the bid validity period, or any extension thereof pursuant to your request;
 - b. I am/we are declared ineligible or post-disqualified upon receipt of your notice to such effect, and (i) I/we failed to timely file a request for reconsideration or (ii) I/we filed a waiver to avail of said right; and
 - c. I am/we are declared the bidder with the Lowest Calculated Responsive Bid, and I/we have furnished the performance security and signed the Contract.

IN WITNESS WHEREOF, I/We have hereunto set my/our hand/s this _____ day of *[month]* *[year]* at *[place of execution]*.

*[Insert NAME OF BIDDER OR ITS AUTHORIZED
REPRESENTATIVE]*

*[Insert signatory's legal capacity]
Affiant*

[Jurat]

[Format shall be based on the latest Rules on Notarial Practice]

Omnibus Sworn Statement (Revised)

[shall be submitted with the Bid]

REPUBLIC OF THE PHILIPPINES)
CITY/MUNICIPALITY OF _____) S.S.

AFFIDAVIT

I, [Name of Affiant], of legal age, [Civil Status], [Nationality], and residing at [Address of Affiant], after having been duly sworn in accordance with law, do hereby depose and state that:

1. *[Select one, delete the other:]*

[If a sole proprietorship:] I am the sole proprietor or authorized representative of [Name of Bidder] with office address at [address of Bidder];

[If a partnership, corporation, cooperative, or joint venture:] I am the duly authorized and designated representative of [Name of Bidder] with office address at [address of Bidder];

2. *[Select one, delete the other:]*

[If a sole proprietorship:] As the owner and sole proprietor, or authorized representative of [Name of Bidder], I have full power and authority to do, execute and perform any and all acts necessary to participate, submit the bid, and to sign and execute the ensuing contract for [Name of the Project] of the [Name of the Procuring Entity], as shown in the attached duly notarized Special Power of Attorney;

[If a partnership, corporation, cooperative, or joint venture:] I am granted full power and authority to do, execute and perform any and all acts necessary to participate, submit the bid, and to sign and execute the ensuing contract for [Name of the Project] of the [Name of the Procuring Entity], as shown in the attached [state title of attached document showing proof of authorization (e.g., duly notarized Secretary's Certificate, Board/Partnership Resolution, or Special Power of Attorney, whichever is applicable);];

3. [Name of Bidder] is not "blacklisted" or barred from bidding by the Government of the Philippines or any of its agencies, offices, corporations, or Local Government Units, foreign government/foreign or international financing institution whose blacklisting rules have been recognized by the Government Procurement Policy Board, **by itself or by relation, membership, association, affiliation, or controlling interest with another blacklisted person or entity as defined and provided for in the Uniform Guidelines on Blacklisting;**
4. Each of the documents submitted in satisfaction of the bidding requirements is an authentic copy of the original, complete, and all statements and information provided therein are true and correct;
5. [Name of Bidder] is authorizing the Head of the Procuring Entity or its duly authorized representative(s) to verify all the documents submitted;
6. *[Select one, delete the rest:]*

[If a sole proprietorship:] The owner or sole proprietor is not related to the Head of the Procuring Entity, members of the Bids and Awards Committee (BAC), the Technical Working Group, and the BAC Secretariat, the head of the Project Management Office or the end-user unit, and the project consultants by consanguinity or affinity up to the third civil degree;

[If a partnership or cooperative:] None of the officers and members of [Name of Bidder] is related to the Head of the Procuring Entity, members of the Bids and Awards Committee (BAC), the Technical Working Group, and the BAC Secretariat, the head of the Project Management Office or the end-user unit, and the project consultants by consanguinity or affinity up to the third civil degree;

[If a corporation or joint venture:] None of the officers, directors, and controlling stockholders of *[Name of Bidder]* is related to the Head of the Procuring Entity, members of the Bids and Awards Committee (BAC), the Technical Working Group, and the BAC Secretariat, the head of the Project Management Office or the end-user unit, and the project consultants by consanguinity or affinity up to the third civil degree;

7. *[Name of Bidder]* complies with existing labor laws and standards; and
8. *[Name of Bidder]* is aware of and has undertaken the responsibilities as a Bidder in compliance with the Philippine Bidding Documents, which includes:
 - a. Carefully examining all of the Bidding Documents;
 - b. Acknowledging all conditions, local or otherwise, affecting the implementation of the Contract;
 - c. Making an estimate of the facilities available and needed for the contract to be bid, if any; and
 - d. Inquiring or securing Supplemental/Bid Bulletin(s) issued for the *[Name of the Project]*.
9. *[Name of Bidder]* did not give or pay directly or indirectly, any commission, amount, fee, or any form of consideration, pecuniary or otherwise, to any person or official, personnel or representative of the government in relation to any procurement project or activity.
10. **In case advance payment was made or given, failure to perform or deliver any of the obligations and undertakings in the contract shall be sufficient grounds to constitute criminal liability for Swindling (Estafa) or the commission of fraud with unfaithfulness or abuse of confidence through misappropriating or converting any payment received by a person or entity under an obligation involving the duty to deliver certain goods or services, to the prejudice of the public and the government of the Philippines pursuant to Article 315 of Act No. 3815 s. 1930, as amended, or the Revised Penal Code.**

IN WITNESS WHEREOF, I have hereunto set my hand this _____ day of _____, 20____ at _____, Philippines.

*[Insert NAME OF BIDDER OR ITS AUTHORIZED
REPRESENTATIVE]
[Insert signatory's legal capacity]
Affiant*

Jurat
[Format shall be based on the latest Rules on Notarial Practice]

Price Schedule for Goods Offered from Abroad
[shall be submitted with the Bid if bidder is offering goods from Abroad]

For Goods Offered from Abroad

Name of Bidder _____ Project ID No. _____ Page ___ of ___

1	2	3	4	5	6	7	8	9
Item	Description	Country of origin	Quantity	Unit price CIF port of entry (specify port) or CIP named place (specify border point or place of destination)	Total CIF or CIP price per item (col. 4 x 5)	Unit Price Delivered Duty Unpaid (DDU)	Unit price Delivered Duty Paid (DDP)	Total Price delivered DDP (col 4 x 8)
	Brand							

Name: _____

Legal Capacity: _____

Signature: _____

Duly authorized to sign the Bid for and behalf of: _____

Price Schedule for Goods Offered from Within the Philippines
[shall be submitted with the Bid if bidder is offering goods from within the Philippines]

For Goods Offered from Within the Philippines

Name of Bidder _____ Project ID No. _____ Page ____ of ____

1	2	3	4	5	6	7	8	9	10
Item	Description	Country of origin	Quantity	Unit price EXW per item	Transportation and all other costs incidental to delivery, per item	Sales and other taxes payable if Contract is awarded, per item	Cost of Incidental Services, if applicable, per item	Total Price, per unit (col 5+6+7+8)	Total Price delivered Final Destination (col 9) x (col 4)
	Brand								

Name: _____

Legal Capacity: _____

Signature: _____

Duly authorized to sign the Bid for and behalf of: _____

NFCC COMPUTATION FOR ELIGIBILITY CHECK

- A. Summary of the Applicant Supplier's/Distributor's/Manufacturer's assets and liabilities on the basis of the attached income tax return and audited financial statement, stamped "RECEIVED" by the Bureau of Internal Revenue or BIR authorized collecting agent, for the immediately preceding year and a certified copy of Schedule of Fixed Assets particularly the list of construction equipment.

	Year 20_____
1. Total Assets	
2. Current Assets	
3. Total Liabilities	
4. Current Liabilities	
5. Net Worth(1-3)	
6. Net Working Capital(2-4)	

- B. The Net Financial Contracting Capacity (NFCC) based on the above data is computed as follows:

NFCC= [(Current assets minus current liabilities) (15)] minus the value of all outstanding or uncompleted portions of the projects under ongoing contracts, including awarded contracts yet to be started, coinciding with the contract to be bid.

The values of the domestic bidder's current assets and current liabilities shall be based on the latest Audited Financial Statements (AFS) submitted to the BIR.

The Bidder shall attach the AFS to the NFCC Computation for Eligibility Check Form.

NFCC=P_____

Submitted by:

Name of Supplier/Distributor/Manufacturer _____

Signature of Authorized Representative _____

Date: _____

STATEMENT OF SINGLE LARGEST COMPLETED CONTRACT SIMILAR TO THE CONTRACT TO BE BID

This is to certify that _____ (company) _____ has the following completed contracts within Three (3) years from the date of submission and receipt of bids.

Date of the Contract	Contracting Party	Name of Contract	Kind of Goods Sold	Amount of Contract	Date of Delivery/ End-user's Acceptance	Date of Official Receipt	Bidder is A) Manufacturer B) Supplier C) Distributor

Name and Signature of
Authorized Representative

Date

***Instructions:**

- a) Cut-off date as of:
 - (i) Up to the day before the deadline of submission of bids.
- b) In the column under "Dates", indicate the dates of Delivery/ End-user's Acceptance and Official Receipt.
- c) "Name of Contract". Indicate here the Nature/ Scope of the Contract for the Procuring Entity to determine the relevance of the entry with the Procurement at hand. Example: "Supply and Delivery of _____ for Valenzuela Medical Center"

STATEMENT OF: (I) ONGOING CONTRACTS AND; (II) AWARDED BUT NOT YET STARTED CONTRACTS

This is to certify that _____ has the following ongoing and awarded but not yet started contracts:

Date of the Contract	Contracting Party	Name of Contract	Kind of Goods Sold	Amount of Contract	Value of Outstanding Contracts	Bidder is A) Manufacturer B) Supplier C) Distributor

Name and Signature of
Authorized Representative

Date

***Instructions:**

- a) State all ongoing contracts including those awarded but not yet started (government and private contracts which may be similar or not similar to the project called for bidding) as of:
 - i. The day before the deadline of submission of bids.
 - b) If there is no ongoing contract including awarded but not yet started as of the aforementioned period, state none or equivalent term.
 - c) The total amount of the ongoing and awarded but not yet started contracts should be consistent with those used in the Net Financial Contracting Capacity (NFCC) in case an NFCC is submitted as an eligibility document.
 - d) "Name of Contract". Indicate here the Nature/ Scope of the Contract for easier tracking of the entries/ representations. Example: "Supply and Delivery of _____ for Valenzuela Medical Center"