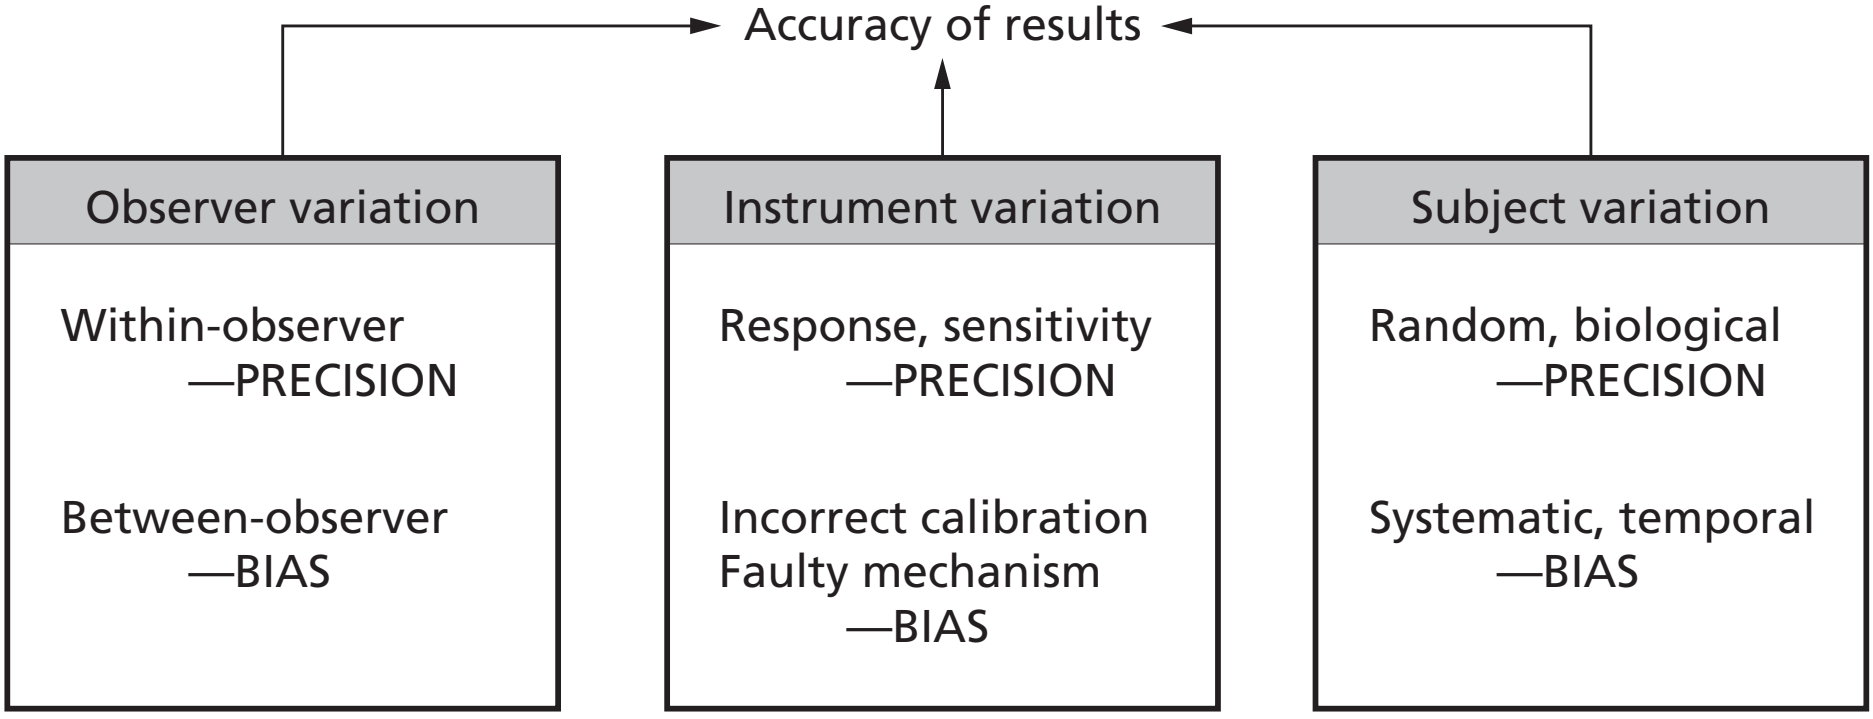

Accuracy of results
Observer variation
Within-observer
—PRECISION
Between-observer
—BIAS
Instrument variation
Response, sensitivity
—PRECISION
Incorrect calibration
Faulty mechanism
—BIAS
Subject variation
Random, biological
—PRECISION
Systematic, temporal
—BIAS