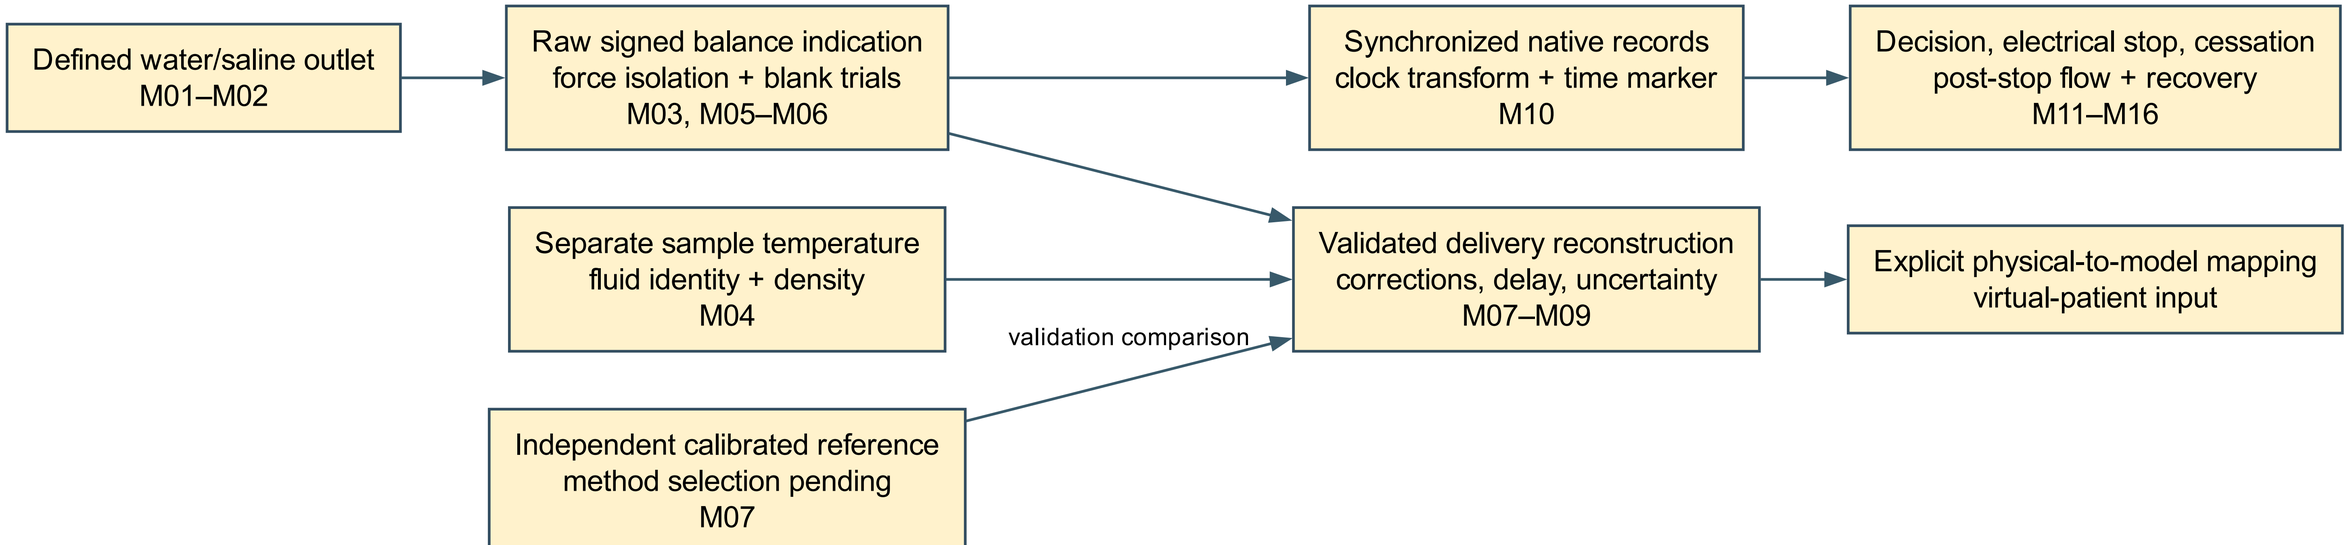
Defined water/saline outlet
M01–M02
Raw signed balance indication
force isolation + blank trials
M03, M05–M06
Synchronized native records
clock transform + time marker
M10
Decision, electrical stop, cessation
post-stop flow + recovery
M11–M16
Separate sample temperature
fluid identity + density
M04
Validated delivery reconstruction
corrections, delay, uncertainty
M07–M09
Explicit physical-to-model mapping
virtual-patient input
validation comparison
Independent calibrated reference
method selection pending
M07