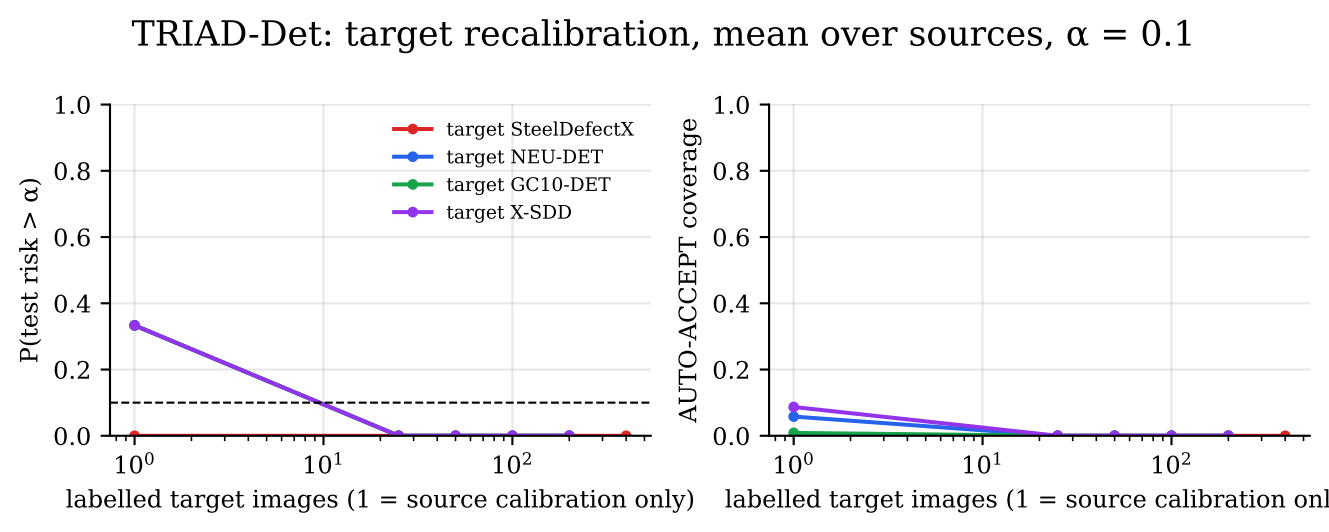
TRIAD-Det: target recalibration, mean over sources, α = 0.1
P(test risk > α)
AUTO-ACCEPT coverage
target SteelDefectX
target NEU-DET
target GC10-DET
target X-SDD
1.0
0.8
0.6
0.4
0.2
0.0
$10^0$
$10^1$
$10^2$
labelled target images (1 = source calibration only)
labelled target images (1 = source calibration onl