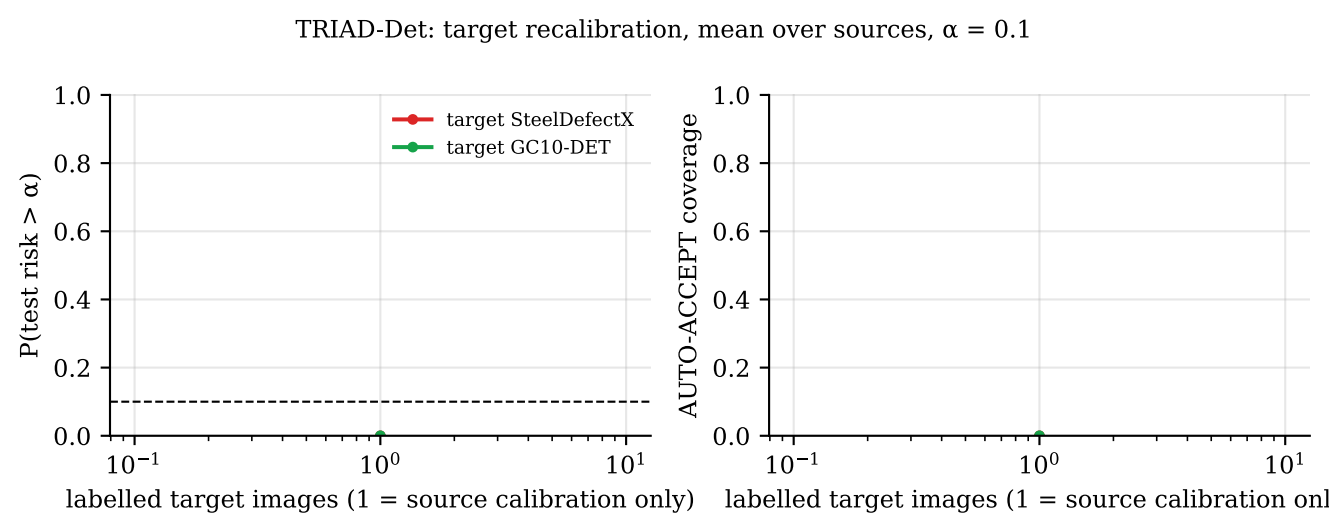
TRIAD-Det: target recalibration, mean over sources, α = 0.1
P(test risk > α)
target SteelDefectX
target GC10-DET
1.0
0.8
0.6
0.4
0.2
0.0
10^{-1}
10^{0}
10^{1}
labelled target images (1 = source calibration only)
AUTO-ACCEPT coverage
labelled target images (1 = source calibration onl