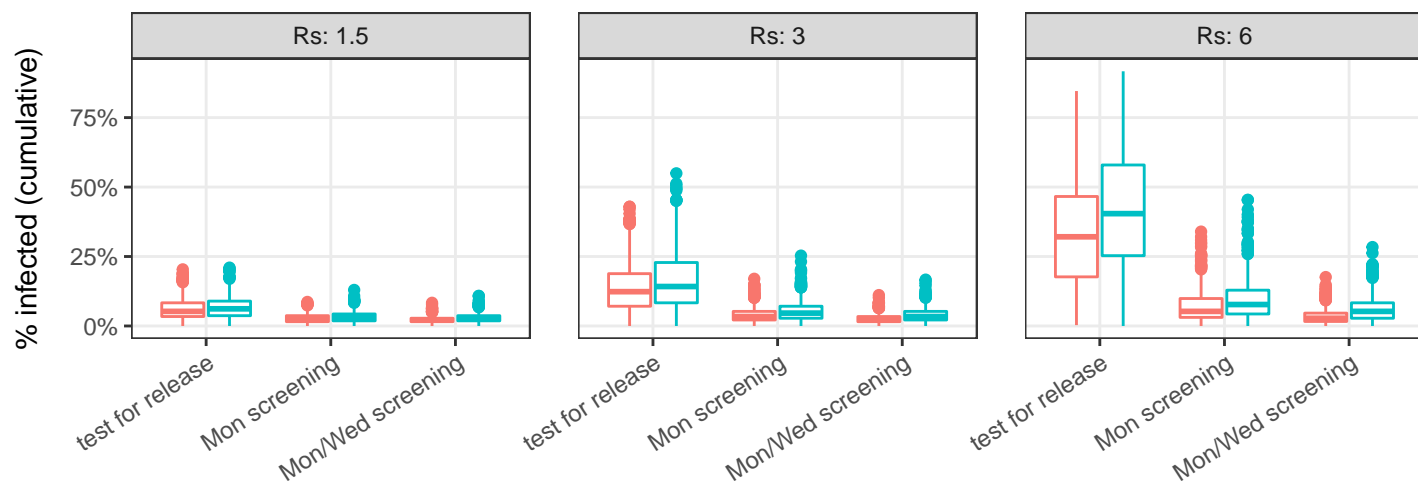


A

mean LFD test compliance:  1.00  0.67

B

 test for release
  Mon screening
  Mon/Wed screening
