



sam_2026-10-08_10-20-43_Connect-GAPDH.pcrd

10/09/2026 13:20

Report Information

User: BioRad/sam

Data File Name: sam_2026-10-08_10-20-43_Connect-GAPDH.pcrd

Data File Path: C:\Users\Samb\Desktop

Well Group Name: All Wells

Report Differs from Last Save: No

Run Setup

Run Information

Run Date: 10/08/2026 10:20

Run User: sam

Run Type: User-defined

Plate File: 20261008-mgig-GAPDH-polyIC-valentina.pltd

ID:

Notes:

Sample Volume: 20

Temperature Control Mode: Calculated

Lid Temperature: 105

Base Serial Number: BR006896

Optical Head Serial Number: 788BR07000

Protocol

1: 95.0°C for 0:30

2: 95.0°C for 0:03

3: 60.0°C for 0:05

Plate Read

4: GOTO 2, 39 more times

5: Melt Curve 65.0°C to 95.0°C: Increment 0.5°C 0:05


Plate Read

Plate Display

[illegible]

Quantification

Step #: 3
Analysis Mode: Target
Cq Determination: Single Threshold
Baseline Method:
GAPDH: Auto Calculated
Threshold Setting:
GAPDH: 4114.20, Auto Calculated

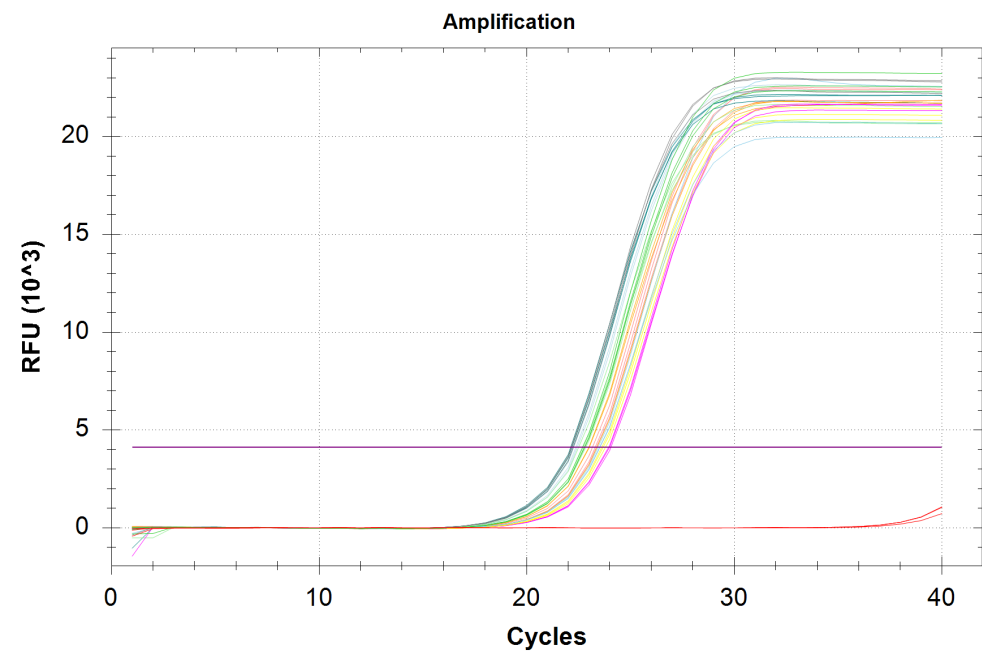

Quantification Data

Well	Fluor	Target	Content	Sample	Cq	Cq Mean	Cq Std. Dev
A01	SYBR	GAPDH	Unkn-01	A1PC	23.17	23.27	0.096
A02	SYBR	GAPDH	Unkn-01	A1PC	23.36	23.27	0.096
A03	SYBR	GAPDH	Unkn-01	A1PC	23.30	23.27	0.096
A04	SYBR	GAPDH	Unkn-02	A2PC	22.26	22.36	0.084
A05	SYBR	GAPDH	Unkn-02	A2PC	22.37	22.36	0.084
A06	SYBR	GAPDH	Unkn-02	A2PC	22.43	22.36	0.084
A07	SYBR	GAPDH	Unkn-03	A3PC	22.12	22.18	0.059
A08	SYBR	GAPDH	Unkn-03	A3PC	22.24	22.18	0.059
A09	SYBR	GAPDH	Unkn-03	A3PC	22.18	22.18	0.059
A10	SYBR	GAPDH	Unkn-04	A4PC	23.00	23.13	0.220
A11	SYBR	GAPDH	Unkn-04	A4PC	23.39	23.13	0.220
A12	SYBR	GAPDH	Unkn-04	A4PC	23.02	23.13	0.220
B01	SYBR	GAPDH	Unkn-05	A5PC	22.50	22.69	0.175
B02	SYBR	GAPDH	Unkn-05	A5PC	22.71	22.69	0.175
B03	SYBR	GAPDH	Unkn-05	A5PC	22.85	22.69	0.175
B04	SYBR	GAPDH	Unkn-06	B1PC	24.06	24.00	0.055
B05	SYBR	GAPDH	Unkn-06	B1PC	23.95	24.00	0.055
B06	SYBR	GAPDH	Unkn-06	B1PC	23.99	24.00	0.055
B07	SYBR	GAPDH	Unkn-07	B2PC	23.79	23.70	0.091
B08	SYBR	GAPDH	Unkn-07	B2PC	23.68	23.70	0.091

Quantification Data

Well	Fluor	Target	Content	Sample	Cq	Cq Mean	Cq Std. Dev
B09	SYBR	GAPDH	Unkn-07	B2PC	23.61	23.70	0.091
B10	SYBR	GAPDH	Unkn-08	B3PC	23.53	23.49	0.049
B11	SYBR	GAPDH	Unkn-08	B3PC	23.43	23.49	0.049
B12	SYBR	GAPDH	Unkn-08	B3PC	23.51	23.49	0.049
C01	SYBR	GAPDH	Unkn-09	B4PC	22.16	22.18	0.053
C02	SYBR	GAPDH	Unkn-09	B4PC	22.24	22.18	0.053
C03	SYBR	GAPDH	Unkn-09	B4PC	22.14	22.18	0.053
C04	SYBR	GAPDH	Unkn-10	B5PC	22.69	22.75	0.058
C05	SYBR	GAPDH	Unkn-10	B5PC	22.77	22.75	0.058
C06	SYBR	GAPDH	Unkn-10	B5PC	22.80	22.75	0.058
C07	SYBR	GAPDH	NTC-01		N/A	0.00	0.000
C08	SYBR	GAPDH	NTC-01		N/A	0.00	0.000
C09	SYBR	GAPDH	NTC-01		N/A	0.00	0.000

QC Parameters

Data

Description	Value	Use	Results	Exclude Wells	All excluded wells
Negative control with a Cq less than	38	True		False	
NTC with a Cq less than	38	True		False	
NRT with a Cq less than	38	True		False	
Positive control with a Cq greater than	30	True		False	
Unknown without a Cq	N/A	True		False	
Standard without a Cq	N/A	True		False	
Efficiency greater than	110.0	True			
Efficiency less than	90.0	True			
Std Curve R^2 less than	0.980	True			
Replicate group Cq Std Dev greater than	0.20	True	GAPDH:A10, A11, A12.	False	