
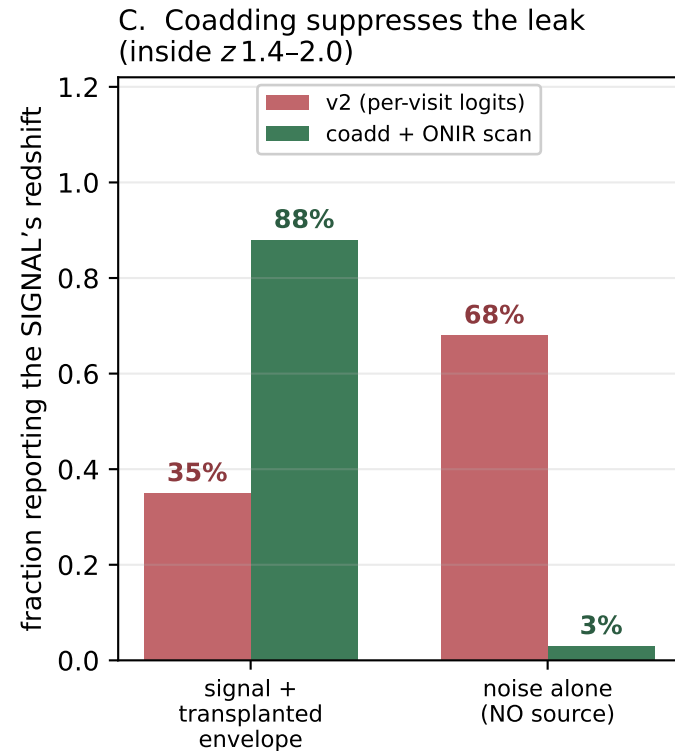
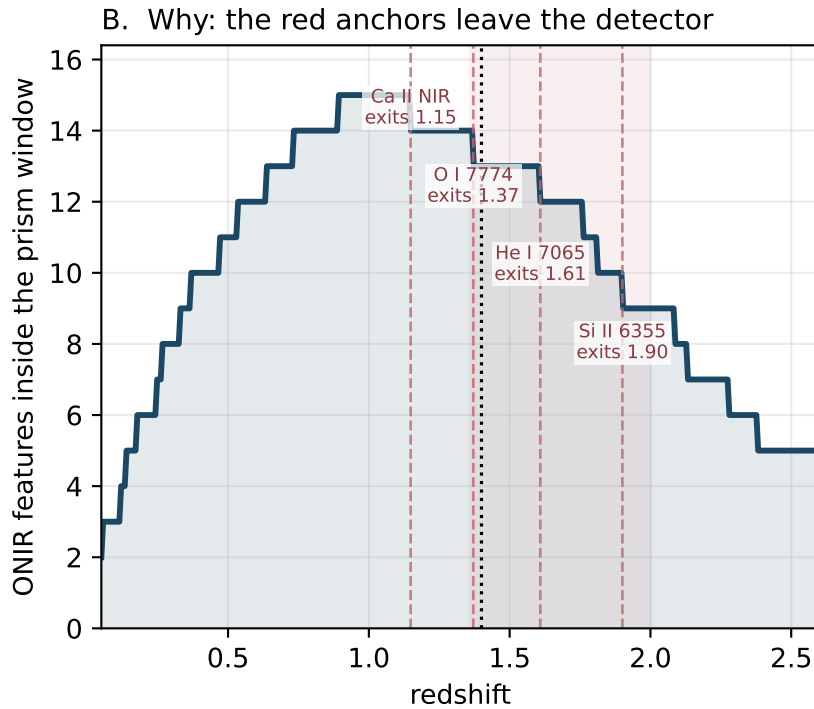


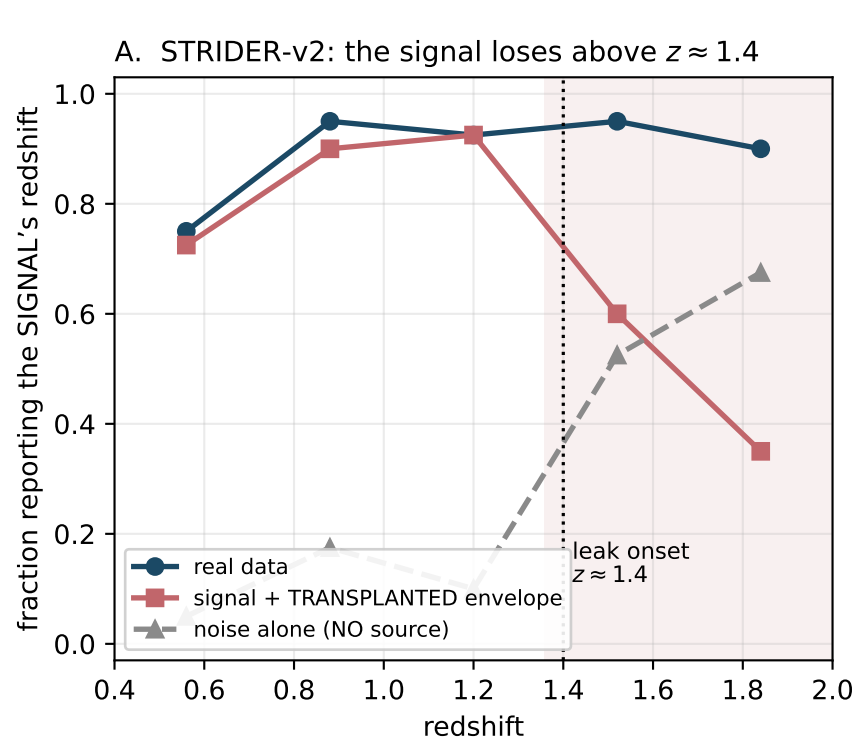

Transplant protocol: clean signal from a target object, noise drawn from a DIFFERENT object's error envelope at a well-separated redshift. v2: $n=200$, $z 0.4-2.0$. Coadd scan: $n=78-90$, untrained template matching, positive control passed.