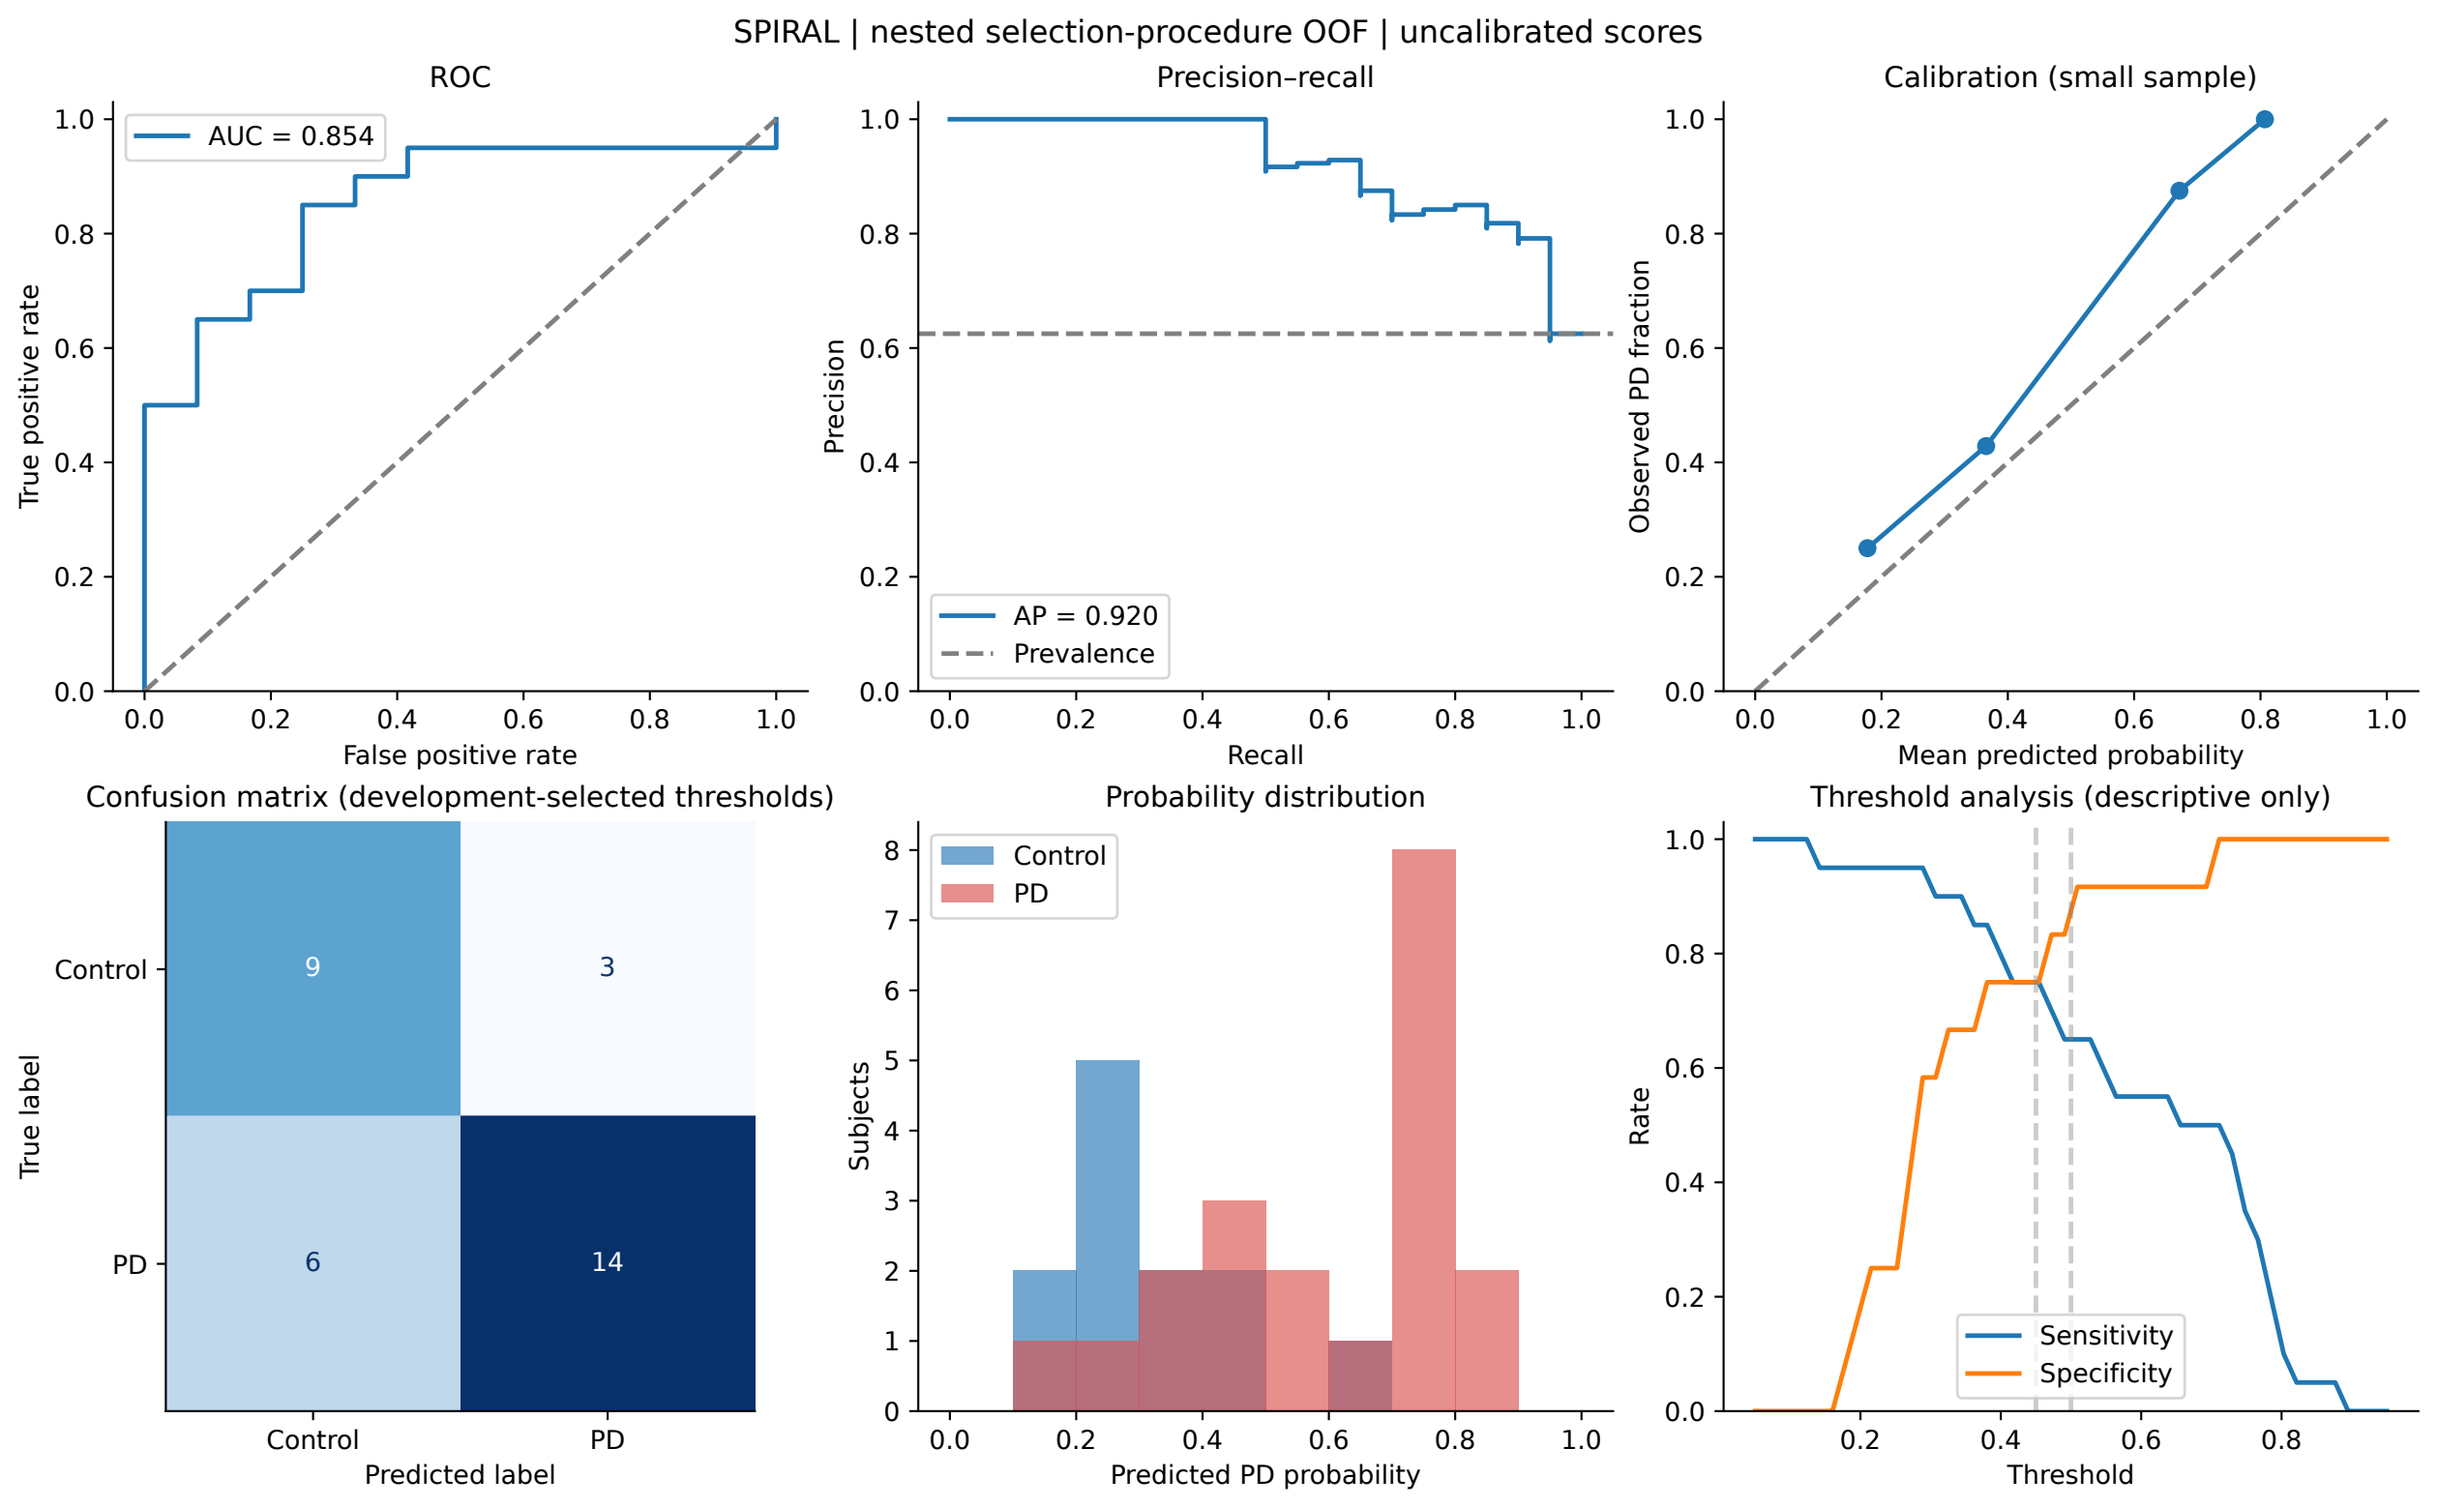
SPIRAL | nested selection-procedure OOF | uncalibrated scores
ROC
AUC = 0.854
True positive rate
False positive rate
Precision–recall
AP = 0.920
Prevalence
Precision
Recall
Calibration (small sample)
Observed PD fraction
Mean predicted probability
Confusion matrix (development-selected thresholds)
Control
PD
9
3
6
14
True label
Predicted label
Probability distribution
Control
PD
Subjects
Predicted PD probability
Threshold analysis (descriptive only)
Sensitivity
Specificity
Rate
Threshold