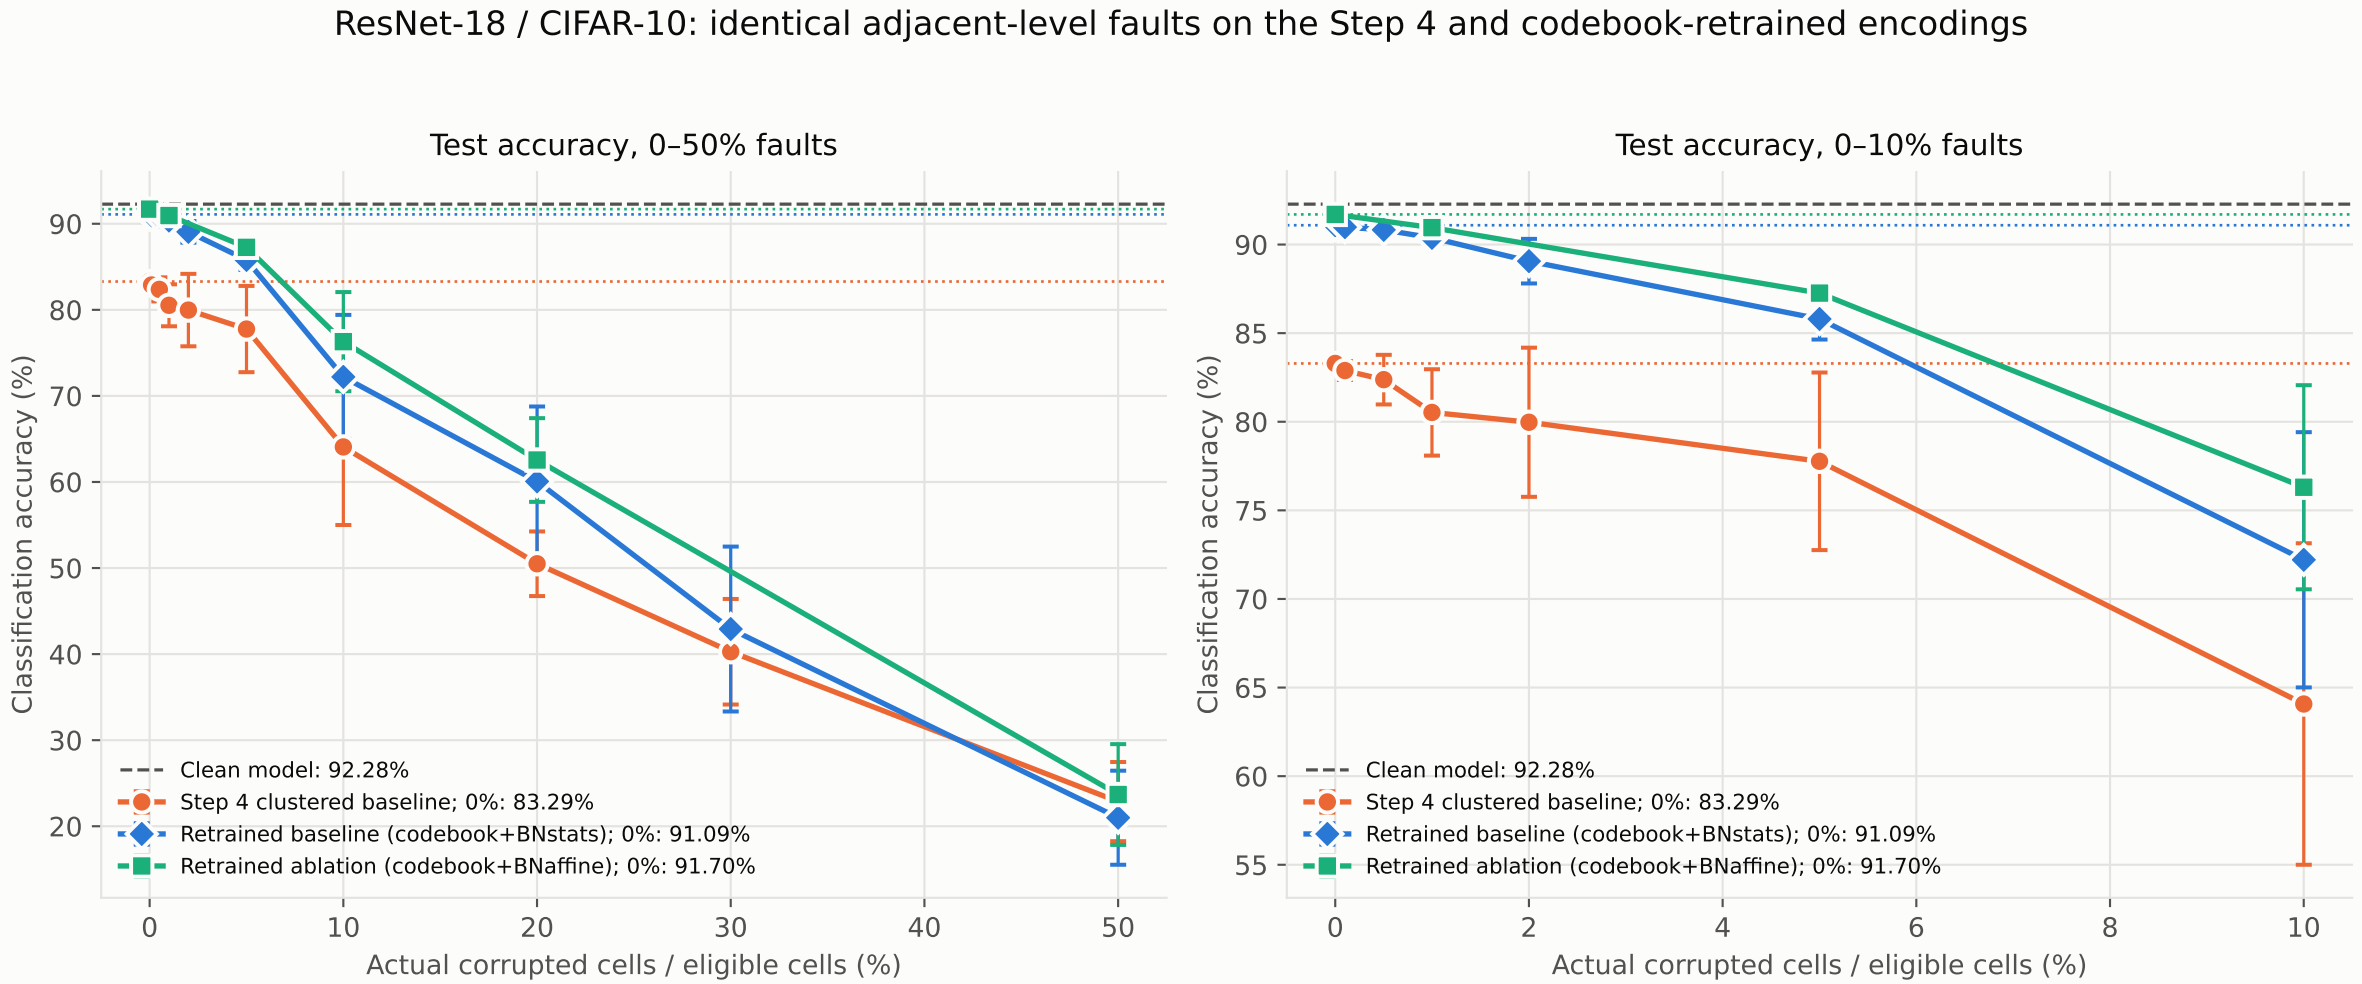
ResNet-18 / CIFAR-10: identical adjacent-level faults on the Step 4 and codebook-retrained encodings
Test accuracy, 0–50% faults
Test accuracy, 0–10% faults
Classification accuracy (%)
Actual corrupted cells / eligible cells (%)
Clean model: 92.28%
Step 4 clustered baseline; 0%: 83.29%
Retrained baseline (codebook+BNstats); 0%: 91.09%
Retrained ablation (codebook+BNaffine); 0%: 91.70%
Mean ± 1 sample SD across 5 static patterns per nonzero rate; identical cells faulted in every encoding. Dotted lines: each encoding at 0% faults. No LoRA.