

BS-200/BS-220/BS-120/BS-130/BS-180 Chemistry Analyzer

Host Interface Manual



© 2007-2009 Shenzhen Mindray Bio-medical Electronics Co., Ltd. All rights Reserved.

For this manual, the issued Date is 2009-08.

Intellectual Property Statement

SHENZHEN MINDRAY BIO-MEDICAL ELECTRONICS CO., LTD. (hereinafter called Mindray) owns the intellectual property rights to this Mindray product and this manual. This manual may refer to information protected by copyright or patents and does not convey any license under the patent rights or copyright of Mindray, or of others.

Mindray intends to maintain the contents of this manual as confidential information. Disclosure of the information in this manual in any manner whatsoever without the written permission of Mindray is strictly forbidden.

Release, amendment, reproduction, distribution, rental, adaptation, translation or any other derivative work of this manual in any manner whatsoever without the written permission of Mindray is strictly forbidden.




OmniLab

DigiPrince

MINDRAY

BeneView, WATO,

BeneHeart,  are the trademarks, registered or otherwise, of Mindray in China and other countries. All other trademarks that appear in this manual are used only for informational or editorial purposes. They are the property of their respective owners.

Responsibility on the Manufacturer Party

Contents of this manual are subject to change without prior notice.

All information contained in this manual is believed to be correct. Mindray shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this manual.

Mindray is responsible for the effects on safety, reliability and performance of this product, only if:

- all installation operations, expansions, changes, modifications and repairs of this product are conducted by Mindray authorized personnel;
- the electrical installation of the relevant room complies with the applicable national and local requirements; and
- the product is used in accordance with the instructions for use.

**WARNING:**

It is important for the hospital or organization that employs this equipment to carry out a reasonable service/maintenance plan. Neglect of this may result in machine breakdown or personal injury.

**NOTE:**

This equipment must be operated by skilled/trained clinical professionals.

Warranty

THIS WARRANTY IS EXCLUSIVE AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING WARRANTIES OF MERCHANTABILITY OR FITNESS FOR ANY PARTICULAR PURPOSE.

Define:

- **Main unit:** Integrated facilities which implements the specified function separately. General speaking, it should include power supply, control system and some functional modules.
- **Accessories:** Materials connected to Main Unit to extend or implement specified function.
- **Consumables:** Disposable or short-life parts which should be replaced each time after use or periodically

Exemptions

Mindray's obligation or liability under this warranty does not include any transportation or other charges or liability for direct, indirect or consequential damages or delay resulting from the improper use or application of the product or the use of parts or accessories not approved by Mindray or repairs by people other than Mindray authorized personnel.

This warranty shall not extend to:

- **Malfunction or damage caused by improper use or man-made failure.**
- **Malfunction or damage caused by unstable or out-of-range power input.**
- **Malfunction or damage caused by force majeure such as fire and earthquake.**

- **Malfunction or damage caused by improper operation or repair by unqualified and unauthorized service people.**
- **Malfunction of the instrument or part whose serial number is not legible enough.**
- **Others not caused by instrument or part itself.**

The standard warranty period is as below:

- **Main unit: 18 months from shipment**
- **Accessories: 15 months from shipment**
- **Consumables: N/A**

Return Policy

Return Procedure

In the event that it becomes necessary to return this product or part of this product to Mindray, the following procedure should be followed:

- 1 Return authorization: Contact the international Customer Service Department and obtain a Return Materials Authorization number. This number must appear on the outside of the shipping container. Returned shipments will not be accepted if the number is not clearly visible. Please provide the model number, serial number, and a brief description of the reason for return.
- 2 Freight policy: The customer is responsible for freight charges when this product is shipped to Mindray for service (this includes customs charges).
- 3 Return address: Please send the part(s) or equipment to the address offered by the international Customer Service Department

Company Contact

Manufacturer: **Shenzhen Mindray Bio-Medical Electronics Co., Ltd.**

E-mail Address: **service@mindray.com.cn**

Tel: **+86 755 26582479 26582888**

Fax: **+86 755 26582934 26582500**

EC-Representative: **Shanghai International Holding Corp. GmbH(Europe)**

Address: **Eiffestraße 80, Hamburg 20537, Germany**

Tel: 0049-40-2513175

Fax: 0049-40-255726

Preface

Who Should Read This Manual


This manual is written for LIS (Laboratory Information Management System) developers and those who need to learn the HL7 interface used by Mindray. Instructions are provided in this manual for LIS developers to guide them to develop LIS interface that enables their LIS to communicate with the chemistry analyzer of Mindray. The developers are expected to have knowledge of LIS and HL7 standards, and capacity of network programming. The communication protocol is TCP/IP for network layer and HL7 version 2.3.1 for application layer. LIS developers are recommended to develop the LIS interface using Visual C++, Visual Basic, etc. in the Windows operating system.

What Can You Find in This Manual

This operation manual introduces the HL7 interface used by Mindray on the BS-200/BS-220/BS-120/BS-130/BS-180 Chemistry Analyzer. Chapter 1 describes the HL7 interface generally. The BS-200/BS-220/BS-120/BS-130/BS-180 supports bidirectional communication with LIS, that is, it can not only send test results to LIS but also download sample information from LIS. Chapter 2 explains the bidirectional communication in detail. Please note that the "Manufacturer" and "Model" appearing in all HL7 messages of this manual respectively refer to the name of the manufacturer and the product model, which will be assigned with corresponding values of each product.

Conventions Used in This Manual

This chart explains the symbols used in this manual.

When you see ...	Then ...
 NOTE:	Read the statement following the symbol. The statement is alerting you to information that requires your attention.

Contents

- Preface 1**
 - Who Should Read This Manual 1
 - What Can You Find in This Manual..... 1
 - Conventions Used in This Manual 1
- Contents 1**
- 1 Mindray HL7 Interface..... 2**
 - 1.1 Messages Compatible with HL7 Interface..... 2
 - 1.2 HL7 Lower Layer Protocol 2
 - 1.3 Minimal Lower Layer Protocol（MLLP） 3
- 2 Communication and HL7 Protocol 4**
 - 2.1 Message Grammar 4
 - 2.2 Compatible HL7 Messages 5
- 3 Communication Process and Message Example 24**

1 Mindray HL7 Interface

HL7 interface is developed by Mindray for the BS-200/BS-220/BS-120/BS-130/BS-180 Chemistry Analyzer to adapt to the prevailing Laboratory Information Management System (LIS). It provides a channel for analyzer and other IP-based networks. With TCP/IP, the LIS host can receive test results from chemistry analyzers, which also send patient information, sample information and test results to LIS in real-time or batch mode. Therefore, users can identify samples by both scanning sample bar code and downloading from LIS host. This chapter describes the two communication modes (sending and downloading). All data are transmitted in format of HL7 v2.3.1. This interface enables bidirectional communication between the chemistry analyzer and the LIS host.

1.1 Messages Compatible with HL7 Interface

HL7, a transmission standard for electronic data and providing nurse for inpatients, was first defined by Americans and now has been applied by many countries. Mindray HL7 interface is defined based upon HL7 v2.3.1. Refer to *HL7 Interface Standards Version 2.3.1* for details.

Only portion of the messages, segments and other data defined are used for Mindray HL7 interface that needs only part of these data.

1.2 HL7 Lower Layer Protocol

TCP/IP is a byte stream protocol, which does not provide message border. HL7 is a higher layer protocol that is based upon messages but provides no message termination mechanism. To determine the message border, the minimal lower layer protocol is used. Refer to *HL7 Interface Standards Version 2.3.1* for details.

Communication Layer

Messages are transmitted in format of:

<SB> ddddd <EB><CR>

Where,

■ <SB> = Start Block character (1 byte)

ASCII <VT>, namely <0x0B>, must not be confused with the SOH or STX in ASCII.

■ ddddd = Data (variable number of bytes)

dddd is an HL7 message, which only includes ISO 8859-1 characters (hexadecimal 20-FF) and <CR>, exclusive of other control characters and those that can't be printed out.

■ <EB> = End Block character (1 byte)

ASCII <FS>, namely <0x1C>, must not be confused with the ETX or EOT in ASCII.

■ <CR> = Carriage Return (1 byte)

Enter character in ASCII is <0x0D>.

1.3 Minimal Lower Layer Protocol (MLLP)

This interface is compatible with the Minimal Lower Layer Protocol (MLLP) of HL7.

MLLP, an encapsulation of HL7 messages, is defined in the HL7 standard. HL7 messages are encapsulated with a single character at the beginning and a dual character at the end. The characters used by the HL7 interface are default in the HL7 standard.

Start character: Hexadecimal <0B>

End character: Hexadecimal <1C><0D>

2 Communication and HL7 Protocol

Communication here concerns result sending and sample information downloading. The former means the analyzer transmits the measurement data to an external system (such as the LIS). There are two types of transmission: real-time and batch. Batch-mode transmission is not allowed in two conditions: 1) Real-time mode is enabled; 2) The system is in testing status. The latter means the analyzer downloads sample information from LIS in real-time or batch mode. Real-time mode can be achieved only if a sample bar code reader is equipped. Batch-mode downloading refers to retrieving samples in certain period of the day.

This chapter introduces the message types (Ver. 2.3.1) used by Mindray HL7 interface.



NOTE:

HL7 supports many types of messages, but only 5 of them are employed on the Mindray HL7 interface.

2.1 Message Grammar

This section introduces the general grammar of Mindray HL7 interface.



NOTE:

For complete and detailed descriptions of HL7 message grammar, refer to the HL7 standard written by the HL7 standard committee.

Each HL7 message is composed of segments that end with <CR>.

Each segment consists of a name (three characters) and variable fields that are composed of components and subcomponents. The separators of each element are defined in the MSH segment in every message.

For instance,

```
MSH|^~\&|Manufacturer|Model|||20060427194802||ORU^R01|1|P|2.3.1|||0||ASCII|||
```

Where, the five characters following MSH are defined as delimiters to separate the fields, components and subcomponents. Although the characters can be any non-text ones, the HL7 standard recommends you to use the following:

Character	Description
	Field separator
^	Component separator
&	Subcomponent separator
~	Repetition separator
\	Escape character

The first field of MSH includes all separators and most of other fields are empty. These fields are optional and not used by Mindray HL7 interface.

Field 9	Includes message types (ORU)
Field 10	Includes an unique text string to indicate message ID
Field 11	Includes processing ID (P refers to product)
Field 12	Defines the version of HL7 (2.3.1) for the message

The order of the segments following MSH in every message is specially specified.



NOTE:

A segment is defined as optional or to be repeated by using the following grammar:


[] indicates the segment in it is optional.

{ } indicates the segment in it can be repeated for 0 or 1 time or more.


2.2 Compatible HL7 Messages

All messages used for HL7 interface include ORU, ACK, QRY, QCK and DSR.

Test results are transferred as follows:

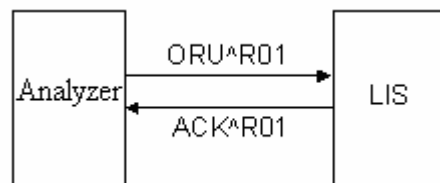

Sample information is downloaded from LIS as follows:

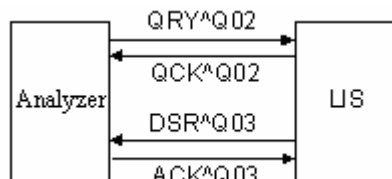

ORU/ACK: Observe result (unsolicited)/Acknowledgment

ORU^R01 is used to transmit sample result, QC result and calibration results to the LIS host. (Transmission of calibration results is not allowed on the BS-200/BS-220/BS-120/BS-130/BS-180)

An **ORU^R01** message includes:

- Patient information (patient name, sample ID, etc)
- Doctor's order (sample type, sender, tester, clinical diagnosis, etc)
- Test results (test No., concentration, unit, reference, etc)

When the test information reaches the LIS server, you can select desired items as needed.

On the BS-200/BS-220/BS-120/BS-130/BS-180, each ORU^R01 message transmits one test, which could be routine test, ISE Analyte, off-system test or calculation test. A sample with multiple tests will be transmitted via multiple ORU messages.

The structure of an **ORU** message is as follows:

<u>ORU</u>	<u>Description</u>
MSH	Message header
PID	Patient identification
OBR	Observation report ID
OBX	Observation/Result

■ Calibration result includes the following information:

- Test information (test No. and test name)
- Calibration rule and date/time
- Calibrator information (quantity, sequence number, name, lot No., expiration date, concentration, etc)
- Calibration result (response, number of calibration parameters, parameter value)

All calibration results of a test can be transmitted via one message. The above-mentioned information can be applied as needed. Refer to following contents for details.

■ QC result includes the following information:

- Test information (test No. and test name)
- Control information (name, lot No., expiration date, concentration level, mean value)
- Date/time and QC result (concentration and unit)

The above-mentioned information can be applied as needed. Refer to following contents for details.

On the BS-200/BS-220/BS-120/BS-130/BS-180, each ORU^R01 message carries the result of one QC run.

The message structure for calibration and QC results are show below:

<u>ORU</u>	<u>Observational</u>	<u>Results</u>	<u>Description</u>
<u>(Unsolicited)</u>			
MSH			Message Header
OBR			Observation report(calibration and QC)

ACK^R01 message responds to ORU message and is as follows:

<u>ACK</u>	<u>Acknowledgment</u>	<u>Description</u>
MSH		Message Header
MSA		Message Acknowledgment

QRY/QCK: Query/Query acknowledgment

QRY^Q02 message is used for sample information query on LIS and has an event Q02. The structure of **QRY** message is as follows:

<u>QRY</u>	<u>Description</u>
MSH	Message Header
QRD	Query Definition
QRF	Query Filter

QCK^Q02 message responds to QRY^Q02 message and is as follows:

<u>QCK</u>	<u>Description</u>
MSH	Message Header
MSA	Message Acknowledgment
ERR	Error
QAK	Query Acknowledgment

DSR/ACK: Display response/ Acknowledgment

DSR^Q03 message sends and displays searched results, i.e. send sample information from LIS to the analyzer. The structure of **DSR** message is as follows:

<u>DSR</u>	<u>Description</u>
MSH	Message Header
MSA	Message Acknowledgment
ERR	Error
QAK	Query Acknowledgment
QRD	Query Definition
QRF	Query Filter
{DSP}	Display Data
DSC	Continuation Pointer

ACK^Q03 responds to DSR^Q03 message and is as follows:

<u>ACK</u>	<u>Description</u>
MSH	Message Header
MSA	Message Acknowledgement
ERR	Error

Message Segment

This section describes the components of each segment: field name, field length and description.

All fields used in message segment are listed in following tables. The numbers followed by a '#' symbol indicate that the fields are required for the message.



NOTE:

Some fields, though without values, are provided in Mindray's HL7 protocol for function extension in future.

■ MSH Message Header

All HL7 messages begin with MSH, which is the first segment of an HL7 message and always located at the beginning of the message. The MSH segment defines the intention, source, purpose and grammar of the message.

The MSH segment of Mindray HL7 interface message uses the following fields:

No.	Field	Length	Description
1#	Field Separator	1	Includes the separator between segment ID and the first real field, and defines the field separators () of the remaining part of the message.
2#	Encoding Characters	4	Includes component, repetition, escape and subcomponent separators (^~\&).
3	Sending Application	180	Sending application, set to "Manufacturer".
4	Sending Facility	180	Sending facility, set to "Model".
5	Receiving Application	180	Void and reserved. Receiving application.
6	Receiving Facility	180	Void and reserved. Receiving facility.
7	Date/Time Message	Of 26	Time of the current message. Calling the system time.
8	Security	40	Void and reserved. Security.
9#	Message Type	7	Type of the message, such as ORU^R01.

No.	Field	Length	Description
10#	Message Control ID	20	Message control ID. Indicates one message each and increases from 1 with message increasing.
11#	Processing ID	3	Processing ID. Always set to P (product).
12#	Version ID	60	Version ID. Version of HL7 protocol: 2.3.1.
13	Sequence Number	15	Void and reserved. Serial number
14	Continuation Pointer	180	Void and reserved. Continuation pointer
15	Accept Acknowledgment Type	2	Void and reserved. Type of accepted acknowledgment
16	Application Acknowledgment Type	2	Void and reserved. Type of application response, used as result type. 0- Sample result; 1- Calibration result; 2- QC result. It is void in non-ORU messages.
17	Country Code	2	Void and reserved. Country code
18	Character Set	10	Character set. ASCII is used.
19	Principal Language Of Message	60	Void and reserved. Principle language of the message
20	Alternate Character Set Handling Scheme	20	Void and reserved. Handling scheme of alternate character

Comments: MSH segment applies to all messages. Fields 3 and 4 are determined by LIS manufacturer; fields 5 and 6 are set to "Manufacturer" and "Model"; fields 10 and 16 are integers; others are strings.

■ MSA - message acknowledgment segment

The MSA segment of Mindray HL7 interface message uses the following fields:

No.	Field	Length	Description
1#	Acknowledgment Code	2	Acknowledgment code. AA stands for accepted, AE for error and AR for rejected.
2#	Message Control ID	20	Message control ID, corresponding to MSH-10.
3	Text Message	80	Text message, a description of error or reject event, corresponding to field 6. It can be written into error logs.
4	Expected Sequence Number	15	Void and reserved. Expected sequence number.

No.	Field	Length	Description
5	Delayed Acknowledgment Type	1	Void and reserved. Delayed acknowledgment type.
6	Error Condition	100	Error condition (status code).

Note: Fields of MSA-6 are introduced as follows.

The status code list is shown as the figure below.

Status Code (MSA-6)	Status Text(MSA-3)	Description/Comment
Succeed:		AA
0	Message accepted	Succeed
Error code:		AE
100	Segment sequence error	Segment sequence is incorrect or required segment is missed.
101	Required field missing	Required field in a segment is missed.
102	Data type error	Data type of a field is incorrect.
103	Table value not found	Table value is not found, therefore not used temporarily.
Reject code:		AR
200	Unsupported message type	Message type is not supported.
201	Unsupported event code	Event code is not supported.
202	Unsupported processing id	Processing ID is not supported.
203	Unsupported version id	Version ID is not supported.
204	Unknown key identifier	Key identifier is unknown, such as inexistent patient information.
205	Duplicate key identifier	The key identifier already exists.
206	Application record locked	The transaction could not be performed at the application storage level, such as locked database.
207	Application internal error	Unknown application internal error.

Comments: MSA segment applies to ACK^R01, QCK^Q02 and ACK^Q03 messages. Fields 4 and 6 are integers, while others are strings.

■ PID Patient Identification

The PID segment constitutes patient information and uses the following fields:

No.	Field	Length	Description
1	Set ID – PID	10	Identifies different patient information segments
2	Patient ID	20	Patient admission No.
3#	Patient Identifier List	20	Medical record number
4	Alternate Patient ID – PID	20	Bed No.
5#	Patient Name	48	Name of patient
6	Mother's Maiden Name	48	Patient zone
7	Date/Time of Birth	26	Birth date of patient. (Format: YYYYMMDDHHMMSS). It could be void.
8	Sex	1	Patient gender. M for male F for female O for others
9	Patient Alias	48	Blood type (O, A, B and AB)
10	Race	80	Void and reserved. Race of patient.
11	Patient Address	106	Void and reserved. Address of patient.
12	County Code	4	Void and reserved. County code of patient.
13	Phone Number - Home	40	Void and reserved. Phone number (home) of patient.
14	Phone Number - Business	40	Void and reserved. Phone number (business) of patient.
15	Primary Language	60	Void and reserved. Primary language of patient.
16	Marital Status	80	Void and reserved. Marital status of patient.
17	Religion	80	Void and reserved. Religion of patient.
18	Patient Account Number	20	Void and reserved.
19	SSN Number -Patient	16	Void and reserved.
20	Driver's License Number – Patient	25	Void and reserved.
21	Mother's Identifier	20	Void and reserved. Mother's identifier.
22	Ethnic Group	80	Void and reserved.
23	Birth Place	60	Void and reserved. Birth place of patient.
24	Multiple Birth Indicator	1	Void and reserved. Multiple birth indicator, Y(yes) or N(no).

No.	Field	Length	Description
25	Birth Order	2	Void and reserved. Birth order, an integer greater than 0.
26	Citizenship	80	Void and reserved.
27	Veterans Status	Military 60	Void and reserved. Veteran military status of patient.
28	Nationality	80	Void and reserved.
29	Patient Death and Time	Date 26	Void and reserved. Patient death date and time.
30	Patient Indicator	Death 1	Void and reserved. Patient death indicator, Y (yes) or N (no).

Comments: PID segment only applies to ORU^R01 message. Fields 1 and 25 are integers; fields 24 and 30 are Booleans; others are strings.

■ OBR Observation Request

The OBR segment transmits the doctor's orders associated with the patient report. If MSH-16 is 0, Mindray HL7 interface uses the following fields:

No.	Field	Length	Description
1	Set ID – OBR	10	Identifies different OBR segments.
2	Placer Order Number	22	Order number of placer, used as sample bar code.
3	Filler Order Number	22	Order number of filler, used as sample ID.
4#	Universal Service ID	200	Universal service ID, set to "Manufacturer"^"Model".
5	Priority	2	STAT or not. Y for yes and N for no.
6	Requested Date/time	26	Void and reserved. Requesting date/time.
7	Observation Date/Time	26	Observation date/time, used as testing date/time.
8	Observation End Date/Time	26	Void and reserved. Observation end date/time.
9	Collection Volume	20	Void and reserved. Collection volume.
10	Collector Identifier	60	Void and reserved. Collector identifier.
11	Specimen Action Code	1	Void and reserved. Specimen action code.
12	Danger Code	60	Void and reserved. Danger code.
13	Relevant Clinical Info.	300	Clinical diagnosis.
14	Specimen Received Date/Time	26	Void and reserved. Specimen receiving date/time.

No.	Field	Length	Description
15	Specimen Source	300	Sample source, used as sample type, such as blood, urine, etc
16	Ordering Provider	120	Order provider, used as sender.
17	Order Callback Phone Number	40	Void and reserved. Sending department
18	Placer Field 1	60	Characteristic of sample (icterus, hemolysis and lipemia)
19	Placer Field 2	60	Void and reserved.
20	Filler Field 1	60	Attending doctor
21	Filler Field 2	60	Treatment department
22	Result Rpt/Status Change – Date/Time	26	Void and reserved. Result report/status change-date/time.
23	Charge to Practice	40	Void and reserved. Charge to practice.
24	Diagnostic Serv Sect ID	10	Void and reserved. Diagnosis ID.
25	Result Status	1	Void and reserved. Status of result.
26	Parent Result	200	Void and reserved. Parent result.
27	Quantity/Timing	200	Void and reserved. Quantity/time.
28	Result Copies To	150	Void and reserved. Result copies to.
29	Parent	150	Void and reserved. Parent order.
30	Transportation Mode	20	Void and reserved. Transportation mode.
31	Reason for Study	300	Void and reserved. Reason for study.
32	Principal Result Interpreter	200	Void and reserved. Principal result interpreter.
33	Assistant Result Interpreter	200	Void and reserved. Assistant result interpreter.
34	Technician	200	Void and reserved. Technician.
35	Transcriptionist	200	Void and reserved. Transcriptionist.
36	Scheduled Date/Time	26	Void and reserved. Scheduled date/time.
37	Number of Sample Containers	4	Void and reserved. Number of sample containers.
38	Transport Logistics of Collected Sample	60	Void and reserved. Transport logistics of collected sample.
39	Collector's Comment	200	Void and reserved. Collector's comment.
40	Transport Arrangement Responsibility	60	Void and reserved. Transport arrangement responsibility.

No.	Field	Length	Description
41	Transport Arranged	30	Void and reserved. Transport arranged.
42	Escort Required	1	Void and reserved. Escort required.
43	Planned Patient Transport Comment	200	Void and reserved. Planned patient transport comment.
44	Ordering Facility Name	60	Void and reserved. Name of placer.
45	Ordering Facility Address	106	Void and reserved. Address of placer.
46	Ordering Facility Phone Number	48	Void and reserved. Phone number of placer.
47	Ordering Provider Address	106	Void and reserved. Address of provider.

Comments: OBR segment only applies to ORU^R01 message. Fields 1, 3 and 37 are integers; field 9 is a floating number; others are strings.

To transmit calibration result (MSH-16 is 1), Mindray HL7 interface uses the following fields: (Calibration result transmission is not allowed on BS-200/BS-220/BS-120/BS-130/BS-180)

No.	Field	Length	Description
1	Set ID – OBR	10	Identifies different OBR segments.
2	Placer Order Number	22	Order number of placer, used as test No.
3	Filler Order Number	22	Order number of filler, used as test name.
4#	Universal Service ID	200	Universal service ID, set to "Manufacturer"^"Model".
5	Priority	2	STAT or not. Y for yes and N for no.
6	Requested Date/time	26	Void and reserved. Requesting date/time.
7	Observation Date/Time	26	Observation date/time, used as calibration date/time.
8	Observation End Date/Time	26	Void and reserved. Observation end date/time.
9	Collection Volume	20	Calibration rule. It includes 1-One-point linear; 1-Two-point linear; 3-Multi-point linear; 4-Logit-Log5P; 5-Exponential 5P; 6-Polynomial 5P; 7-Parabola; 8-Spline.
10	Collector Identifier	60	K factor
11	Specimen Action Code	1	Number of calibrators
12	Danger Code	60	Calibrator No.

No.	Field	Length	Description
13	Relevant Clinical Info.	300	Calibrator name
14	Specimen Received Date/Time	26	Lot No.
15	Specimen Source	300	Expiration date
16	Ordering Provider	120	Standard concentration
17	Order Callback Phone Number	40	Concentration level. High-H, Medium-M, Low-L
18	Placer Field 1	60	Response
19	Placer Field 2	60	Number of calibration parameters
20	Filler Field 1	60	Calibration value
21	Filler Field 2	60	Void and reserved.
22	Result Rpt/Status Change – Date/Time	26	Void and reserved. Result report/status change-date/time.
23	Charge to Practice	40	Void and reserved. Charge to practice.
24	Diagnostic Serv Sect ID	10	Void and reserved. Diagnosis ID.
25	Result Status	1	Void and reserved. Status of result.
26	Parent Result	200	Void and reserved. Parent result.
27	Quantity/Timing	200	Void and reserved. Quantity/time.
28	Result Copies To	150	Void and reserved. Result copies to.
29	Parent	150	Void and reserved. Parent order.
30	Transportation Mode	20	Void and reserved. Transportation mode.
31	Reason for Study	300	Void and reserved. Reason for study.
32	Principal Result Interpreter	200	Void and reserved. Principal result interpreter.
33	Assistant Result Interpreter	200	Void and reserved. Assistant result interpreter.
34	Technician	200	Void and reserved. Technician.
35	Transcriptionist	200	Void and reserved. Transcriptionist.
36	Scheduled Date/Time	26	Void and reserved. Scheduled date/time.
37	Number of Sample Containers	4	Void and reserved. Number of sample containers.
38	Transport Logistics of Collected Sample	60	Void and reserved. Transport logistics of collected sample.
39	Collector's Comment	200	Void and reserved. Collector's comment.
40	Transport Arrangement Responsibility	60	Void and reserved. Transport arrangement responsibility.

No.	Field	Length	Description
41	Transport Arranged	30	Void and reserved. Transport arranged.
42	Escort Required	1	Void and reserved. Escort required.
43	Planned Patient Transport Comment	200	Void and reserved. Planned patient transport comment.
44	Ordering Facility Name	60	Void and reserved. Name of placer.
45	Ordering Facility Address	106	Void and reserved. Address of placer.
46	Ordering Facility Phone Number	48	Void and reserved. Phone number of placer.
47	Ordering Provider Address	106	Void and reserved. Address of provider.

Comments: This segment only applies to ORU^R01 message. Fields 1, 9, 11, 19 and 37 are integers; field 10 is a floating number; others are strings. Fields 12-18 vary with the number of calibrators in the format of V1^V2^...Vi. Field 20 varies with the number of calibration parameters and is also separated by ^.

Different calibration rules have various parameters:

Linear (one-point, two-point and multi-point): K and R0;

Logit-Log4P: K, R0, a and b;

Logit-Log5P: K, R0, a, b and c;

Polynomial 5P: K, R0, a, b, c and d;

Parabola: R0, a and b;

Spline: 4*(n-1) parameters, which are R0i, ai, bi, ci. n is number of calibrators.

To transmit QC result (MSH-16 is 2), Mindray HL7 interface uses the following fields:

No.	Field	Length	Description
1	Set ID – OBR	10	Identifies different OBR segments.
2	Placer Order Number	22	Order number of placer, used as test No..
3	Filler Order Number	22	Order number of filler, used as test name.
4#	Universal Service ID	200	Universal service ID, set to "Manufacturer"^"Model".
5	Priority	2	STAT or not. Y for yes and N for no.
6	Requested Date/time	26	Requesting date/time, used as QC date/time
7	Observation Date/Time	26	Void and reserved. Observation date/time

No.	Field	Length	Description
8	Observation Date/Time End	26	Void and reserved. Observation end date/time
9	Collection Volume	20	Void and reserved
10	Collector Identifier	60	Void and reserved
11	Specimen Code Action	1	Void and reserved
12	Danger Code	60	Void and reserved
13	Relevant Clinical Info.	300	Control name
14	Specimen Received Date/Time	26	Lot No.
15	Specimen Source	300	Expiration date
16	Ordering Provider	120	Void and reserved
17	Order Callback Phone Number	40	Concentration level. High-H, Medium-M, Low-L
18	Placer Field 1	60	Mean value (mean concentration)
19	Placer Field 2	60	Standard deviation
20	Filler Field 1	60	Test result (concentration)
21	Filler Field 2	60	Unit
22	Result Rpt/Status Change – Date/Time	26	Void and reserved. Result report/status change-date/time.
23	Charge to Practice	40	Void and reserved. Charge to practice.
24	Diagnostic Serv Sect ID	10	Void and reserved. Diagnosis ID.
25	Result Status	1	Void and reserved. Status of result.
26	Parent Result	200	Void and reserved. Parent result.
27	Quantity/Timing	200	Void and reserved. Quantity/time.
28	Result Copies To	150	Void and reserved. Result copies to.
29	Parent	150	Void and reserved. Parent order.
30	Transportation Mode	20	Void and reserved. Transportation mode.
31	Reason for Study	300	Void and reserved. Reason for study.
32	Principal Result Interpreter	200	Void and reserved. Principal result interpreter.
33	Assistant Result Interpreter	200	Void and reserved. Assistant result interpreter.
34	Technician	200	Void and reserved. Technician.
35	Transcriptionist	200	Void and reserved. Transcriptionist.

No.	Field	Length	Description
36	Scheduled Date/Time	26	Void and reserved. Scheduled date/time.
37	Number of Sample Containers	4	Void and reserved. Number of sample containers.
38	Transport Logistics of Collected Sample	60	Void and reserved. Transport logistics of collected sample.
39	Collector's Comment	200	Void and reserved. Collector's comment.
40	Transport Arrangement Responsibility	60	Void and reserved. Transport arrangement responsibility.
41	Transport Arranged	30	Void and reserved. Transport arranged.
42	Escort Required	1	Void and reserved. Escort required.
43	Planned Patient Transport Comment	200	Void and reserved. Planned patient transport comment.
44	Ordering Facility Name	60	Void and reserved. Name of placer.
45	Ordering Facility Address	106	Void and reserved. Address of placer.
46	Ordering Facility Phone Number	48	Void and reserved. Phone number of placer.
47	Ordering Provider Address	106	Void and reserved. Address of provider.

Comments: This segment only applies to ORU^R01 message. Fields 1, 11 and 37 are integers; others are strings. Each QC run is transmitted in one message.

■ OBX Observation

The OBX segment transmits the observations. If sample results are to be transmitted (MSH-16 is 0)—Each patient may have multiple test results, then more than one OBX segment will be used to transmit the results. On the BS-200/BS-220/BS-120/BS-130/BS-180, all test results of a patient are transmitted separately. The HL7 interface does not check the repeatability of the test results, which should be performed by the user system.

The OBX segment of Mindray HL7 interface uses the following fields:

No.	Field	Length	Description
1	Set ID – OBX	10	Identifies different OBX segments.
2	Value Type	3	Value type, identifies the test result. NM (numeric), numeric value, for quantitative tests ST (string), for qualitative tests
3#	Observation Identifier	590	Observation identifier, used as test ID.

No.	Field	Length	Description
4	Observation Sub-ID	20	Observation Sub-ID, used as test name.
5	Observation Value	65536	Observation value, used as test result (concentration, negative(-), positive(+), weak positive(+/-), etc).
6	Units	90	Unit of test result.
7	References Range	90	Reference range for test result. It is qualitative reference for qualitative tests.
8	Abnormal Flags	5	Abnormal flag to indicate whether the test result is normal or not. User can define the flags via the data dictionary on the operation software of chemistry analyzer.
9	Probability	5	Void and reserved. Probability.
10	Nature of Abnormal Test	2	Void and reserved. Reason of abnormal test.
11#	Observe Result Status	1	Status of observation result, set to F-final results.
12	Date Last Observe Normal Values	26	Void and reserved. Date of last normal observation value.
13	User Defined Access Checks	20	User-defined access check, used as original result.
14	Date/Time of the Observation	28	Observation date/time, used as testing date/time.
15	Producer's ID	60	Void and reserved. Used as test department.
16	Responsible Observer	80	Responsible observer, used as tester.
17	Observation Method	60	Void and reserved. Observation method.

Comments: OBX segment only applies to ORU^R01 message. Fields 1, 3 and 9 are integers; fields 5 and 13 are floating numbers; others are strings.

■ QRD - query definition segment

The QRD segment of Mindray HL7 interface uses the following fields:

No.	Field	Length	Description
1#	Query Date/Time	26	Query date/time, i.e. system date/time.
2#	Query Format Code	1	Query format code, set to R (record-oriented format).
3#	Query Priority	1	Query priority, set to D (deferred).

No.	Field	Length	Description
4#	Query ID	10	Query ID, indicates different queries and increases from 1.
5	Deferred Response Type	1	Void and reserved. Deferred response type.
6	Deferred Response Date/Time	26	Void and reserved. Deferred response date/time.
7#	Quantity Limited Request	10	Quantity limited request, set to RD (records).
8#	Who Subject Filter	60	Subject filter, used as sample bar code.
9#	What Subject Filter	60	Subject filter. OTH for query and CAN for canceling
10#	What Department Data Code	60	Void and reserved. Department data code.
11	What Data Code Value Qual.	20	Void and reserved. Data code value qualifier.
12	Query Results Level	1	Void and reserved. Query results level. T for Full results

Comments: QRD segment may appear in QRY^Q02 and DSR^Q03 messages. Field 8 is bar code for real-time downloading and null for group downloading; field 4 is an integer, while others are strings.

■ QRF - query filter segment

The QRF segment is used together with the QRD segment and uses the following fields:

No.	Field	Length	Description
1#	Where Subject Filter	20	Subject address filter, set to "Model".
2	When Data Start Date/Time	26	Data start date/time, used as start receipt date/time.
3	When Data End Date/Time	26	Data end date/time, used as end receipt date/time.
4	What User Qualifier	60	Void and reserved. User qualifier.
5	Other QRY Subject Filter	60	Void and reserved. Other QRY subject filter.
6	Which Date/Time Qualifier	12	Object type. RCT(Specimen receipt date/time, receipt of specimen in filling ancillary (Lab))
7	Which Date/Time Status Qualifier	12	Object status. COR(Corrected only (no final with corrections))
8	Date/Time Selection Qualifier	12	Date/time selection qualifier. ALL(All values within the range)

No.	Field	Length	Description
9	When Quantity/Timing Qualifier	60	Void and reserved. Time interval.

Comments: QRF segment only applies to QRY^Q02 message. Fields 3 and 4 are 0 o'clock and query time of the day, and used as search conditions. All fields are strings.

■ ERR - error segment

The ERR segment adds error description to acknowledgment message and uses the following fields:

No.	Field	Length	Description
1#	Error Code and Location	80	Error code and location.

Comments: ERR segment may appear in QCK^Q02, DSR^Q03 or ACK^Q03 message. The only field of this segment is an integer.

■ QAK - query acknowledgment segment

The QAK segment includes query response information and uses the following fields:

No.	Field	Length	Description
1	Query Tag	32	Query tag, set to SR (sample request information).
2	Query Status	Response 2	Query response status: OK: Data found, no errors NF: No data found, no errors AE: Application error AR: Application reject

Comments: QAK segment applies to QCK^Q02 and DSR^Q03 messages. All fields of this segment are strings.

■ DSP - display data segment

The DSP segment displays searched sample information and patient information and uses the following fields:

No.	Field	Length	Description
1	Set ID - DSP	4	Identifies different DSP segments.
2	Display Level	4	Display level.
3#	Data Line	300	Data line, i.e. searched contents.
4	Logical Break Point	2	Logical break point.
5	Result ID	20	Result ID.

Comments: DSP segment only applies to DSR^Q03 message. Field 1 is an integer, while others are strings.

The third field "Data Line" displays the sample information downloaded from the LIS server. The sequence of the sample information is shown as follows. The bar code and test No. are required, while other items are optional.

Sequence	Data	Data Type and Value
1	Admission Number	String
2	Bed Number	String
3	Patient Name	String
4	Date of Birth	String. The format is YYYYMMDDHHmmSS, such as 20061122130540.
5	Sex	String. Male/M, Female/F, Other/O
6	Patient Alias	String. It includes O, A, B and AB.
7	Race	String, blank
8	Patient Address	String
9	County Code	String
10	Home Phone Number	String
11	Business Phone Number	String, blank
12	Primary Language	String, blank
13	Marital Status	String, blank
14	Religion	String, blank
15	Patient Account Number	String. It includes Outpatient, inpatient, other.
16	Social Security Number	String. It includes Own and Insurance.
17	Driver License Number	String
18	Ethnic Group	String
19	Birth Place	String
20	Nationality	String
21	Bar Code	String
22	Sample ID	Int
23	Sample Time	String. See item 4
24	STAT	String. It includes Y (yes), N(No) and void. N is default.
25	Collection Volume	Float, blank
26	Sample Type	String. It includes serum, plasma and urine.
27	Fetch Doctor	String
28	Fetch Department	String
29	Test Number^Test Name^Unit^Normal Range	String^string^string^string

The analyzer recognizes a test with its Test Number. For the same test, if the test number in the analyzer and that in the LIS server are not the same, you can open the ItemID.ini file in the folder where the executive file of operating software locates and

configure the test number. Only if test correspondence is set, the test results can be transmitted and sample information be downloaded.

■ **DSC - Continuation pointer segment**

The DSC segment indicates whether the data message is the last one.

No.	Field	Length	Description
1	Continuation pointer	180	Continuation pointer

Comments: DSC segment only applies to DSR^Q03 message. The only field of this segment is void when DSR^Q03 message responds to group query and not void in other conditions. This field is an integer.

3 Communication Process and Message Example

A message of HL7 protocol is the format of:

<SB> dddd <EB><CR>

Where, <SB> means the start of the message and is <VT> in ASCII, that is 0x0B.


<EB> means the end of the message and is <FS> in ASCII, that is 0x1C.

<CR> acts as acknowledgement of message end and is used to separate different messages, that is, 0x0D.

dddd means what to be transferred and includes multiple segments, each of which ends with <CR>, that is, 0x0D.

The following lines list multiple message examples of the HL7 protocol.

1. The chemistry analyzer sends test results to the LIS host by samples, that is, all tests of a sample are transferred via one message. The LIS host responses accordingly when receiving the message.

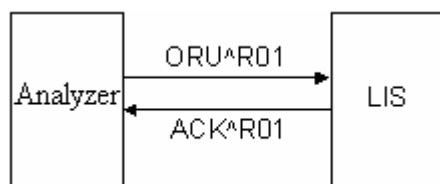

An ORU message may include the following segments: MSH, PID, OBR and OBX (multiple OBX segments may be contained if a sample has more than one test).MSH, standing for message header, is included in each message and in the format of: (The words in brackets are for explanation and not the segments)

MSH|^~\&|Corp.(Manufacturer)|product(Device model)|||20070423140610(System date/time, yyymmddhhMMss)||ORU^R01(Message type)|1(Control ID, used to identify the message and increases from 1)|P(Fixed value, means the product)|2.3.1(Version of HL7 protocol)|||0(0 for sample test result, 1 for calibration result, 2 for QC result, void for others)||ASCII(Character set)|||

There is a patient, who has the following information:

Field	Value
Name of patient	Tommy
Sex of patient	Female
Blood type	A
Birth date	July 19, 1983
Patient No.	854
Bed No.	12

Sample bar code	0000000002
Sample type	Serum
Request time	10:34:22
Sample ID	2
STAT	Yes
Test No.	2, 3 and calculation test1 ([2]+[3])
Test name	test2, test3, calctest1
Test results	5, 10 and 15
Result units	g/ml, g/ml, g/ml

The analyzer sends the test results to LIS via ORU^R01 message as follows:

```

<SB> MSH|^~\&|Manufacturer|Model||20070719145353||ORU^R01|1|P|2.3.1|||0||ASCII|||<CR>
  Corp. name Device Model System date/time Message Type HL7 Version Sample Test Result
  Message ID, which increases from 1, is unique to each message and returned unchanged in the response message.
  Product
  Character Encoding
  PID|1|854||12|Tommy||19830719145307|F|A|||||||<CR>
    Patient No. Bed No. Patient Name Birthday Gender Blood type
    OBR|1|0000000002|2|Mindray^BS-200|Y||||||serum|||||||<CR>
      Sample Barcode Sample ID is for internal use and must not be analyzed by the server Emergency Sample Type
      OBX|1|NM|2|test2|5.000000|g/ml|-|||F|||||<CR>
        Quantitative test Test No., a string, has been converted for use on the server. Test Result Result Unit
        Test name functions as a note and must not be analyzed.
  <EB> <CR>

```

```

<SB> MSH|^~\&|Manufacturer|Model||20070719145353||ORU^R01|2|P|2.3.1|||0||ASCII|||<CR>
  PID|2|854||12|Tommy||19830719145307|F|A|||||||<CR>
  OBR|1|0000000002|2|Mindray^BS-200|Y||||||serum|||||||<CR>
  OBX|1|NM|3|test3|10.000000|g/ml|-|||F|||||<CR>
  <EB> <CR>

```

```

<SB> MSH|^~\&|Manufacturer|Model||20070719145353||ORU^R01|3|P|2.3.1|||0||ASCII|||<CR>
  PID|3|854||12|Tommy||19830719145307|F|A|||||||<CR>
  OBR|1|0000000002|2|Mindray^BS-200|Y||||||serum|||||||<CR>
  OBX|1|NM|102|calctest1|15.000000|g/ml|-|||F|||||<CR>
  <EB> <CR>

```

When receiving the message, the LIS host first judges the legality and type of the message and then replies accordingly. The following is a standard reply by LIS.

<SB> MSH|^~\&|||Manufacturer|Model|20070719145307||ACK^R01|1|P|2.3.1|||0||ASCII||| <CR>

Message Type: Response of ORU

MSA|AA|1|Message accepted|||0| <CR>

Message Is received

Text information, which functions as notes.

Error code

<EB> <CR>

<SB> MSH|^~\&|||Manufacturer|Model|20070719145307||ACK^R01|2|P|2.3.1|||0||ASCII||| <CR>

MSA|AA|2|Message accepted|||0| <CR>

<EB> <CR>

<SB> MSH|^~\&|||Manufacturer|Model|20070719145308||ACK^R01|3|P|2.3.1|||0||ASCII||| <CR>

MSA|AA|3|Message accepted|||0| <CR>

<EB> <CR>

If error is included in the ORU message, it can be returned in the MSA segment, and the analyzer will handle it properly and trigger alarms. When a reject error of 206 occurs on the LIS host, the ACK message for reply is as follows:

<SB> MSH|^~\&|||Manufacturer|Model|20070719145307||ACK^R01|1|P|2.3.1|||0||ASCII||| <CR>

Message Type: Response of ORU

MSA|AR|1|Application record locked|||206| <CR>

Message Is rejected

Text information, which functions as notes.

Error code

<EB> <CR>

2. The chemistry analyzer sends QC test results to the LIS host. On the BS-200/BS-220/BS-120/BS-130/BS-180, each QC test result is sent via one message.

For example: A QC test is requested as follows.

Field	Value
Test No.	1
Test name	test1
Control name	QUAL1, QUAL2
Lot No. of control	1111, 2222
Expiration date of control	July 20, 2008, July 20, 2008
Concentration level of control	High (H) , Middle (M)
Mean value (mean concentration)	5, 8

<SB> MSH|^~\&|Manufacturer|Model||20070723170707||QRY^Q02|1|P|2.3.1|||||ASCII|||<CR>
 QRD|20070723170707|R|D|1||RD|34567743|OTH||T|<CR>
 QRY Time QRY Format Code QRY Priority Quantity Limited Request Sample Barcode What Subject Filter
 QRF|BS-200|20070723170749|20070723170749||RCT|COR|ALL||<CR>
 Which Date/Time Qualifier Which Date/Time Status Qualifier Date/Time Selection Qualifier
 <EB> <CR>

When receiving the message, the LIS returns the QCK^Q02 message and replies as follows if the sample of the bar code exists:

<SB> MSH|^~\&|||Manufacturer|Model|20070723170707||QCK^Q02|1|P|2.3.1|||||ASCII|||<CR>
 MSA|AA|1|Message accepted|||0|<CR>
 ERR|0|<CR>
 Error Code and Location
 QAK|SR|OK|<CR>
 Query Tag Query Response Status
 <EB> <CR>

If the sample of the bar code does not exist, the LIS replies as follows:

<SB> MSH|^~\&|||Manufacturer|Model|20070723170707||QCK^Q02|1|P|2.3.1|||||ASCII|||<CR>
 MSA|AA|1|Message accepted|||0|<CR>
 ERR|0|<CR>
 QAK|SR|NF|<CR>
 No data found
 <EB> <CR>

When the sample of the specified bar code exists on LIS, the LIS returns the QCK^Q02 message and sends the data message DSR^Q03, which contains the patient demographics, sample and test information.

Field	Value
Name of patient	Tom
Sex of patient	Male
Birth date	August 24, 1962
Patient ID	123
Bed No.	456
Sample bar code	34567743
Sample ID	3
Sample sending date&time	16:00 July 23, 2007

Sample type	Urine
Sending doctor	Mary
Sending department	ABC
Test No.	1, 3

The DSR^Q03 message is as follows:

```

<SB> MSH|^~\&|||Manufacturer|Model|20070723170707||DSR^Q03|1|P|2.3.1|||||ASCII||| <CR>
  MSA|AA|1|Message accepted|||0| <CR>
  ERR|0| <CR>
  QAK|SR|OK| <CR>
  QRD|20070723170707|R|D|1|||RD|34567743|OTH|||T| <CR>
  QRF|BS-200|20070723170749|20070723170749|||RCT|COR|ALL|| <CR>

  DSP|1||123||| <CR>
  DSP|2||256||| <CR>
  DSP|3||Tom||| <CR>
  DSP|4||19620824000000||| <CR>
  DSP|5||M||| <CR>

```

Diagram annotations for the DSP segments:

- DSP|1||123|||**: The value **123** is annotated with **Hospital No.**
- DSP|2||256|||**: The value **256** is annotated with **Serial No.**
- DSP|3||Tom|||**: The value **Tom** is annotated with **Bed No.**
- DSP|4||19620824000000|||**: The value **19620824000000** is annotated with **Patient Name**.
- DSP|5||M|||**: The value **M** is annotated with **Birthday**.
- DSP|5||M|||**: The value **M** is annotated with **Gender**.

```

DSP|6|||<CR>
DSP|7|||<CR>
DSP|8|||<CR>
DSP|9|||<CR>
DSP|10|||<CR>
DSP|11|||<CR>
DSP|12|||<CR>
DSP|13|||<CR>
DSP|14|||<CR>
DSP|15|||<CR>
DSP|16|||<CR>
DSP|17|||<CR>
DSP|18|||<CR>
DSP|19|||<CR>
DSP|20|||<CR>
DSP|21||34567743||<CR>
DSP|22||3||<CR>
      |
      | Sample ID
      |
DSP|23||20070723160000||<CR>
      |
      | Sending
      | Time
DSP|24||N||<CR>
      |
      | Emergency
      |
DSP|25|||<CR>
DSP|26||urine||<CR>
      |
      | Sample Type
      |
DSP|27||Mary||<CR>
      |
      | Sender
      |
DSP|28||ABC||<CR>
      |
      | Sending
      | Dept.
DSP|29||1^^^||<CR>
DSP|30||3^^^||<CR>
DSC||<CR>
<EB><CR>

```

No DSR message will be sent if a QCK^Q02 message has been sent indicating no corresponding sample on LIS.

When receiving the DSR message, the analyzer replies as follows:

```

<SB> MSH|^~\&|Manufacturer|Model||20070723170707||ACK^Q03|1|P|2.3.1|||ASCII||<CR>
      MSA|AA|1|Message accepted|||0|<CR>
      ERR|0|<CR>
<EB><CR>

```

4. The chemistry analyzer sends group query request to LIS for downloading all or latest samples of the current day.

The two query modes are distinguished by the time period. See the table below.

Query Mode	Start Time	End Time
All samples of current day	0 o'clock of current day	System time when the query is sent

Latest samples of current day	End time of the latest query	System time when the query is sent
-------------------------------	------------------------------	------------------------------------

For example: A group query is sent to LIS at 17:00 on July 23, 2007 to download all samples of the current day. The query message is as follows:

```

<SB> MSH|^~\&|Manufacturer|Model|||20070320170000||QRY^Q02|1|P|2.3.1|||||ASCII||| <CR>
      QRD|20070320170000|R|D|1||RD||OTH||T| <CR>
      QRF|BS-400|20070320000000|20070320170000||RCT|COR|ALL| <CR>
<EB> <CR>

```

Time interval
(start)
Time interval
(end)

Similarly to single sample query, the LIS host replies accordingly if corresponding samples exist. If yes, the LIS host sends all qualified samples to the analyzer after returning the query reply. Each sample is transferred via a DSR message, and the DSC segment of the last DSR message is void, indicating the end of the group transfer. For example: 3 qualified samples are found on LIS and are as follows:

Field	Values of Sample 1	Values of Sample 2	Values of Sample 3
Name of patient	Jacky	Jessica	Anata
Sex of patient	Male	Female	Female
Birth date	February 16, 1972	May 12, 1983	December 12, 1979
Sample bar code	1587120	1587121	1587125
Sample ID	2	3	9
Sample type	Serum	Plasma	Urine
STAT	No	Yes	Yes
No. of included tests	1, 4	2, 3, 6	8

The DSR messages are as follows:

```
<SB> MSH|^~&||Manufacturer|Model|20070723170000||DSR^Q03|1|P|2.3.1|||||ASCII||| <CR>
MSA|AA|1|Message accepted|||0| <CR>
ERR|0| <CR>
QAK|SR|OK| <CR>
QRD|20070723170000|R|D|1||RD||OTH|||T| <CR>
QRF|BS-200|20070723000000|20070723170000|||RCT|COR|ALL|| <CR>
DSP|1||||| <CR>
DSP|2||||| <CR>
DSP|3||Jacky||| <CR>
DSP|4||19720216000000||| <CR>
DSP|5|M||| <CR>
DSP|6||||| <CR>
DSP|7||||| <CR>
DSP|8||||| <CR>
DSP|9||||| <CR>
DSP|10||||| <CR>
DSP|11||||| <CR>
DSP|12||||| <CR>
DSP|13||||| <CR>
DSP|14||||| <CR>
DSP|15||||| <CR>
DSP|16||||| <CR>
DSP|17||||| <CR>
DSP|18||||| <CR>
DSP|19||||| <CR>
DSP|20||||| <CR>
DSP|21||1587120||| <CR>
DSP|22|2||| <CR>
DSP|23||||| <CR>
DSP|24|N||| <CR>
DSP|25||||| <CR>
DSP|26|serum||| <CR>
DSP|27||||| <CR>
DSP|28||||| <CR>
DSP|29|1^^^||| <CR>
DSP|30|4^^^||| <CR>
DSC|1| <CR>
```

First DSR message of three

```
<EB> <CR>
```

```
<SB> MSH|^~&||Manufacturer|Model|20070723170000||DSR^Q03|2|P|2.3.1|||||ASCII||| <CR>
MSA|AA|2|Message accepted|||0| <CR>
ERR|0| <CR>
QAK|SR|OK| <CR>
QRD|20070723170000|R|D|2||RD||OTH|||T| <CR>
QRF|BS-200|20070723000000|20070723170000|||RCT|COR|ALL|| <CR>
DSP|1||||| <CR>
DSP|2||||| <CR>
DSP|3||Jessica||| <CR>
DSP|4||19830512000000||| <CR>
DSP|5|F||| <CR>
DSP|6||||| <CR>
DSP|7||||| <CR>
DSP|8||||| <CR>
DSP|9||||| <CR>
DSP|10||||| <CR>
DSP|11||||| <CR>
DSP|12||||| <CR>
DSP|13||||| <CR>
```


DSP|14||| <CR>
 DSP|15||| <CR>
 DSP|16||| <CR>
 DSP|17||| <CR>
 DSP|18||| <CR>
 DSP|19||| <CR>
 DSP|20||| <CR>
 DSP|21|1587121|| <CR>
 DSP|22|3|| <CR>
 DSP|23||| <CR>
 DSP|24|Y|| <CR>
 DSP|25||| <CR>
 DSP|26|plasma|| <CR>
 DSP|27||| <CR>
 DSP|28||| <CR>
 DSP|29|2^^^|| <CR>
 DSP|30|3^^^|| <CR>
 DSP|31|6^^^|| <CR>
 DSC|2| <CR>

└─ Second DSR message of three

<EB> <CR>

<SB> MSH|^~\&||Manufacturer|Model|20070723170000||DSR^Q03|3|P|2.3.1||||ASCII|| <CR>
 MSA|AA|3|Message accepted|||0| <CR>
 ERR|0| <CR>
 QAK|SR|OK| <CR>
 QRD|20070723170000|R|D|3||RD||OTH||T| <CR>
 QRF|BS-200|20070723000000|20070723170000||RCT|COR|ALL|| <CR>
 DSP|1||| <CR>
 DSP|2||| <CR>
 DSP|3|Anata|| <CR>
 DSP|4|19791212000000|| <CR>
 DSP|5|F|| <CR>
 DSP|6||| <CR>
 DSP|7||| <CR>
 DSP|8||| <CR>
 DSP|9||| <CR>
 DSP|10||| <CR>
 DSP|11||| <CR>
 DSP|12||| <CR>
 DSP|13||| <CR>
 DSP|14||| <CR>
 DSP|15||| <CR>
 DSP|16||| <CR>
 DSP|17||| <CR>
 DSP|18||| <CR>
 DSP|19||| <CR>
 DSP|20||| <CR>
 DSP|21|1587125|| <CR>
 DSP|22|9|| <CR>
 DSP|23||| <CR>
 DSP|24|Y|| <CR>
 DSP|25||| <CR>
 DSP|26|urine|| <CR>
 DSP|27||| <CR>
 DSP|28||| <CR>
 DSP|29|8^^^|| <CR>

DSC||<CR>
 Third DSR message of the three. Void means the end of multiple-sample transferring
 <EB> <CR>

The analyzer sends back an ACK message to LIS every time when receiving a DSR message. The ACK messages for the above-mentioned DSR messages are:

<SB> MSH|^~\&|Manufacturer|Model|||20070723170000||ACK^Q03|1|P|2.3.1|||ASCII||| <CR>
 MSA|AA|1|Message accepted|||0| <CR>
 ERR|0| <CR>
 <EB> <CR>

<SB> MSH|^~\&|Manufacturer|Model|||20070723170000||ACK^Q03|2|P|2.3.1|||ASCII||| <CR>
 MSA|AA|2|Message accepted|||0| <CR>
 ERR|0| <CR>
 <EB> <CR>

<SB> MSH|^~\&|Manufacturer|Model|||20070723170000||ACK^Q03|2|P|2.3.1|||ASCII||| <CR>
 MSA|AA|2|Message accepted|||0| <CR>
 ERR|0| <CR>
 <EB> <CR>

5. During group query, the chemistry analyzer sends a message to LIS to cancel the query/downloading.

The QRY message is used as follows:

<SB> MSH|^~\&|Manufacturer|Model|||20070723170000||QRY^Q02|1|P|2.3.1|||ASCII||| <CR>
 QRD|20070723170000|R|D|1||RD||CAN|||T| <CR>
 QRF|BS-400|20070723000000|20070723170000|||RCT|COR|ALL|| <CR>
 <EB> <CR>

When receiving the QRY message of cancel, the LIS host stops its operation after sending the current sample.

