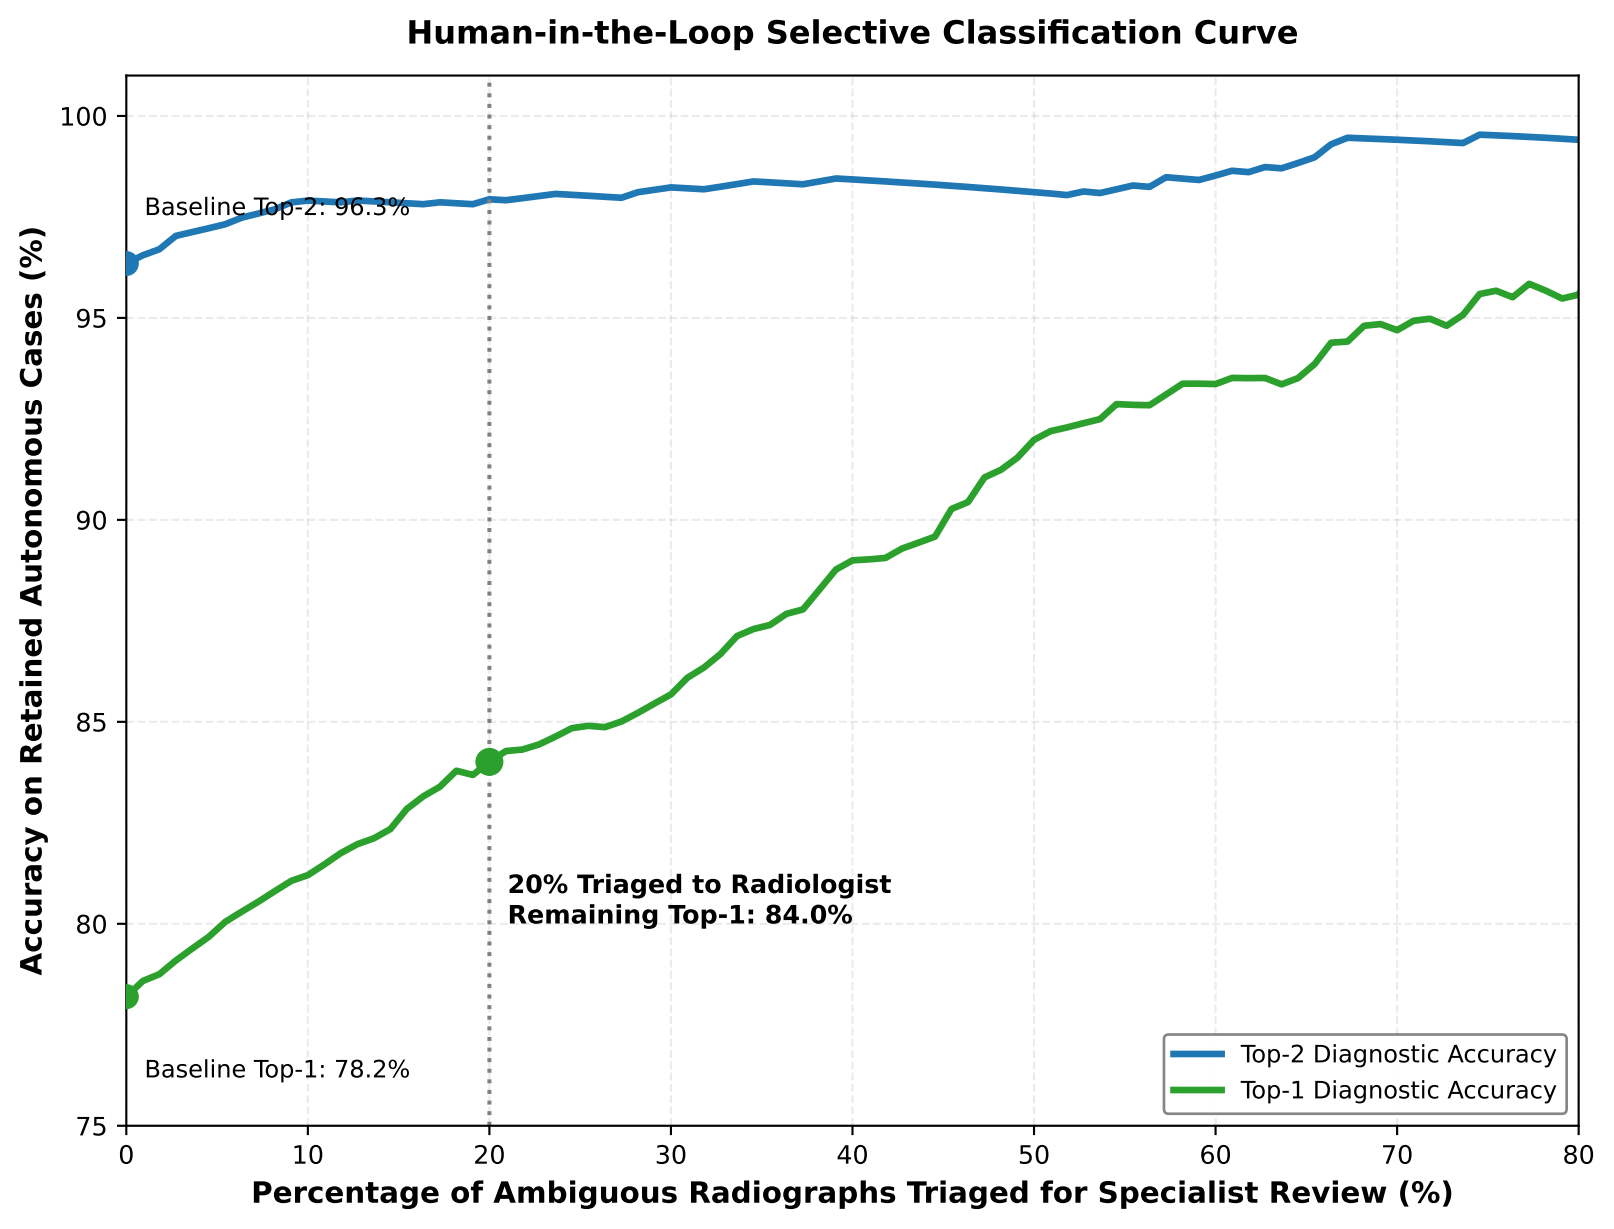
Human-in-the-Loop Selective Classification Curve
Accuracy on Retained Autonomous Cases (%)
Percentage of Ambiguous Radiographs Triaged for Specialist Review (%)
100
95
90
85
80
75
0
10
20
30
40
50
60
70
80
Baseline Top-2: 96.3%
Baseline Top-1: 78.2%
20% Triaged to Radiologist
Remaining Top-1: 84.0%
Top-2 Diagnostic Accuracy
Top-1 Diagnostic Accuracy