



Si 4³: central pump-probe at 1.94 fs; fixed alpha=0.2, gamma=0.004 for TDCDFT


HSE06

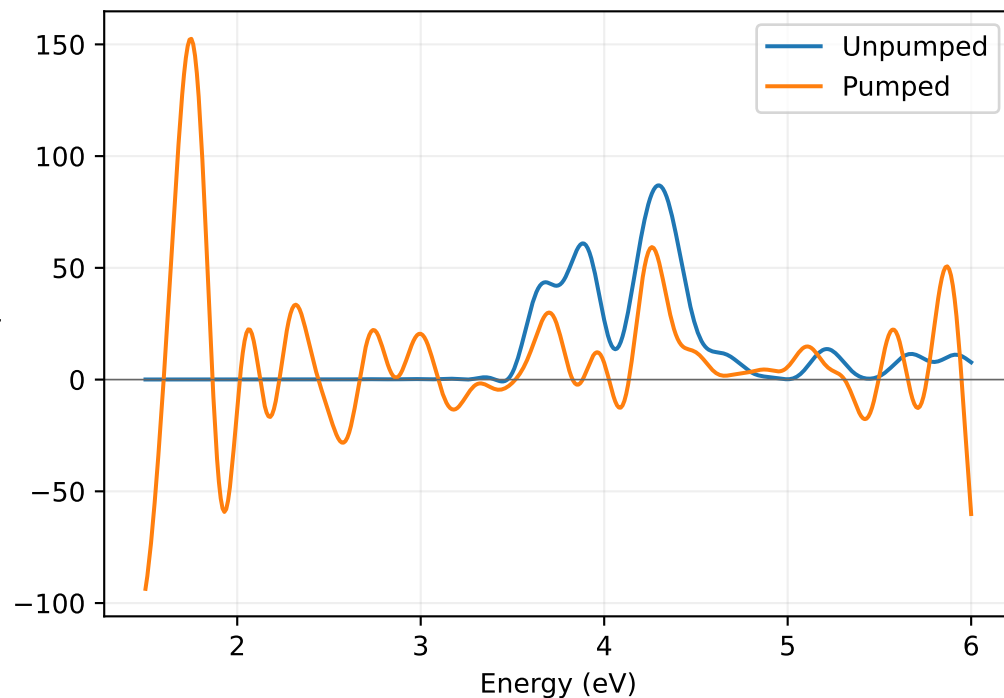

HSE06

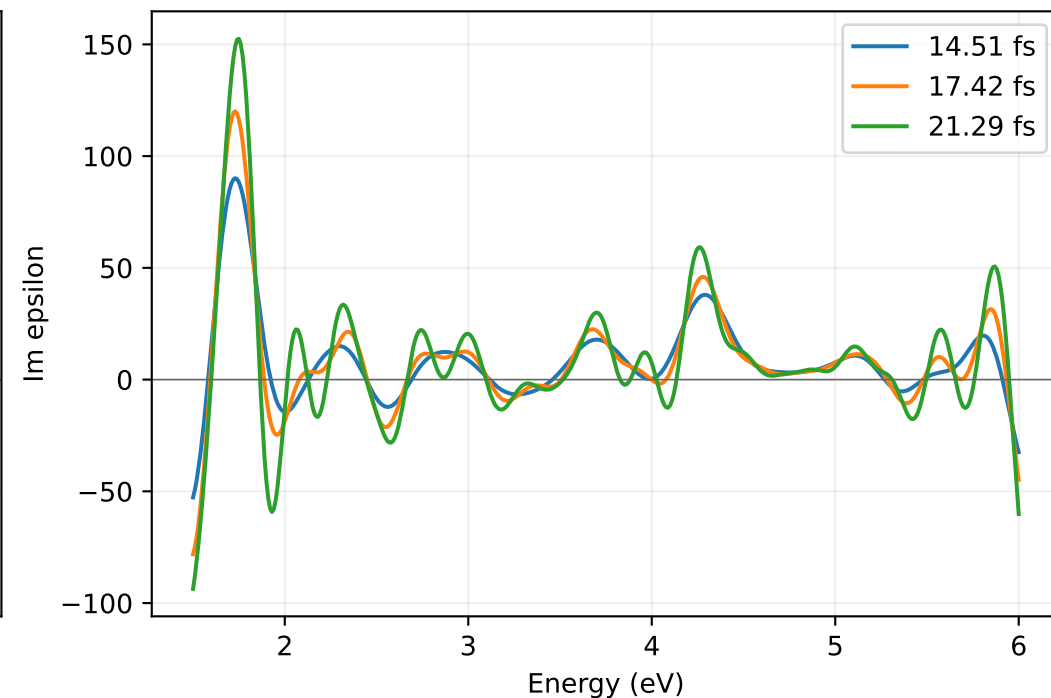

TDCDFT

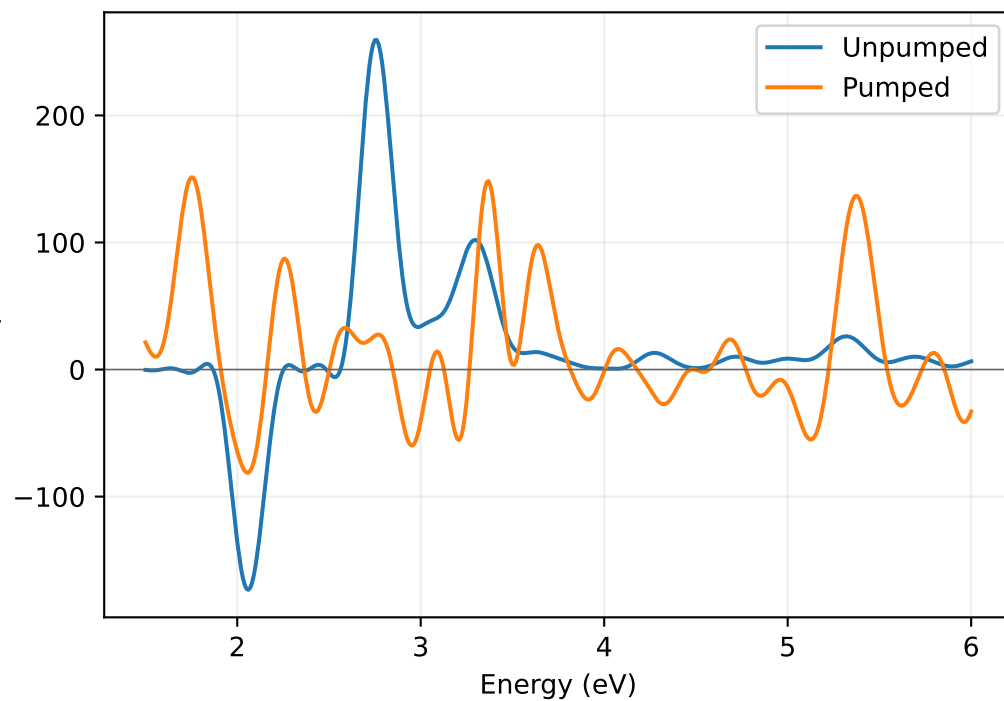

TDCDFT

