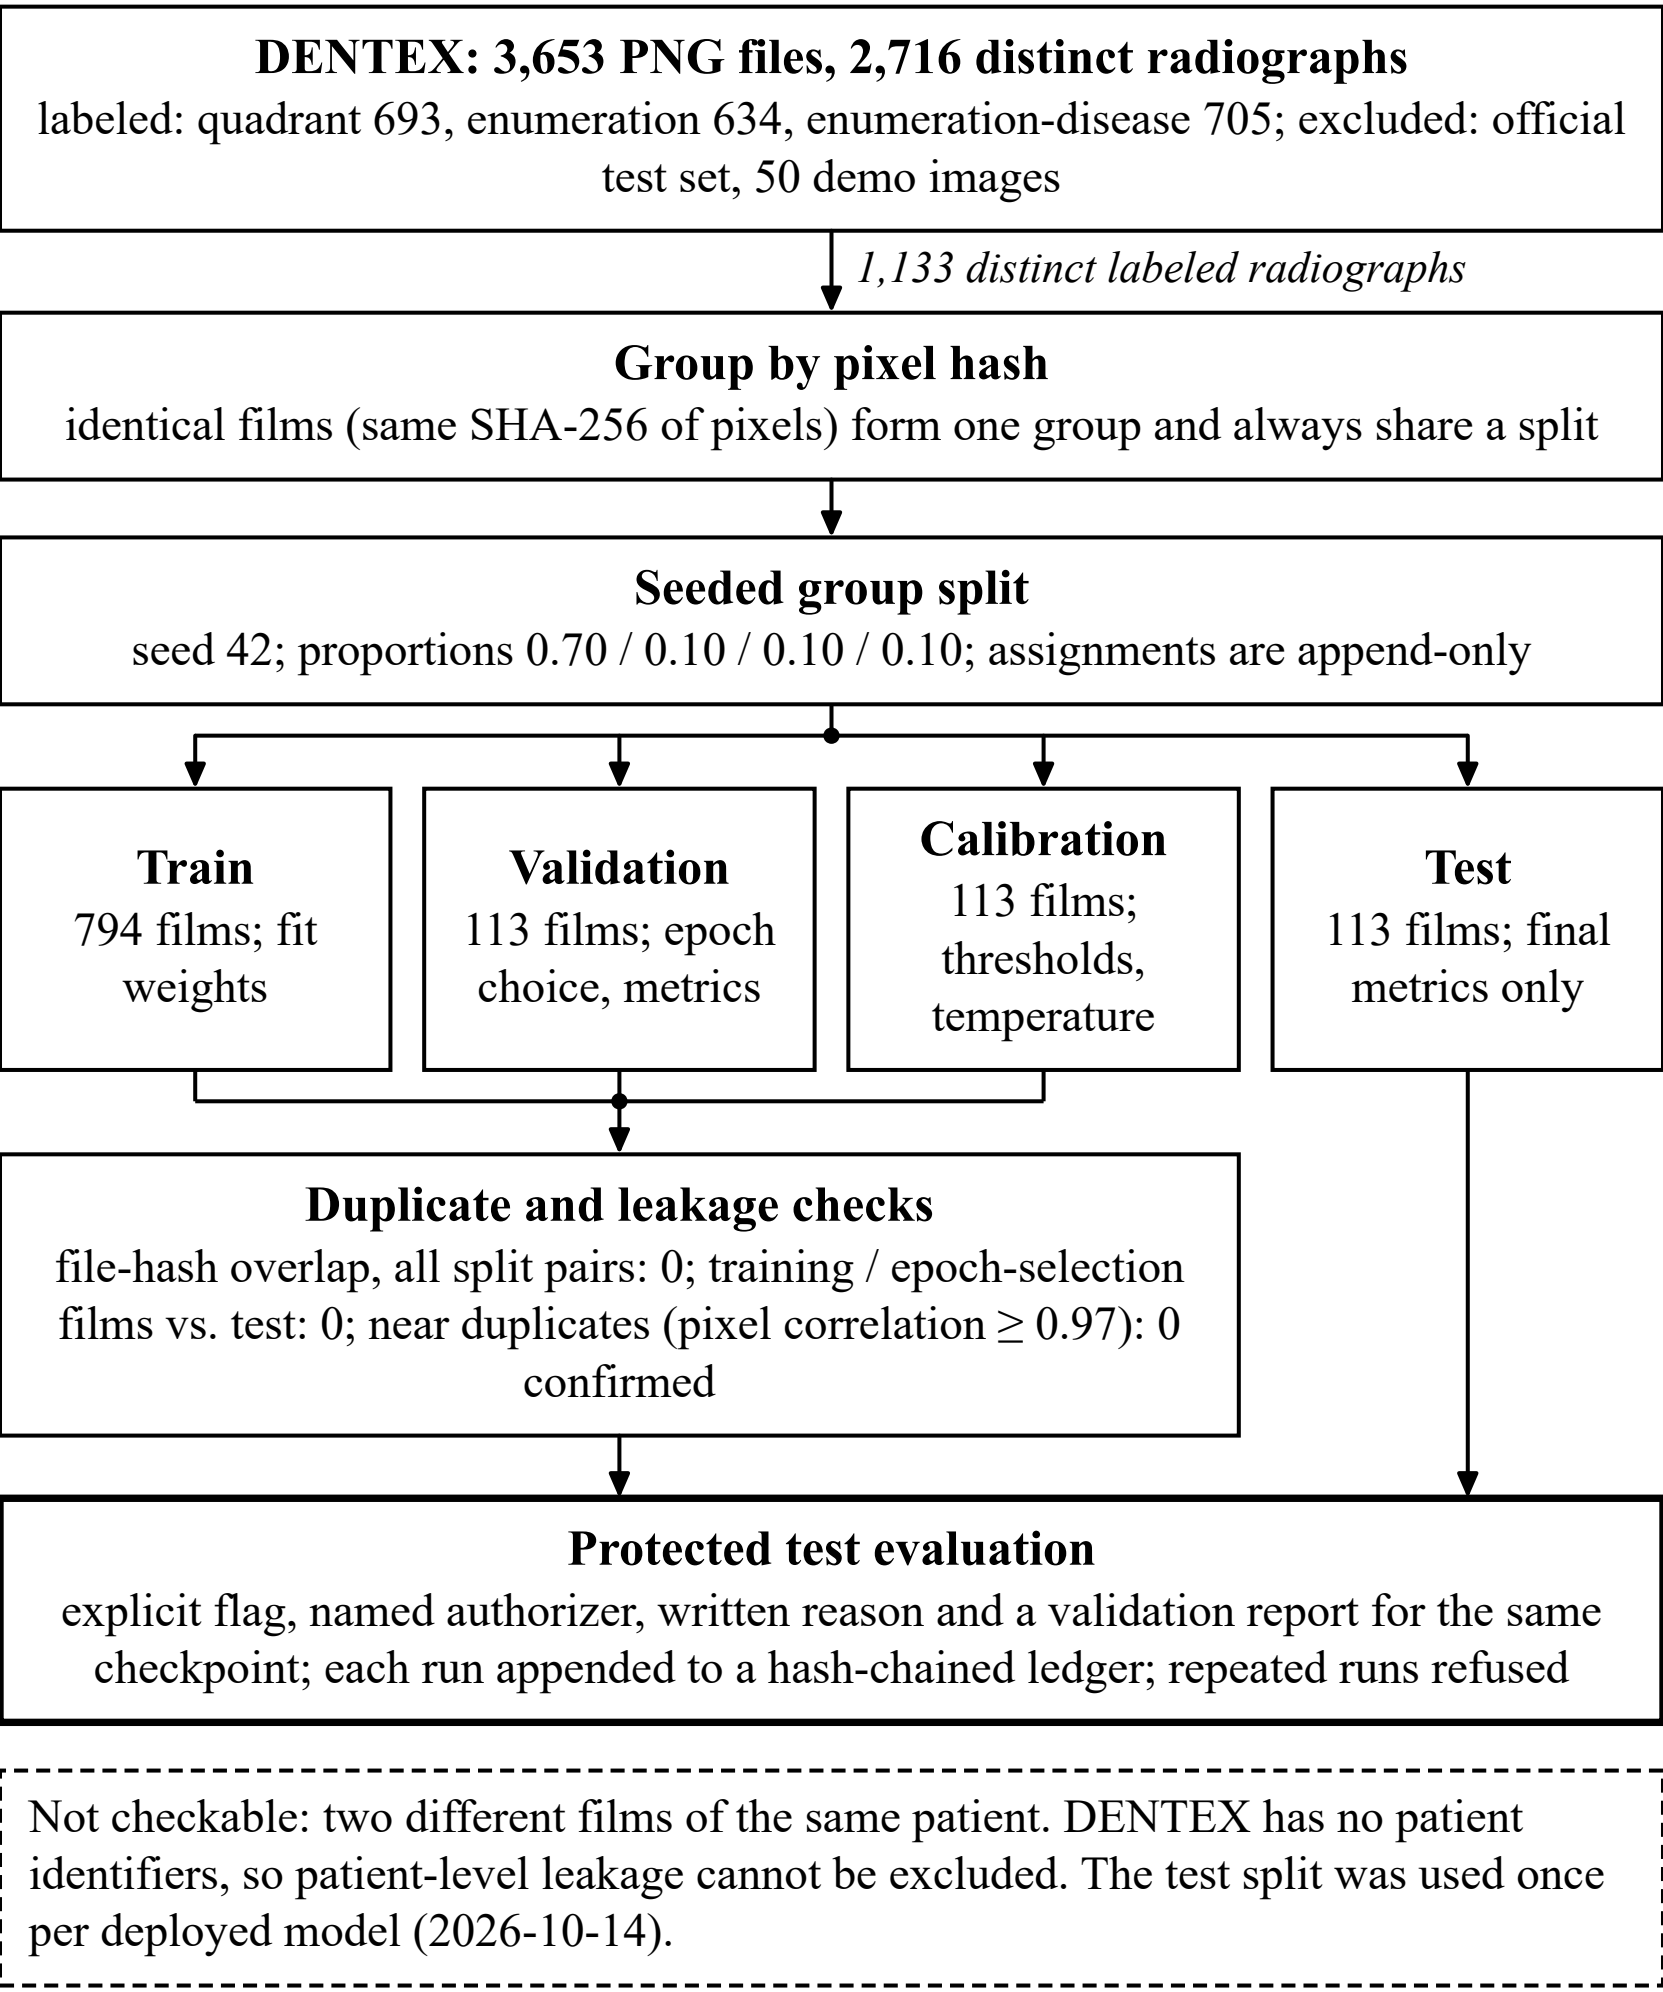

DENTEX: 3,653 PNG files, 2,716 distinct radiographs
labeled: quadrant 693, enumeration 634, enumeration-disease 705; excluded: official test set, 50 demo images
1,133 distinct labeled radiographs
Group by pixel hash
identical films (same SHA-256 of pixels) form one group and always share a split
Seeded group split
seed 42; proportions 0.70 / 0.10 / 0.10 / 0.10; assignments are append-only
Train
794 films; fit weights
Validation
113 films; epoch choice, metrics
Calibration
113 films; thresholds, temperature
Test
113 films; final metrics only
Duplicate and leakage checks
file-hash overlap, all split pairs: 0; training / epoch-selection films vs. test: 0; near duplicates (pixel correlation ≥ 0.97): 0 confirmed
Protected test evaluation
explicit flag, named authorizer, written reason and a validation report for the same checkpoint; each run appended to a hash-chained ledger; repeated runs refused
Not checkable: two different films of the same patient. DENTEX has no patient identifiers, so patient-level leakage cannot be excluded. The test split was used once per deployed model (2026-10-14).