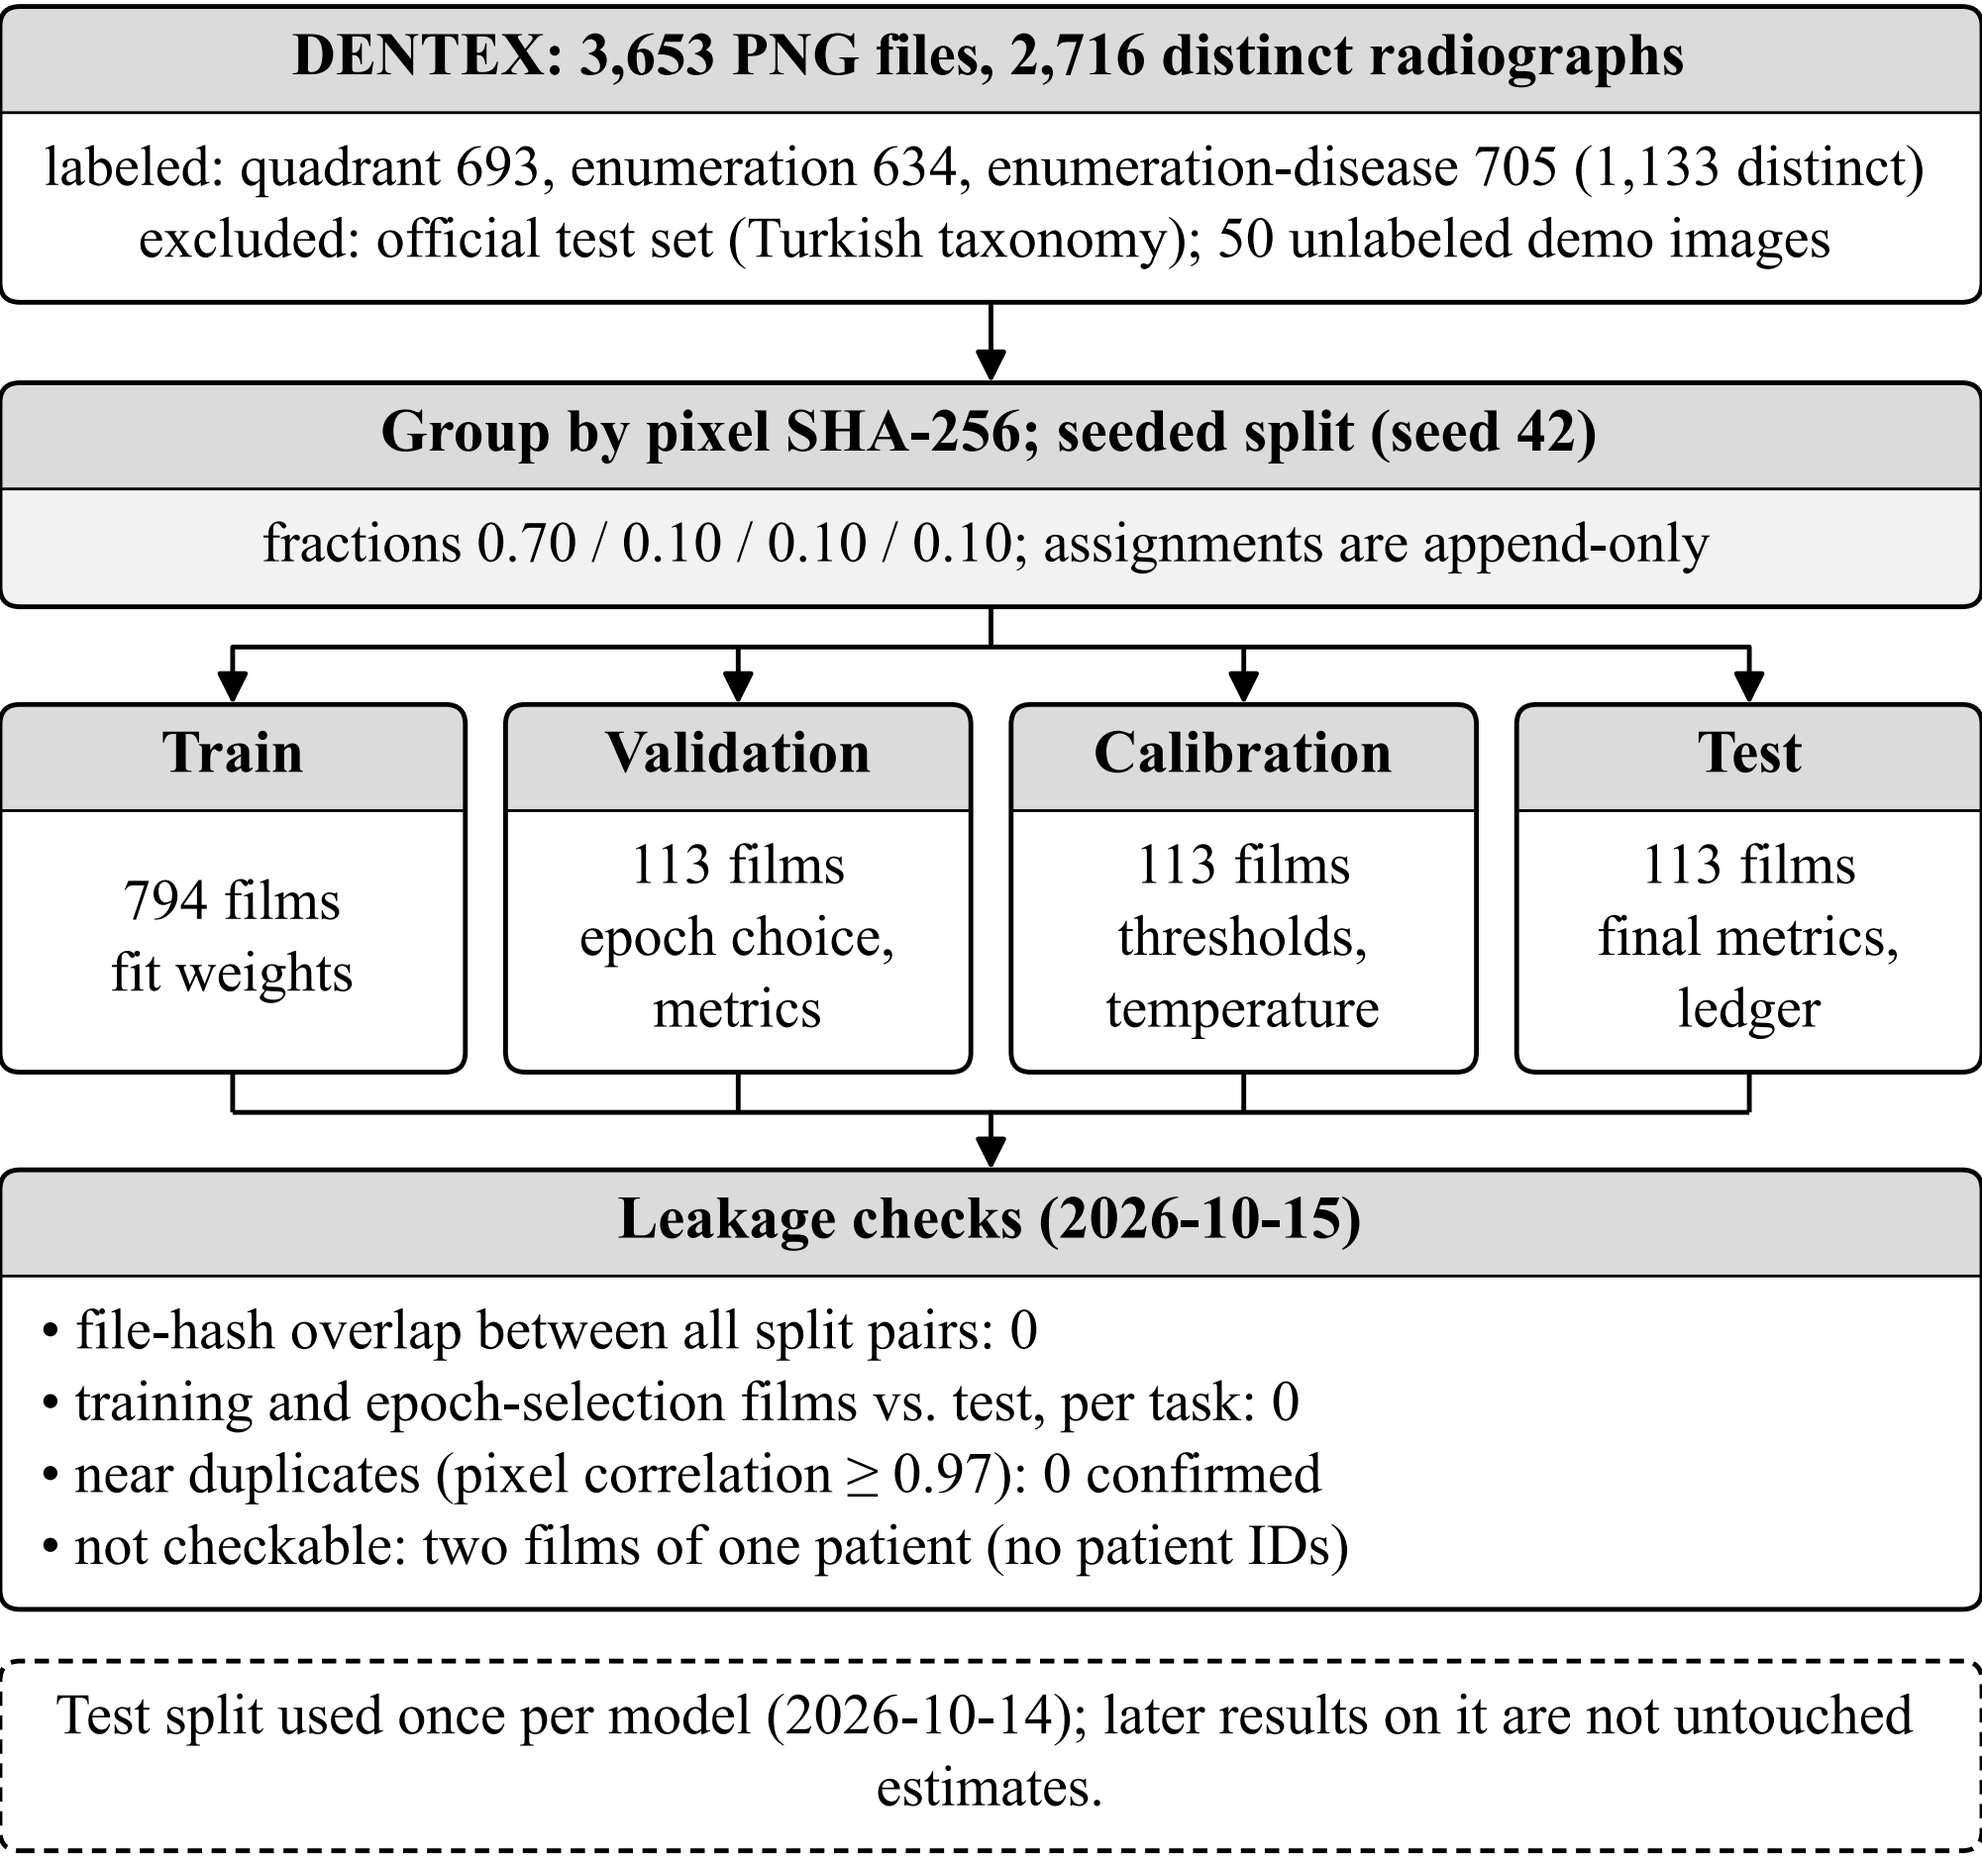

DENTEX: 3,653 PNG files, 2,716 distinct radiographs
labeled: quadrant 693, enumeration 634, enumeration-disease 705 (1,133 distinct)
excluded: official test set (Turkish taxonomy); 50 unlabeled demo images
Group by pixel SHA-256; seeded split (seed 42)
fractions 0.70 / 0.10 / 0.10 / 0.10; assignments are append-only
Train
794 films
fit weights
Validation
113 films
epoch choice,
metrics
Calibration
113 films
thresholds,
temperature
Test
113 films
final metrics,
ledger
Leakage checks (2026-10-15)
• file-hash overlap between all split pairs: 0
• training and epoch-selection films vs. test, per task: 0
• near duplicates (pixel correlation ≥ 0.97): 0 confirmed
• not checkable: two films of one patient (no patient IDs)
Test split used once per model (2026-10-14); later results on it are not untouched estimates.