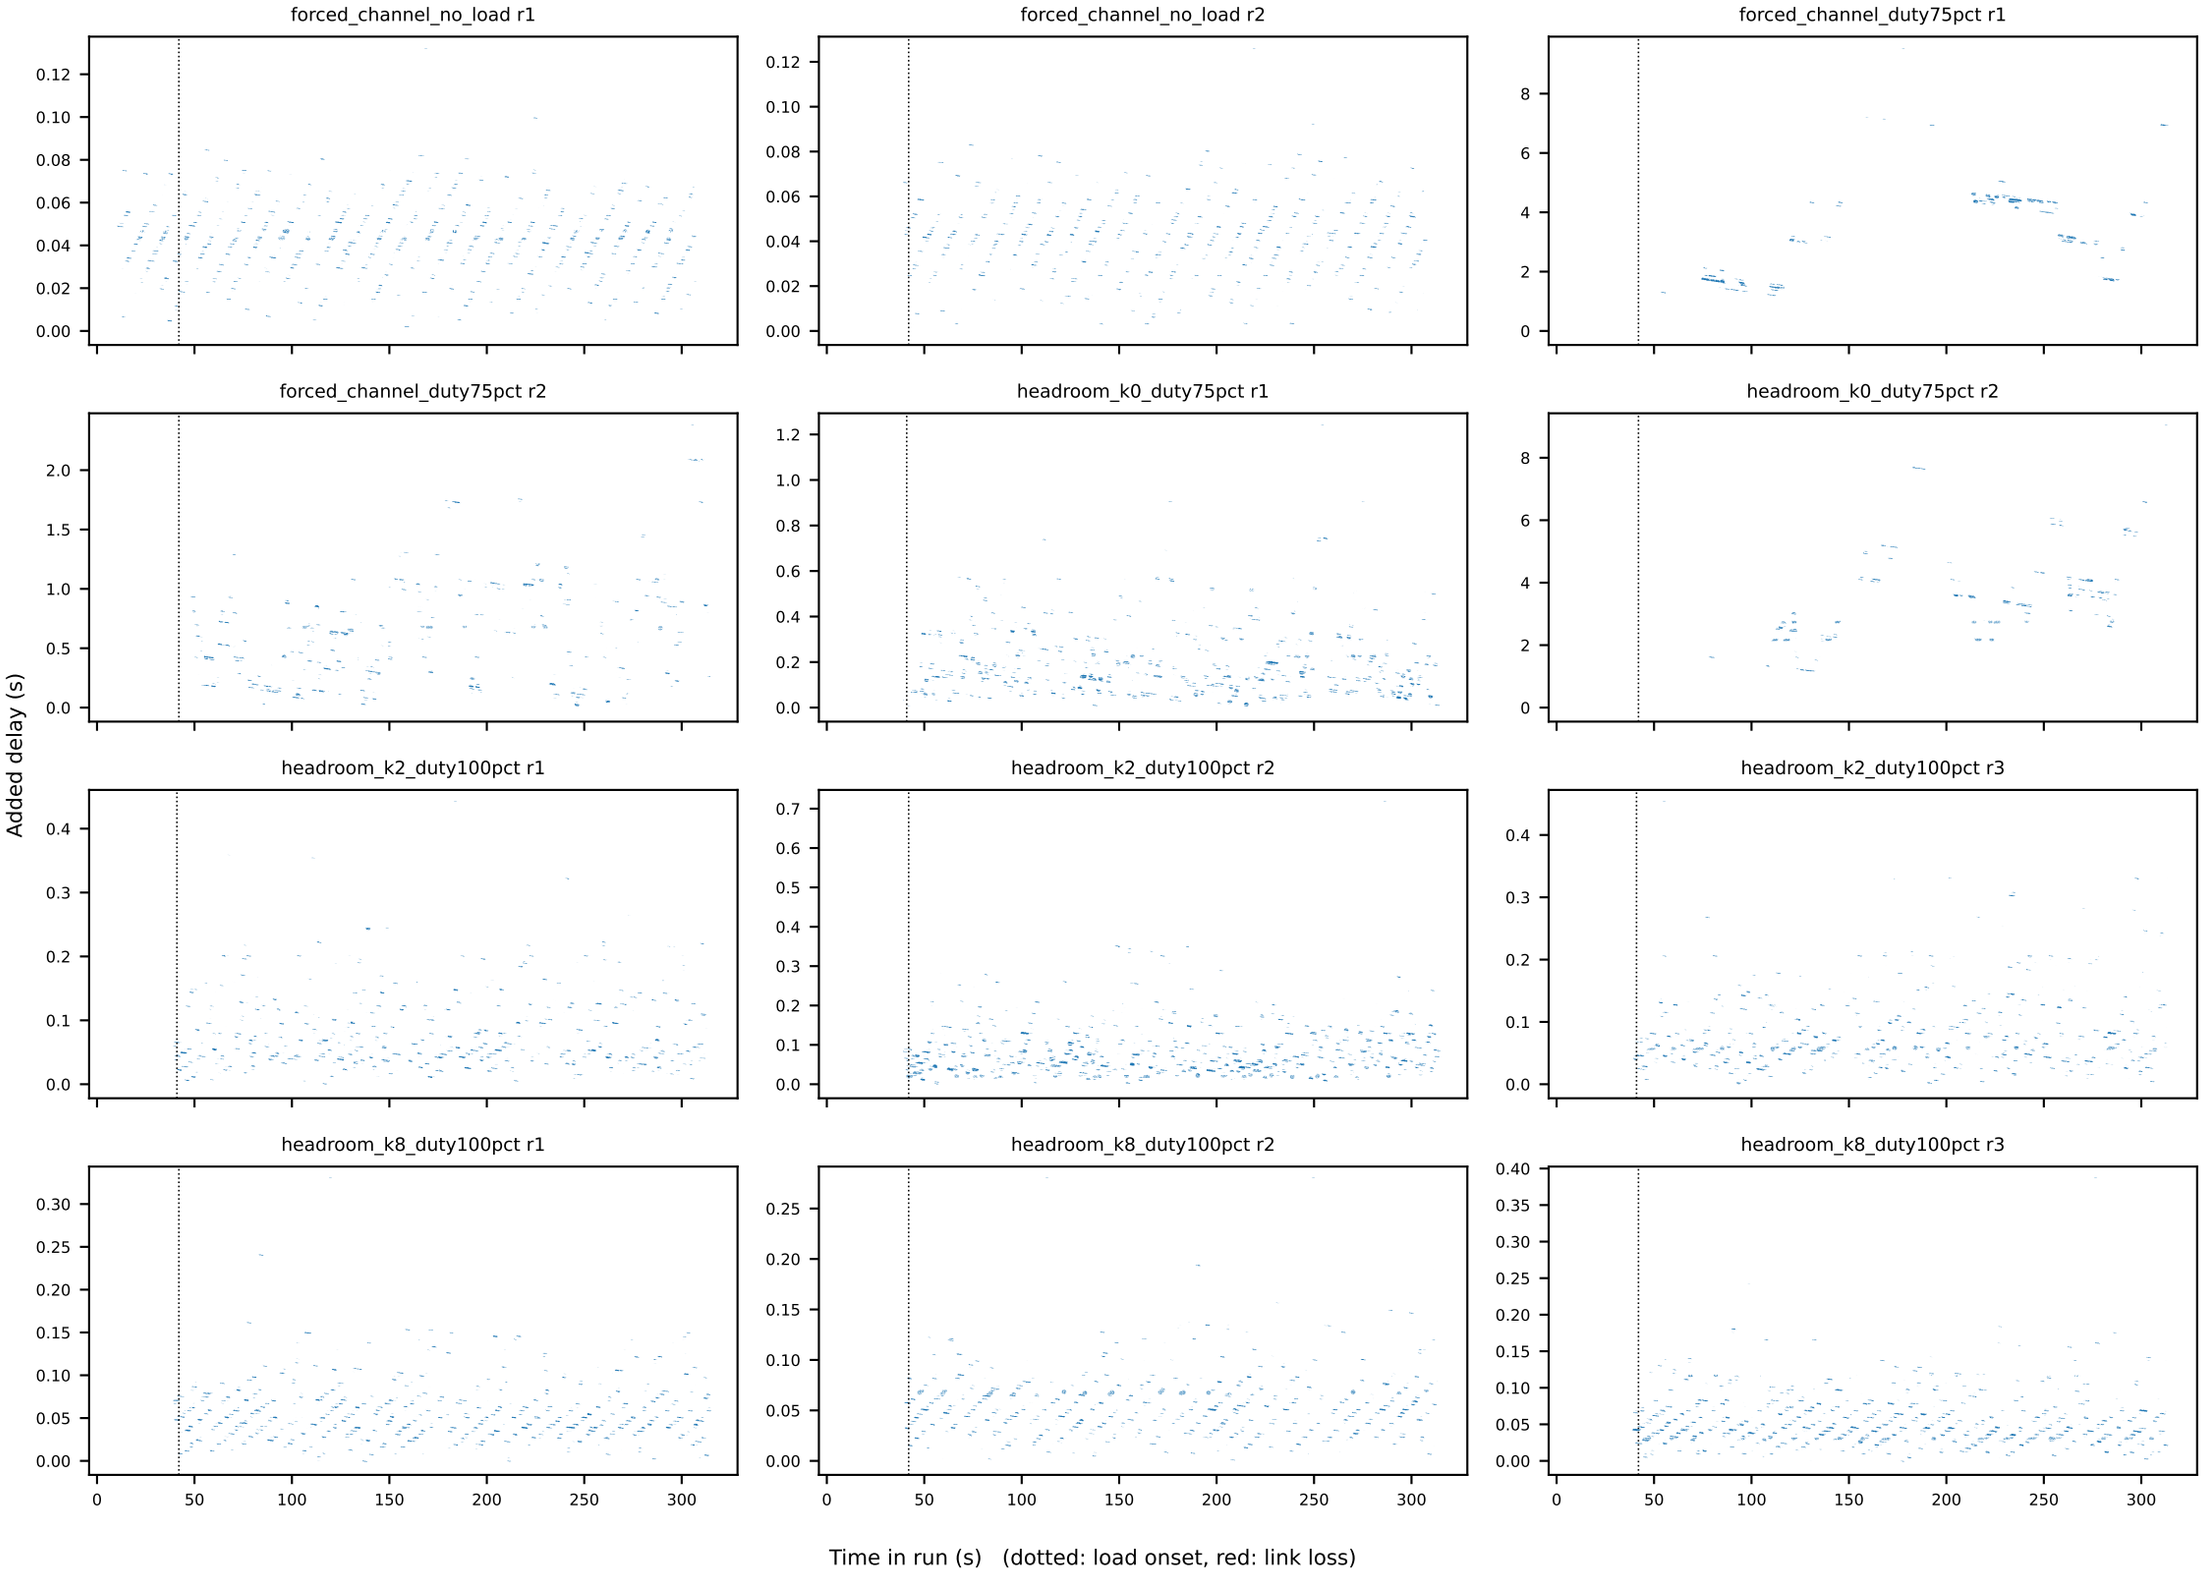

20261008_010249_chamber_2: Polar ECG delay per run
forced_channel_no_load r1
forced_channel_no_load r2
forced_channel_duty75pct r1
forced_channel_duty75pct r2
headroom_k0_duty75pct r1
headroom_k0_duty75pct r2
headroom_k2_duty100pct r1
headroom_k2_duty100pct r2
headroom_k2_duty100pct r3
headroom_k8_duty100pct r1
headroom_k8_duty100pct r2
headroom_k8_duty100pct r3
Added delay (s)
Time in run (s) (dotted: load onset, red: link loss)