Step 3 | Feature engineering ablation

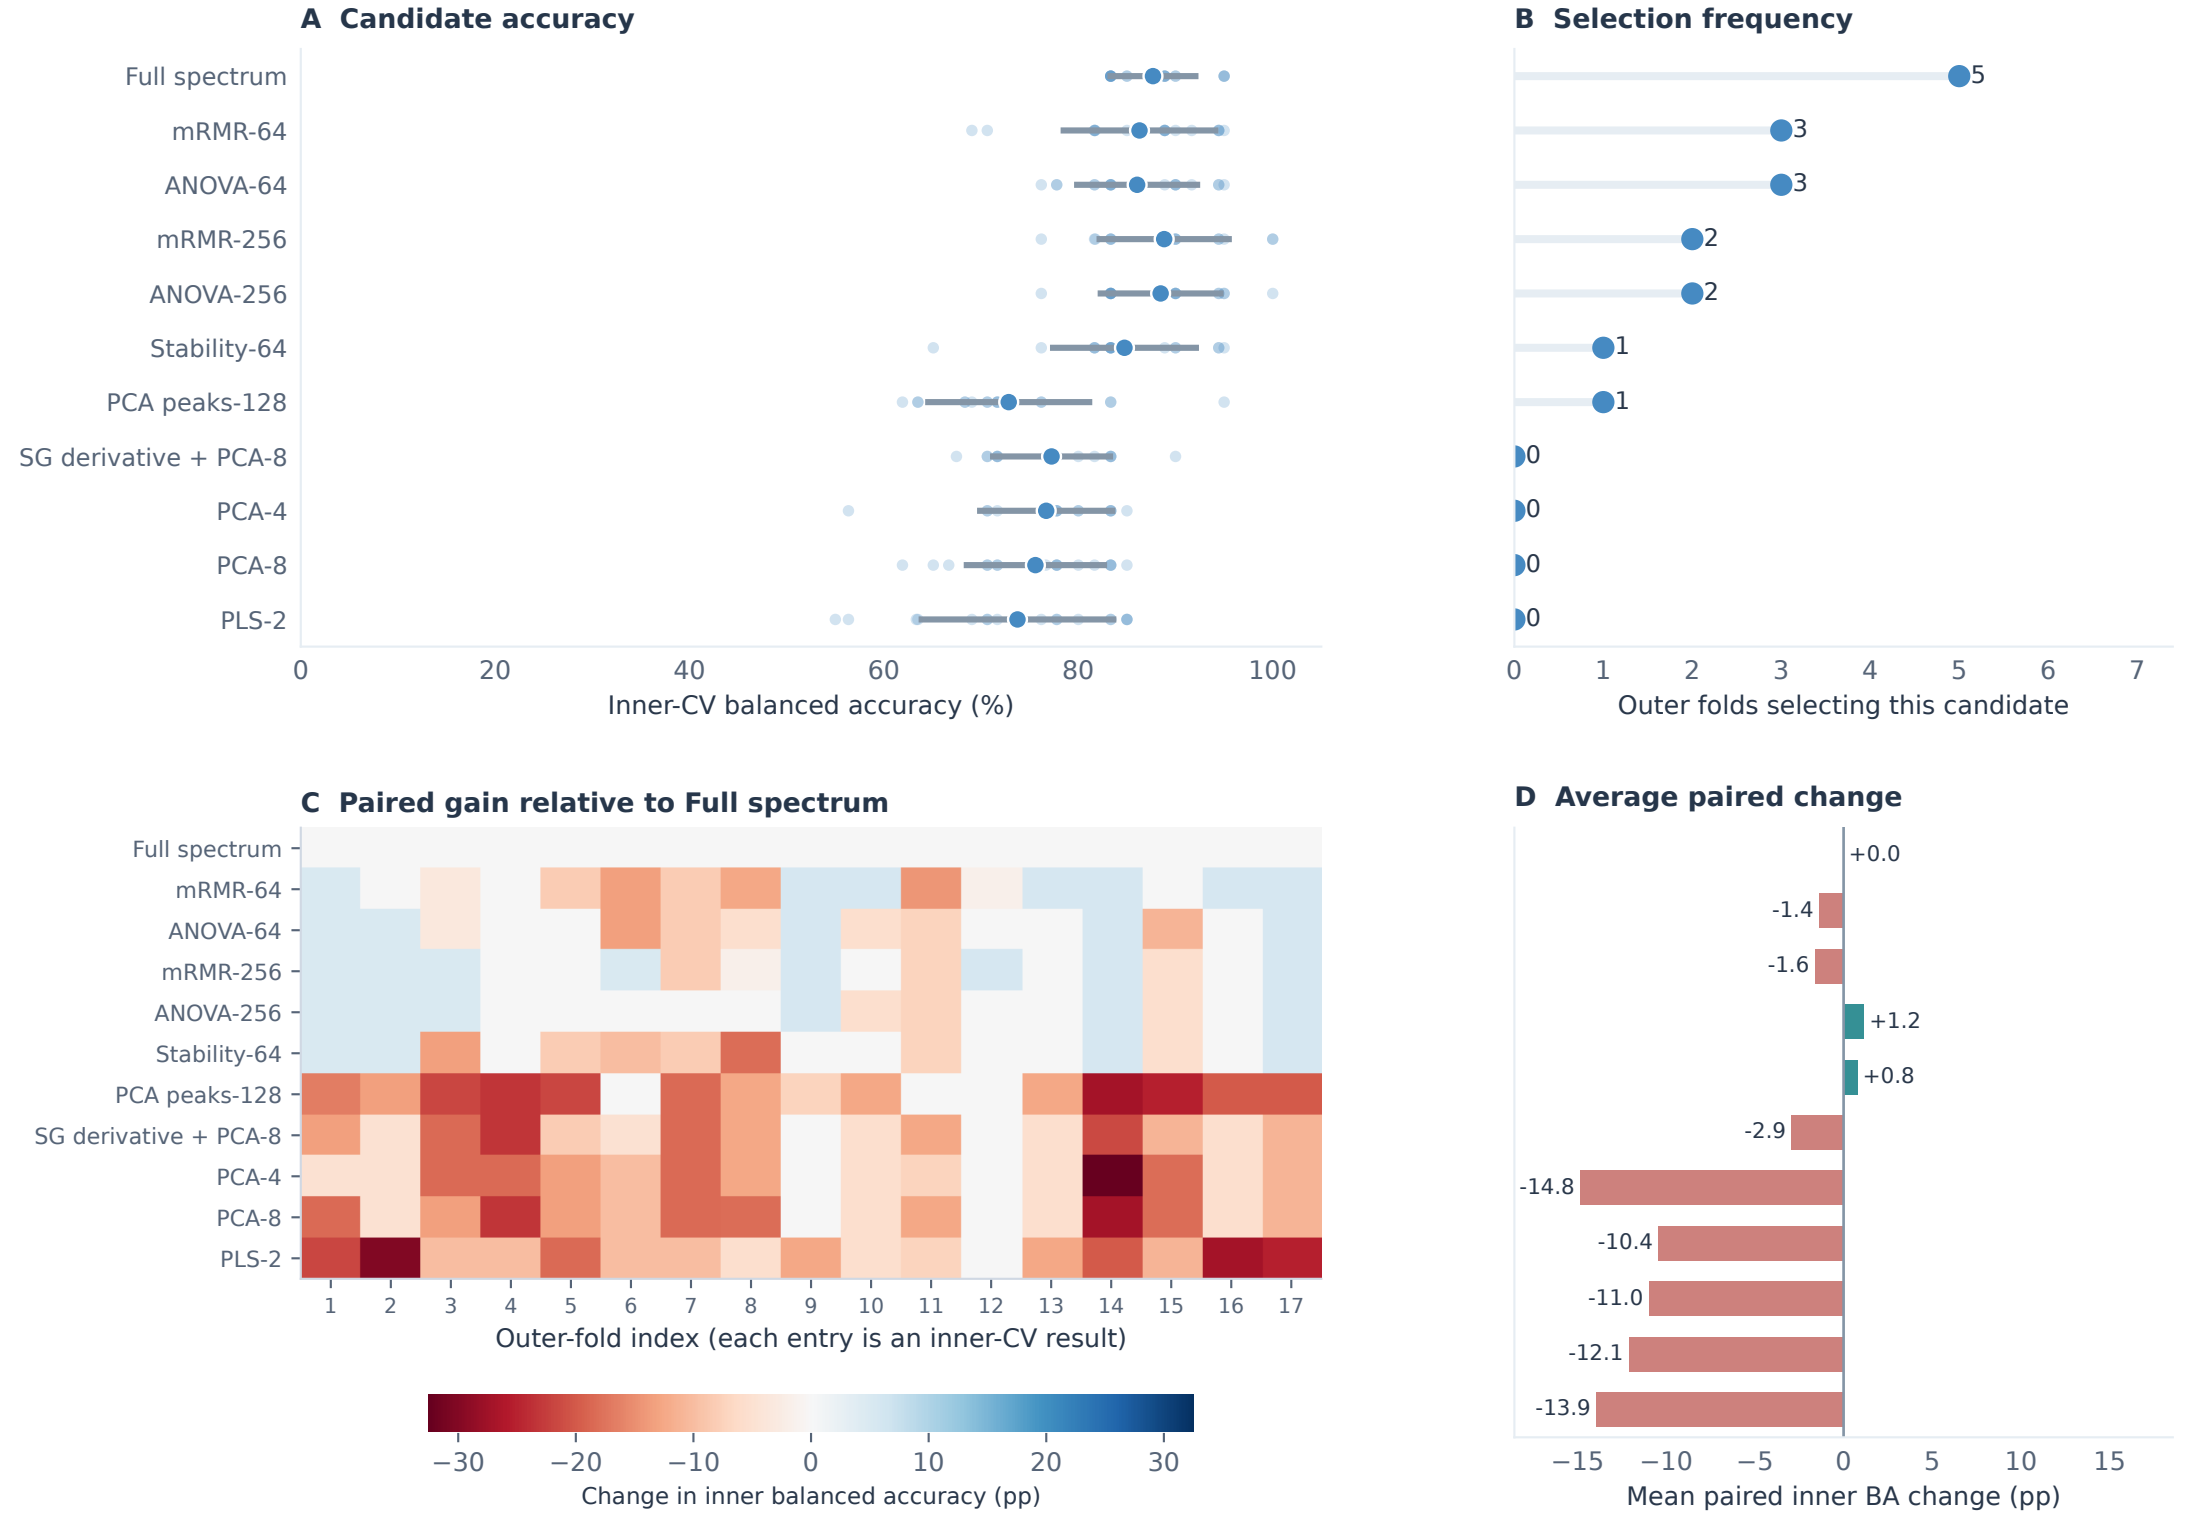

Descriptive inner cross-validation summaries; the selected candidate is refitted before the outer patient is evaluated.