


Aprosoft LFE-Labor

Project I-G
Material 50 hydrogel
Sample 1
Atmosphere vacuum

Temp in °C 24
Measnr 1113
Thickness in 0.4000
I-G_1__50 hydrogel_1_771.lf

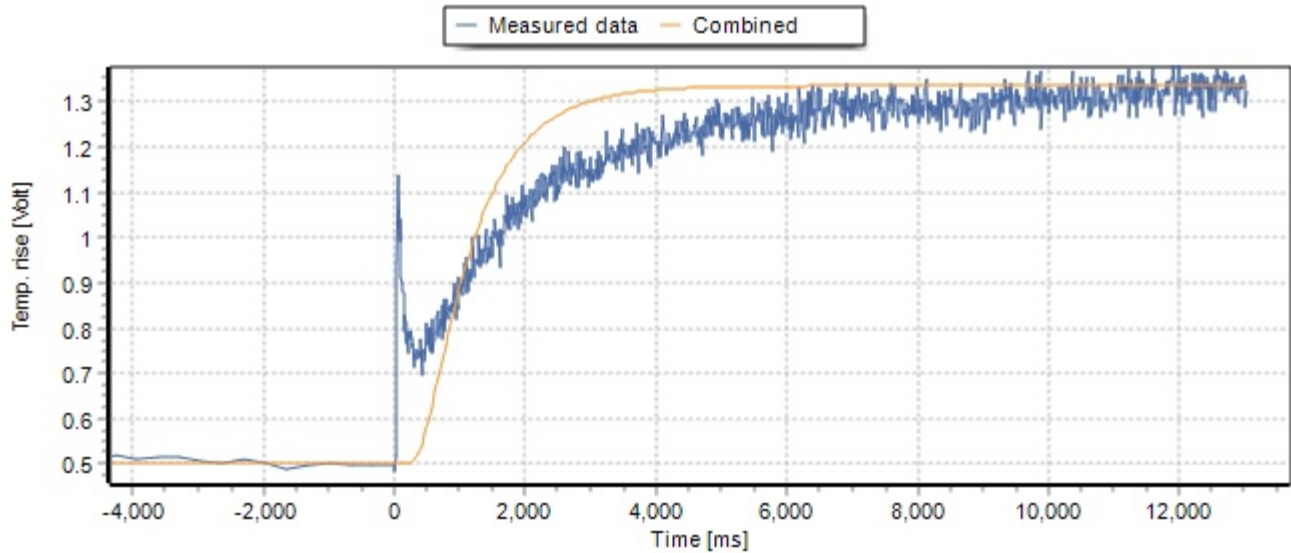

Details

Duration in s 13.0221
Max. in V 1.34
Min. in V 0.5
Halftime in ms 1135.507
Min.type Baseline
Remark

Pulse in ms

Length 0.0500
Type Tri
Trapez time1 0.005
Trapez time2 0.045

Condition

Operator Nathan
Filter 0
Iris 1
Amp. 100

Adiabatic results in cm²/s

Ave. 0.0241
40 0.024
50% 0.0196
60% 0.0172

Finite Pulse in cm²/s

Dusza 0.0196
Azumi 0.0196
Clark 0.0196
Combined
Dusza 0.0211

Heatloss in cm²/s

Dusza 0.0211
Cowan 0.0166
Degiovanni 0
Taylor 0
Cowan 10 0.0194