


Aprosoft LFE-Labor

Project I-G
Material 50 hydrogel
Sample 1
Atmosphere vacuum

Temp in °C 24
Measnr 1113
Thickness in 0.4000
I-G_1__50 hydrogel_1_772.If

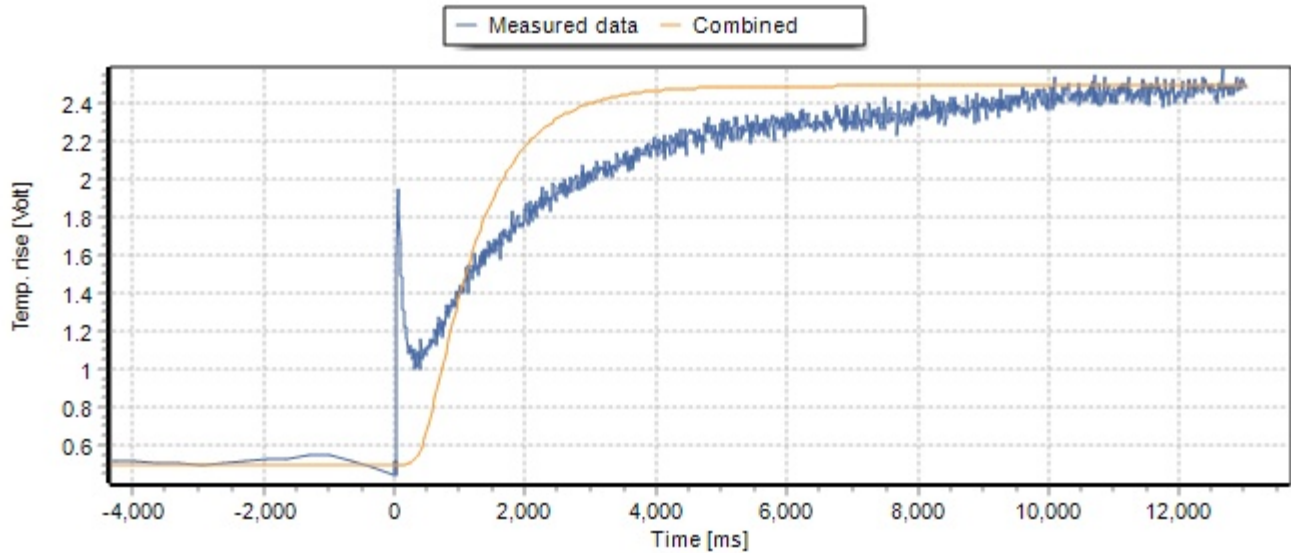

Details

Duration in s 13.0221
Max. in V 2.49
Min. in V 0.5
Halftime in ms 1149.0787
Min.type Baseline
Remark

Pulse in ms

Length 0.0500
Type Tri
Trapez time1 0.005
Trapez time2 0.045

Condition

Operator Nathan
Filter 0
Iris 1
Amp. 200

Adiabatic results in cm²/s

Ave. 0.0237
40 0.0232
50% 0.0193
60% 0.0155

Finite Pulse in cm²/s

Dusza 0.0193
Azumi 0.0193
Clark 0.0193
Combined
Dusza 0.0204

Heatloss in cm²/s

Dusza 0.0204
Cowan 0.016
Degiovanni 0.0193
Taylor 0
Cowan 10 0.0191