

**qPCR Quality Control Summary**

Technician: Seth Goodnight

Date: 2024-05-24

Sample Plate: Jekielek\_qPCR\_P02

**Instrument**

Type: QuantStudio(TM) 7 Flex System


Serial Number 278870712

Last Background check: 2024-05-17

FAM dye calibration: 2023-11-08

ROX dye calibration: 2023-11-08

**Standard Curve:**

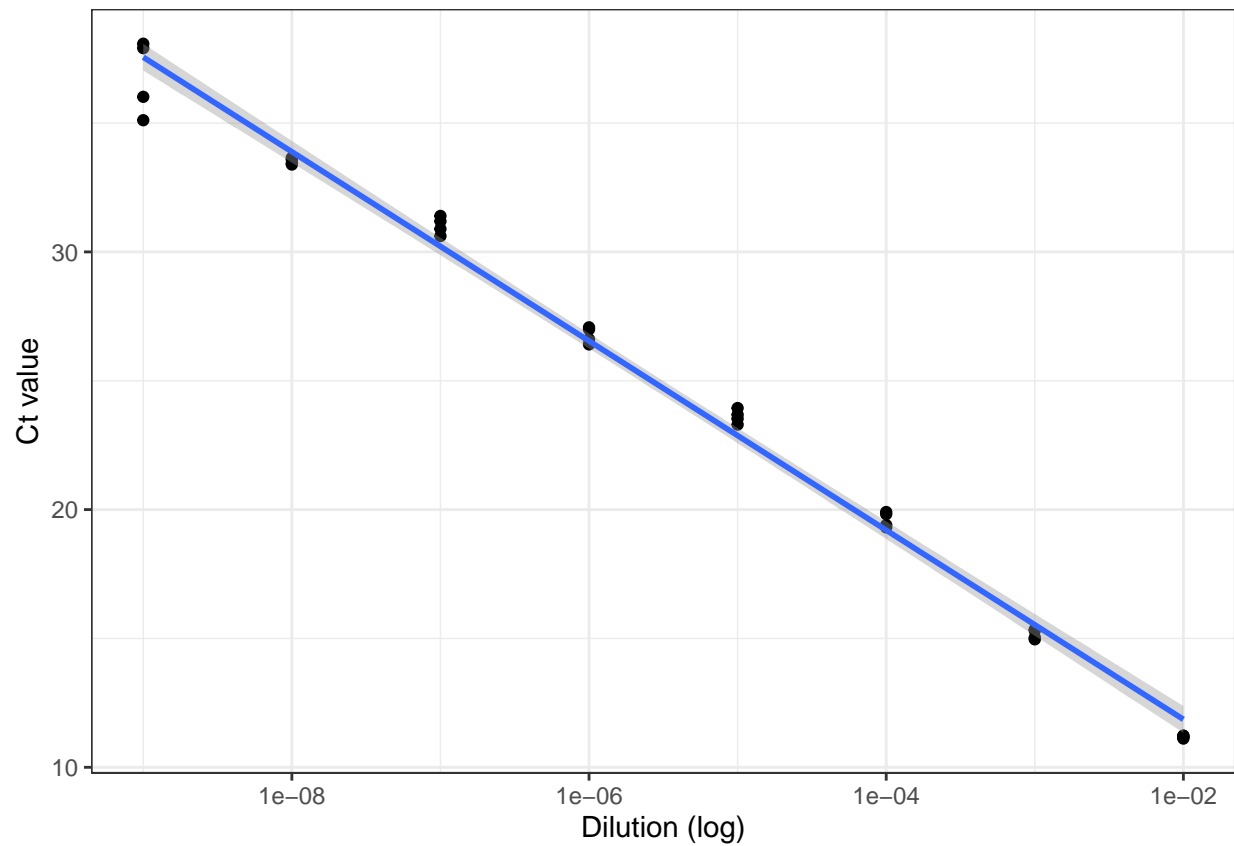

$R^2 = 0.992$

Average sample SD = 0.365225