

qPCR Quality Control Summary

Seth Goodnight

2024-05-25


Instrument

Calibration:

FAM: 11-08-2023

ROX: 11-08-2023

Standard Curve:

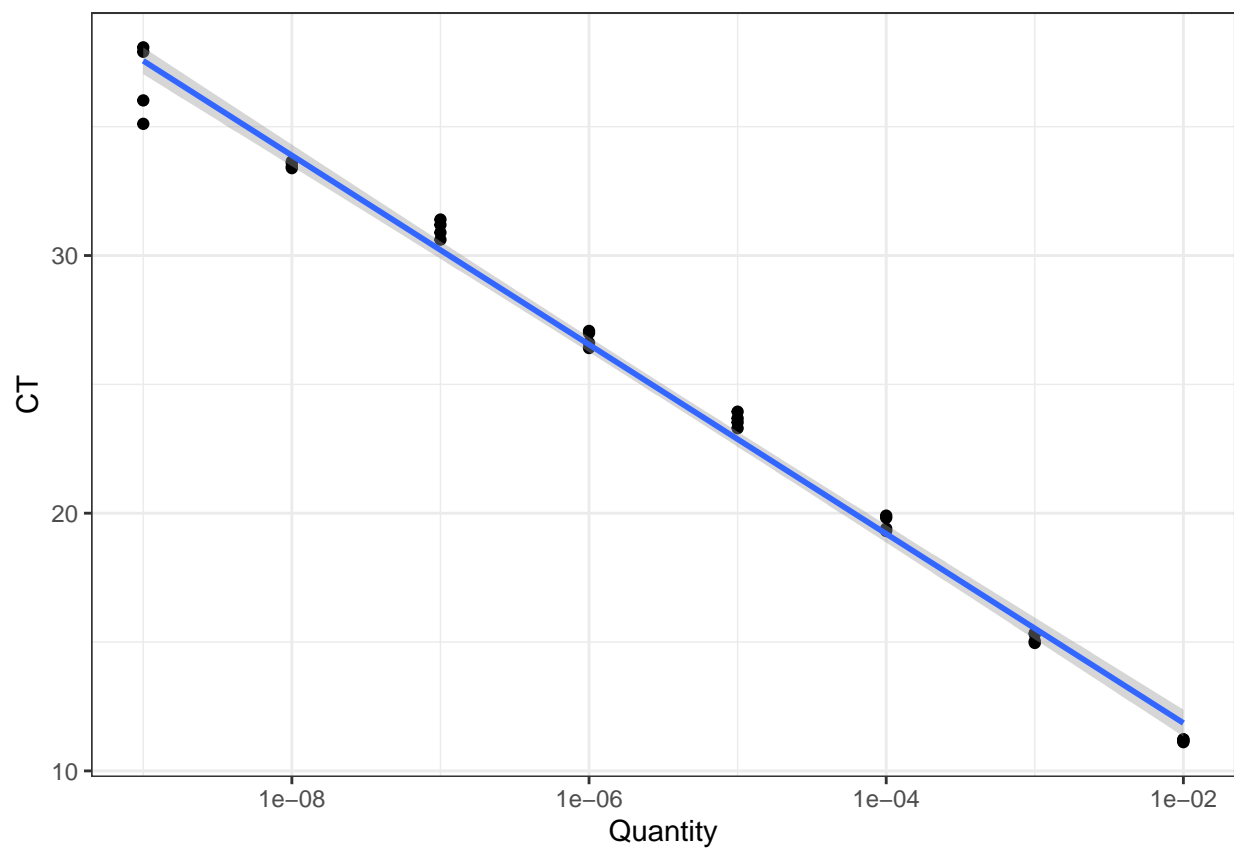

R2=0.992