


# Morning Data Distribution in Measurement Difference: Temperature

## Testo400 - MLX90614



## Testo 400 - SCD30

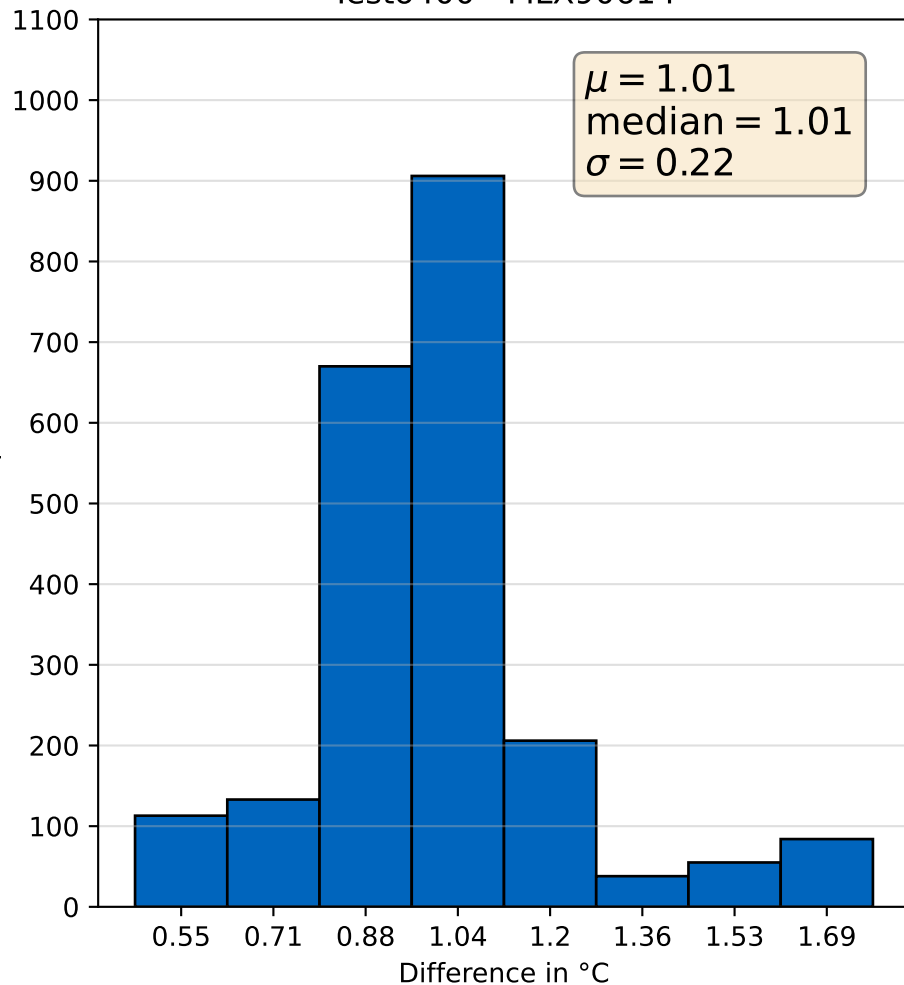