



p_{60} p_{70} p_{80} threshold (gap = 0.005) — gap = 0 (= reference)





TIAGE

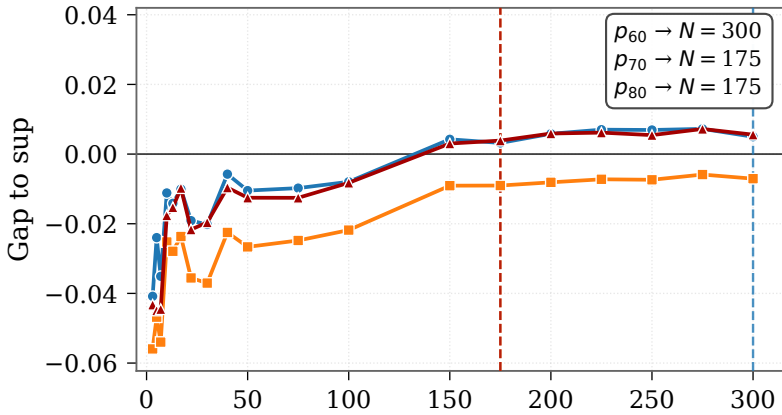

Dialseg711

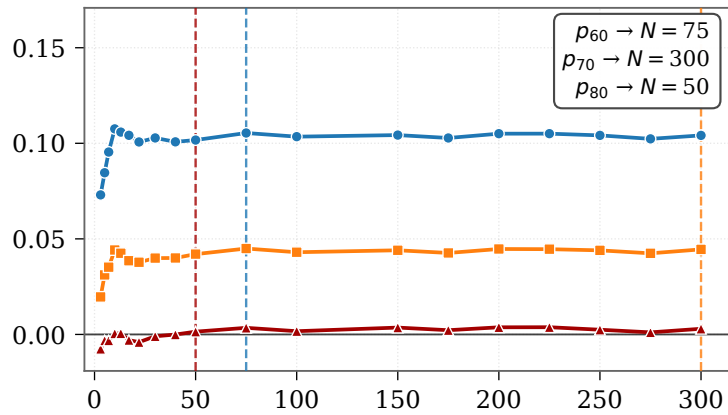

SuperDialseg

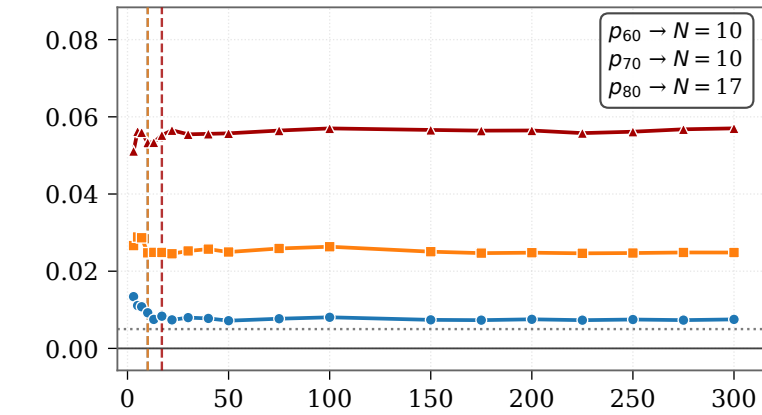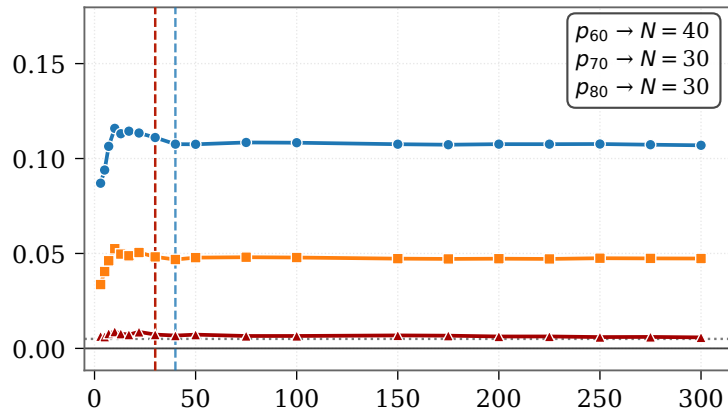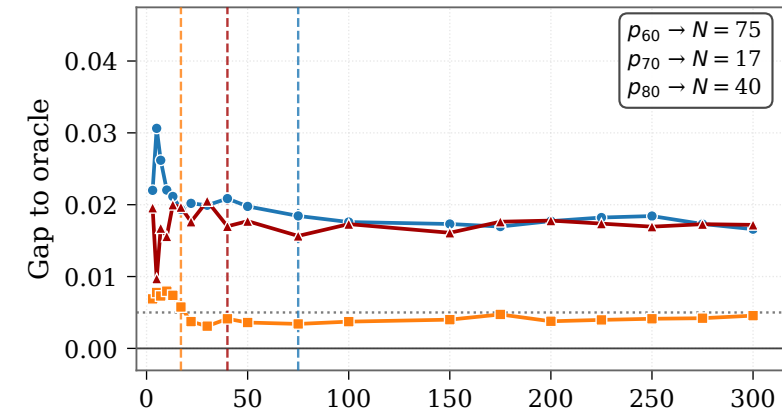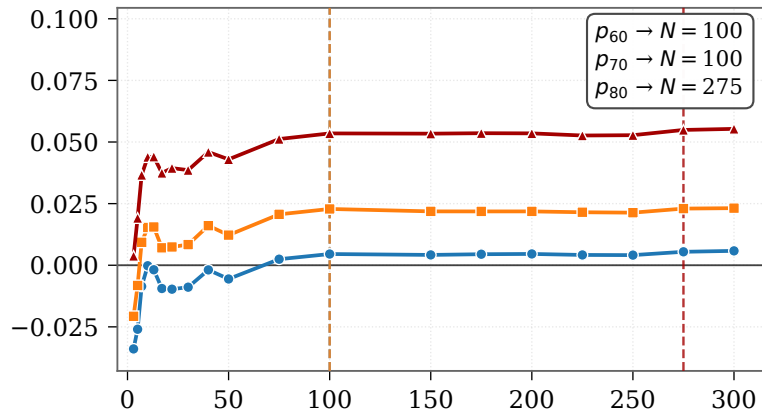

Calibration dialogs N

Calibration dialogs N

Calibration dialogs N