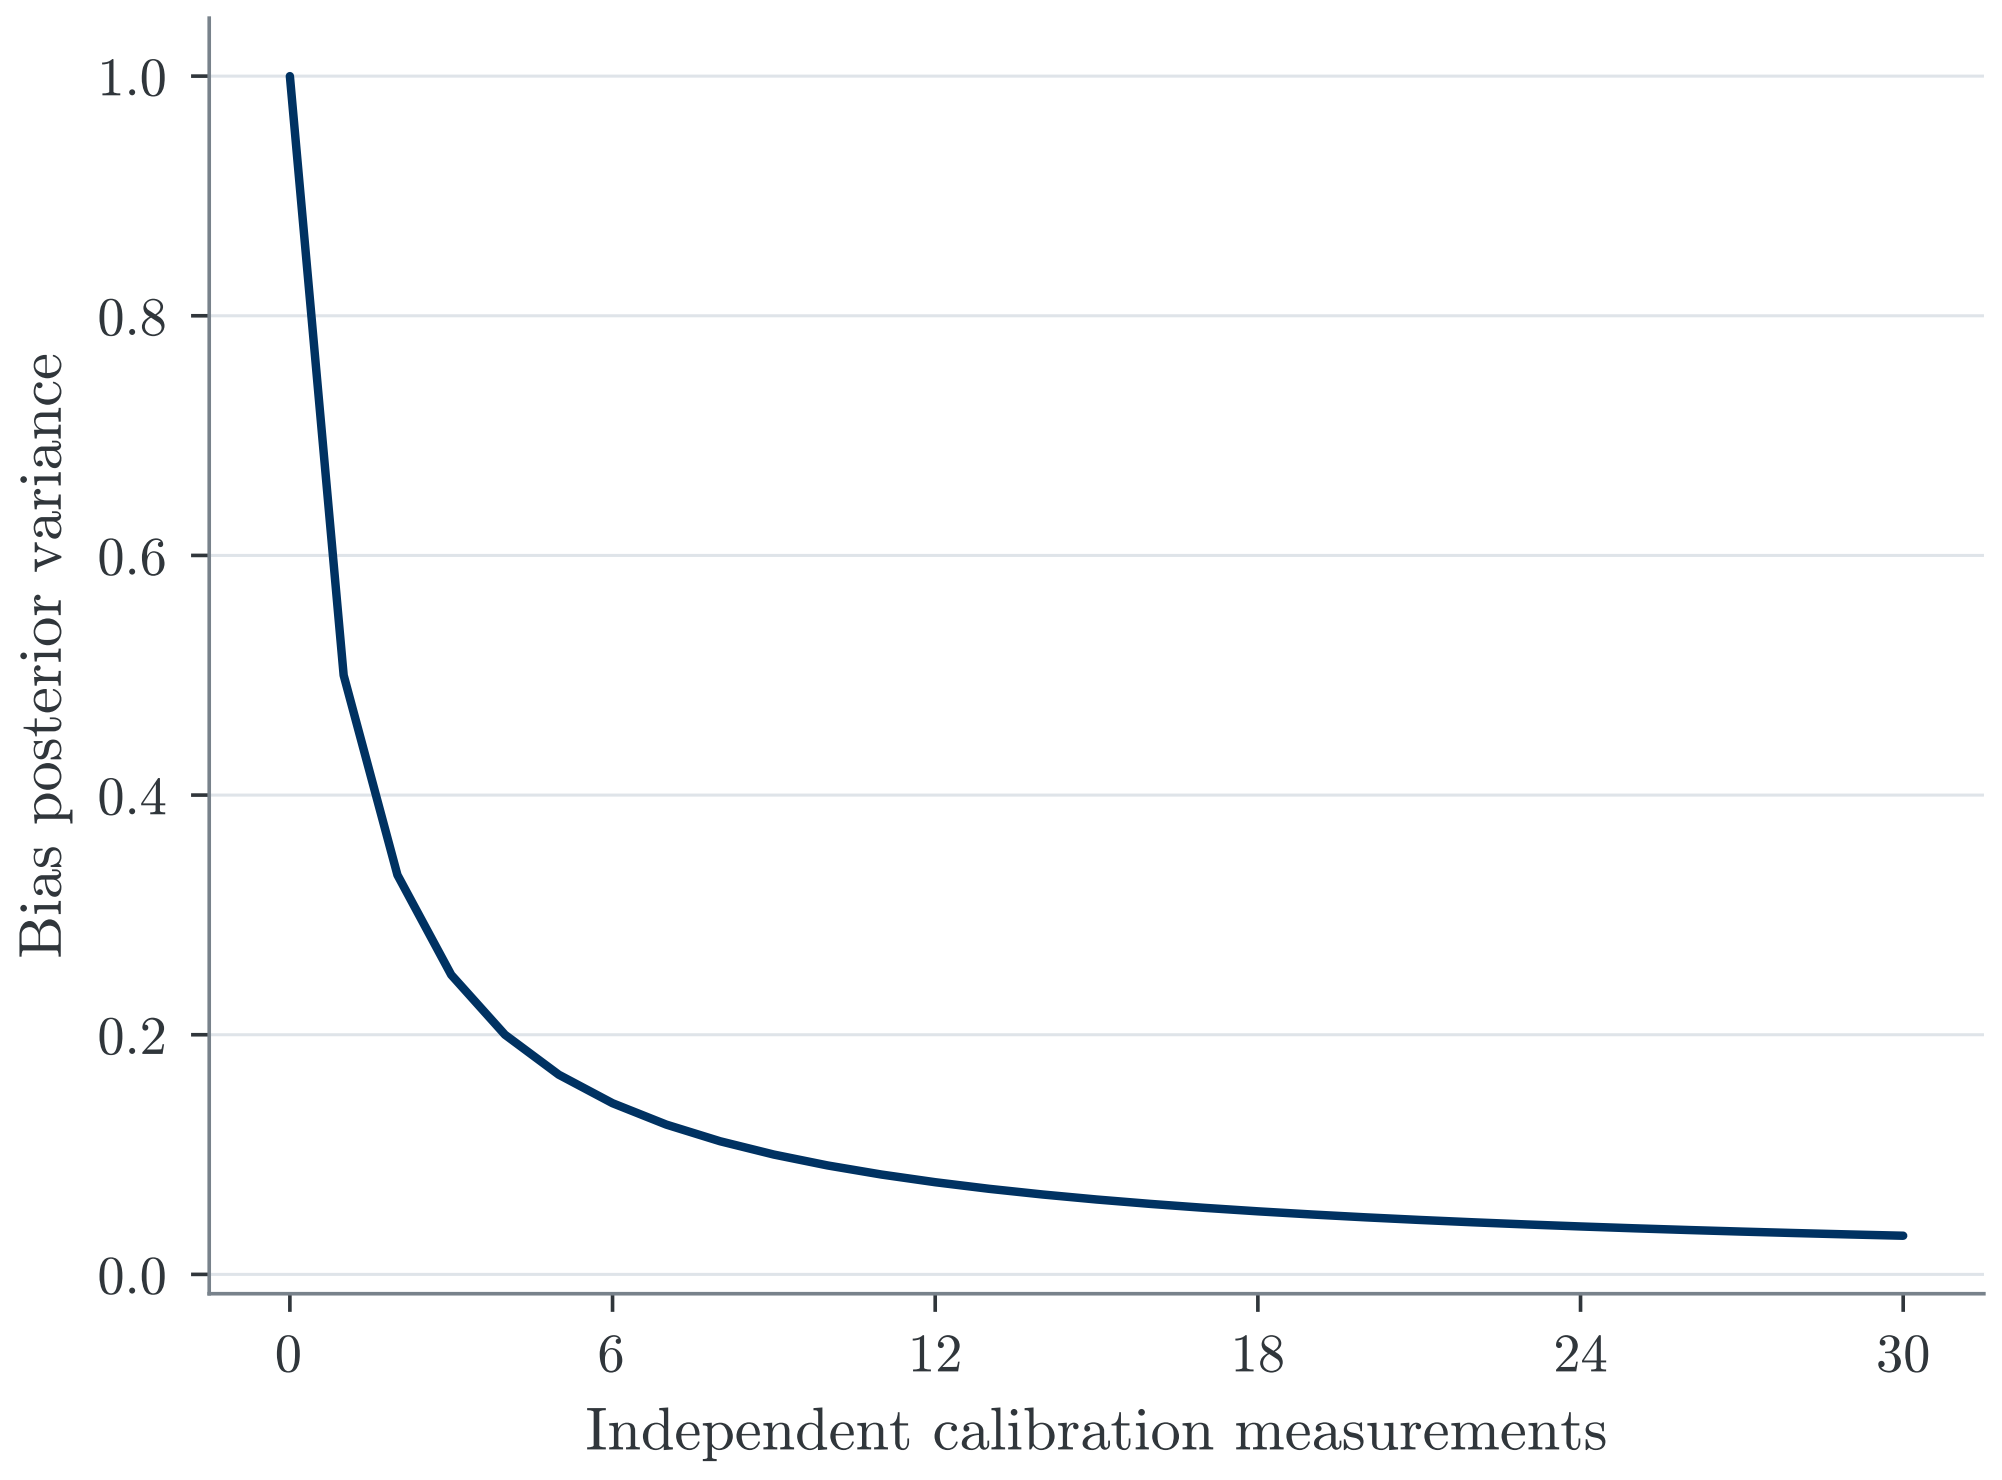
1.0
0.8
0.6
0.4
0.2
0.0
Bias posterior variance
0
6
12
18
24
30
Independent calibration measurements