AANDERAA a xylem brand

TEST & SPECIFICATIONS

Form No. 712 V2,March 2014

Program Version: 04.09.2001

Product: Oxygen Optode 4831
Serial No: 675

Visual and Mechanical Checks:

1.1 Soldering quality
1.2 Visual surface
1.3 Galvanic isolation between housing and electronics

Current Drain and Voltages:

2.1	Average current drain at 0.5 Hz sampling (Max.: 33 mA)	23.0	mA
2.2	CANBus Current drain at 0.5 Hz sampling (Max.: 33 mA)		mA
2.3	Current drain in sleep (Max.: 180 µA)	216	µA
2.4	CANBus Current drain in sleep (Max.: 180 µA)		µA
2.5	DSP IO voltage, J4.18 (3.3 ±0.15V)		V
2.6	DSP Core voltage, J4.17(1.8 ±0.05 V)	1.82	V
2.7	Excitation driver voltage, C4 Analog Board (4.5 ±0.15 V)	4.31	V

Performance test:

	Channel:	Blue		Red	
3.1	Average of Receiver readings (0±150mV)	-1.2	mV	-1.5	mV
3.2	Standard Deviation of Receiver readings (Max.: 45mV/10mV)	1.78	mV	0.58	mV
3.3	Amplitude measm. with non-fluorescence foil (<60mV/650-1200mV)	14.8	mV	1066.7	mV
3.4	CANBus Output test				

Function test from 0 to 40°C:

	Channel:	Blue		Red	
4.1	Minimum amplitude measurement (Blue: >550 mV, Red >650 mV)	679.3	mV	801.6	mV
4.2	Maximum amplitude measurement (Blue: <1600 mV, Red <1400 mV)	1043.2	mV	1256.2	mV
4.3	Minimum phase measurement (Blue: >24°, Red: >1°)	34.72	°	7.51	°
4.4	Maximum phase measurement (Blue: <34°, Red: <5°)	40.33	°	8.56	°
4.5	Maximum standard deviation of Phase measurement: (< 0.02°)	0.05	°	0.04	°
4.6	Minimum temperature raw data measurement: (<-200 mV)			-506.2	mV
4.7	Maximum temperature raw data measurement: (>450 mV)			619	mV

Pressure test :

5.1 Pressure (IW version: 20MPa, DW version 60MPa) 60MPa

Date: 23 Mar 2017

Sign:

Vidar Selsvik, Production Engineer

AANDERAA
a xylem brand

CALIBRATION CERTIFICATE

Form No 830, Juli 2012

Certificate no: 4831_675_00128391
Foil batch no: 1517M

Product: 4831
Calibration date: 15.03.2017

Serial no: 675

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.68472E-03	1.12034E-04	2.31129E-06	2.31460E02	-4.26981E-01	-5.09191E01	4.60068E00
TempCoef	2.42469E01	-3.11061E-02	2.90633E-06	-4.28648E-09	0.00000E00	0.00000E00	

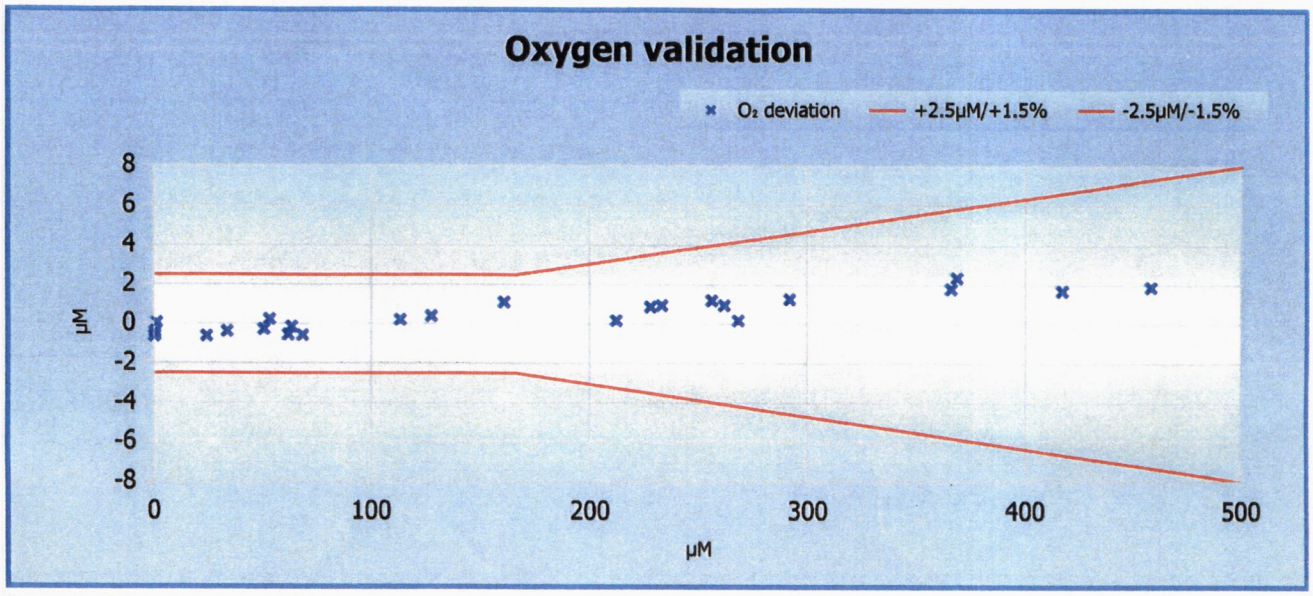

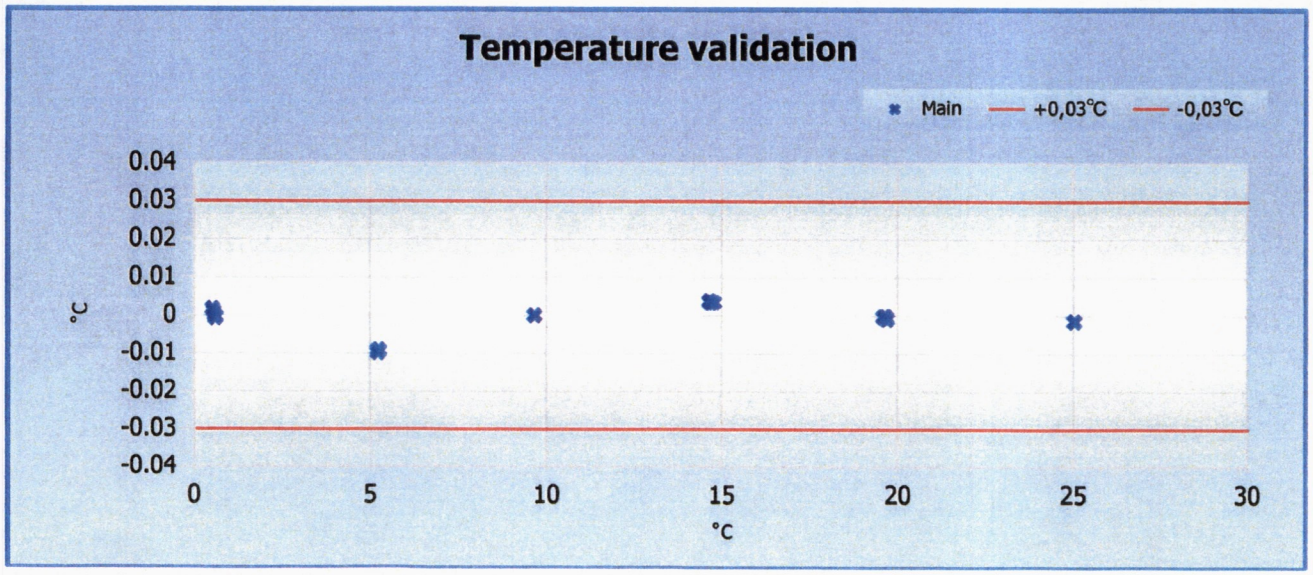

Date:15.03.2017

Tor-Ove Kvalvaag

Tor-Ove Kvalvaag, Calibration Engineer