



Conductivity Calibration Certificate

RBRlegato³ C.T.D, Teledyne Webb Slocum, dry bay (1000dbar)



s/n: 243159

References: Autosal8400B#66289, MS-315#15506, SSW P169, RC#002


Reference Resistance (ohm)	Reference Conductivity (mS/cm)	Voltage Ratio, V	Measured Conductivity (mS/cm)	Calibration Error (mS/cm)	Coefficients	
open	0.0000	-0.000114	0.0007	0.0007	C0:	21.27334E-3
693.9970	7.0680	0.038941	7.0677	-0.0003	C1:	180.95045
331.9137	14.7784	0.081551	14.7780	-0.0004	(K) C2:	1.001942
150.0103	32.6987	0.180589	32.6989	0.0002	X0:	392.55834E-6
100.0113	49.0459	0.270926	49.0455	-0.0004	X1:	-25.941348E-6
75.0201	65.3844	0.361219	65.3840	-0.0004	X2:	1.6104E-6
55.5178	88.3526	0.488155	88.3531	0.0005	X3:	-290.6518E-12
					X4:	-239.5425E-15
Bath	Voltage Ratio	Temperature (ITS-90)	Salinity (PSS-78)	Conductivity (mS/cm)	X5:	15.62451
T15S35	0.2405082	15.62451	35.0074	43.5413	X6:	10
T25S35	0.2927449	24.92789	35.0052	53.0027		

Cell Constant @T15S35 = 4.90514 1/cm

$$C_c = \frac{C_0 + C_1 * C_2 * V - X_0 * (T - X_5)}{1 + X_1 * (T - X_5) + X_2 * (P - X_6) + X_3 * (P - X_6)^2 + X_4 * (P - X_6)^3}$$

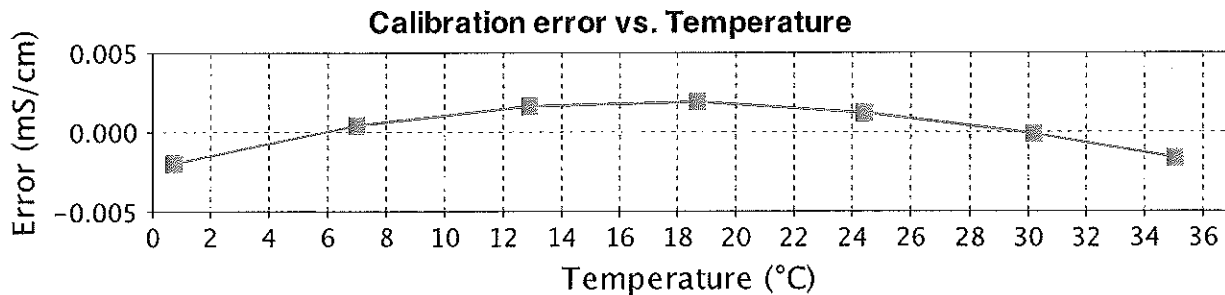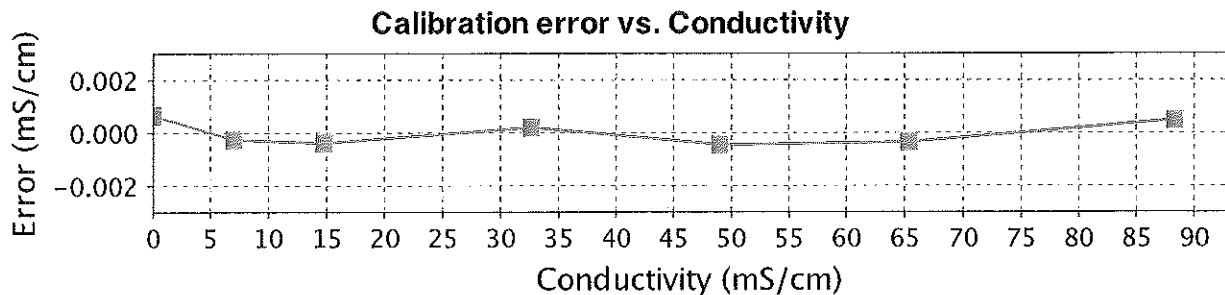

Calibration Date: 2026-06-30
Issue Date: 2026-07-02
File Name: 243159_20260630_1443FinalC.rsk

Operator: 
ytouba

Approver: 
slangstaff




Temperature Calibration Certificate

Logger ID: RBRlegato³ Serial No: 243159 Channel No: 2

Reference Temperature, ITS-90	Voltage ratio, V	Measured Temperature, ITS-90	Calibration error	Coefficients	
-4.88560	0.7298358	-4.88556	0.00004	C0:	3.4760486E-3
0.76676	0.6664510	0.76667	-0.00009	C1:	-250.602E-6
6.99996	0.5918382	6.99992	-0.00004	C2:	2.5251727E-6
12.91270	0.5196144	12.91279	0.00009	C3:	-78.361744E-9
18.68058	0.4507763	18.68073	0.00016		
24.41707	0.3863079	24.41692	-0.00015		
30.19623	0.3270983	30.19613	-0.00010		
35.06478	0.2824139	35.06487	0.00009		

$$T_m = \ln\left(\left(\frac{1}{V}\right) - 1\right)$$

$$T_c = \frac{1}{(C_0 + C_1 T_m + C_2 T_m^2 + C_3 T_m^3)} - 273.15$$

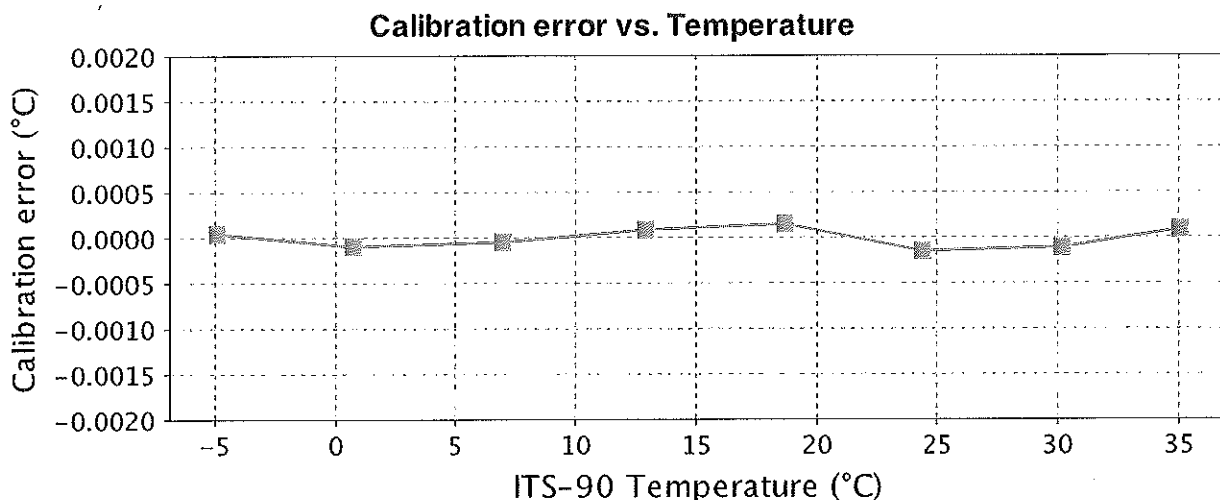

Calibration Date: 2026-06-25
Issue Date: 2026-06-25
Calibration ID: 94010

Operator:

kthakkar

Approver:

jwang



Pressure Calibration Certificate

RBRlegato³ C.T.D, Teledyne Webb Slocum, dry bay (1000dbar)

s/n: 243159

Instrument rating: 1000



Nominal accuracy: 0.05%FS (0.5 dbar)

Reference instrument: Mensor CPC6050 s/n: 41000CAM

Applied pressure, P_{app} (dbar)	Voltage ratio, V	Measured pressure, P_c (dbar)	Calibration error (dbar)	Coefficients
10.219	0.0204464	10.222	0.003	C0: -35.97843
110.151	0.0646457	110.169	0.018	C1: 2.258564E3
210.149	0.1088082	210.146	-0.003	C2: 33.93903
310.151	0.1529313	310.136	-0.015	C3: -23.756813
410.149	0.1970240	410.149	0.000	X0: 10.0679
510.150	0.2410925	510.184	0.034	X1: 66.20981E-3
610.147	0.2850916	610.126	-0.021	X2: -35.255318E-6
710.153	0.3290998	710.144	-0.009	X3: -1.5817163E-6
810.151	0.3730887	810.158	0.007	X4: -109.21925E-6
910.151	0.4170582	910.158	0.007	X5: 21.346275
1010.151	0.4610196	1010.154	0.003	Head (mm) = 150

$$P_c = X_0 + \frac{P_m - X_0 - X_1(T - X_5) - X_2(T - X_5)^2 - X_3(T - X_5)^3}{1 + X_4(T - X_5)}$$

$$P_m = C_0 + C_1V + C_2V^2 + C_3V^3$$

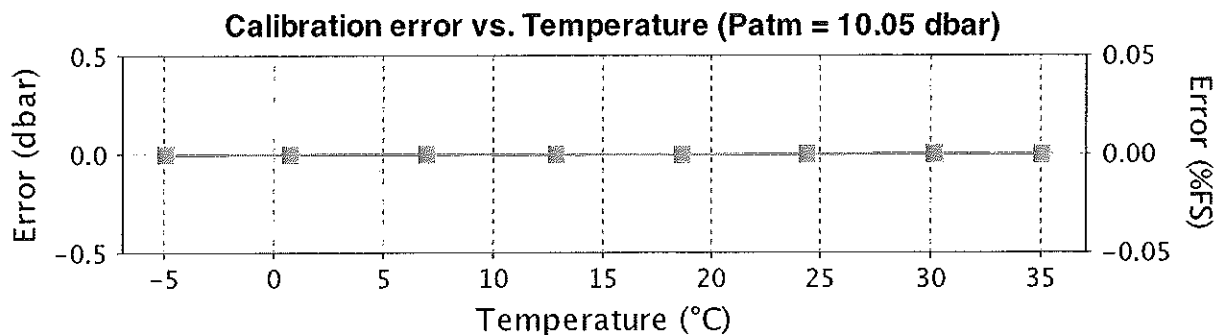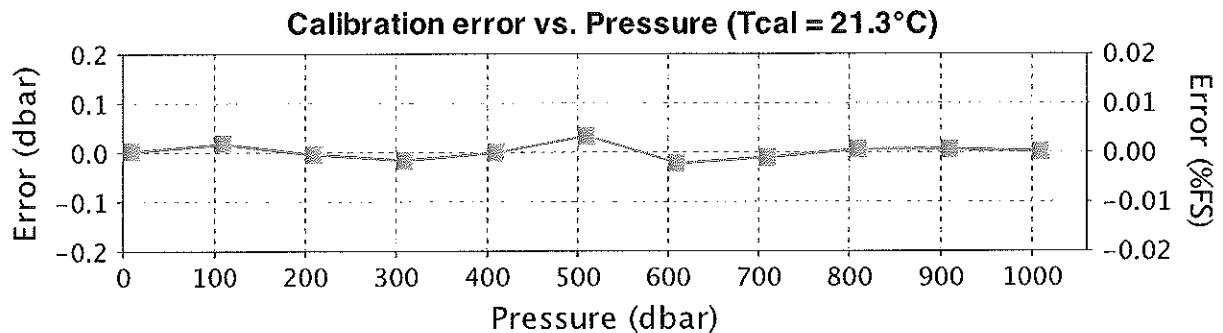

Calibration Date: 2026-06-26
Issue Date: 2026-06-26
File Name: 243159_20260626_1052P.rsk

Operator: P. J. Shah
pshah

Approver: [Signature]
slangstaff