



Conductivity Calibration Certificate

RBRlegato³ C.T.D, Teledyne Webb Slocum, dry bay (1000dbar)



s/n: 243155

References: Autosal8400B#66289, MS-315#15506, SSW P169, RC#002

Reference Resistance (ohm)	Reference Conductivity (mS/cm)	Voltage Ratio, V	Measured Conductivity (mS/cm)	Calibration Error (mS/cm)	Coefficients	
open	0.0000	-0.000190	0.0003	0.0003	C0:	34.686238E-3
693.9970	7.0647	0.038874	7.0645	-0.0002	C1:	180.83623
331.9137	14.7715	0.081492	14.7714	-0.0001	(K) C2:	1.001942
150.0103	32.6836	0.180546	32.6840	0.0004	X0:	1.0396936E-3
100.0113	49.0232	0.270899	49.0230	-0.0002	X1:	-30.63615E-6
75.0201	65.3542	0.361206	65.3538	-0.0004	X2:	1.1858E-6
55.5178	88.3118	0.488162	88.3121	0.0003	X3:	256.4482E-12
					X4:	-555.7214E-15
Bath	Voltage Ratio	Temperature (ITS-90)	Salinity (PSS-78)	Conductivity (mS/cm)	X5:	15.46848
T15S35	0.2396782	15.46848	34.9983	43.3772	X6:	10
T25S35	0.2929341	24.94318	35.0012	53.0133		

Cell Constant @T15S35 = 4.90288 1/cm

$$C_c = \frac{C_0 + C_1 * C_2 * V - X_0 * (T - X_5)}{1 + X_1 * (T - X_5) + X_2 * (P - X_6) + X_3 * (P - X_6)^2 + X_4 * (P - X_6)^3}$$

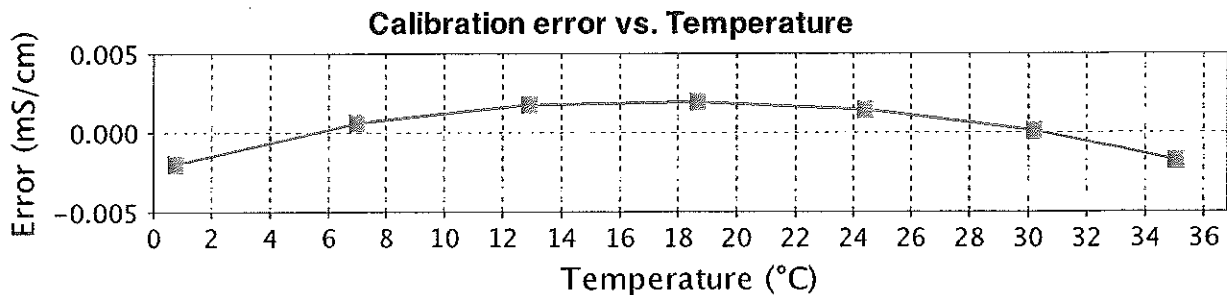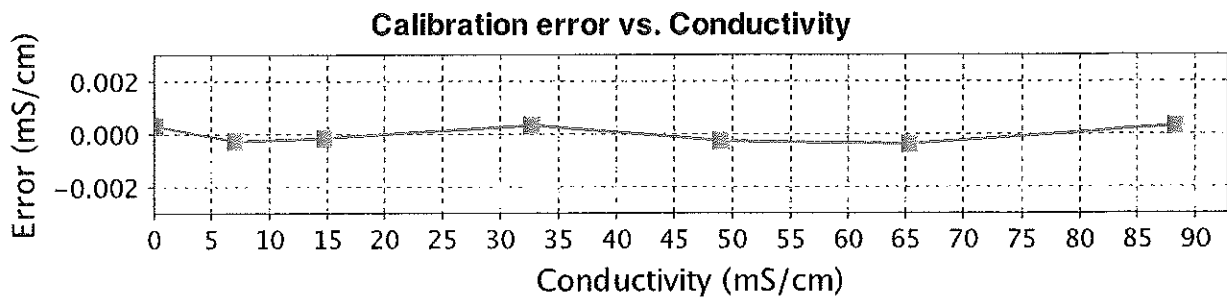

Calibration Date: 2026-07-02
Issue Date: 2026-07-03
File Name: 243155_20260702_130FinalC.rsk

Operator: 
ytlouba

Approver: 
slangstaff




Temperature Calibration Certificate

Logger ID: RBRlegato³ Serial No: 243155 Channel No: 2


Reference Temperature, ITS-90	Voltage ratio, V	Measured Temperature, ITS-90	Calibration error	Coefficients	
-4.88561	0.7301757	-4.88559	0.00002	C0:	3.4733557E-3
0.76677	0.6674091	0.76675	-0.00002	C1:	-252.9568E-6
6.99996	0.5935723	6.99994	-0.00002	C2:	2.434454E-6
12.91271	0.5220861	12.91275	0.00004	C3:	-76.31643E-9
18.68058	0.4538854	18.68060	0.00002		
24.41706	0.3899071	24.41704	-0.00002		
30.19623	0.3310234	30.19617	-0.00006		
35.06477	0.2864793	35.06481	0.00004		


$$T_m = \ln\left(\left(\frac{1}{V}\right) - 1\right)$$

$$T_c = \frac{1}{(C_0 + C_1 T_m + C_2 T_m^2 + C_3 T_m^3)} - 273.15$$

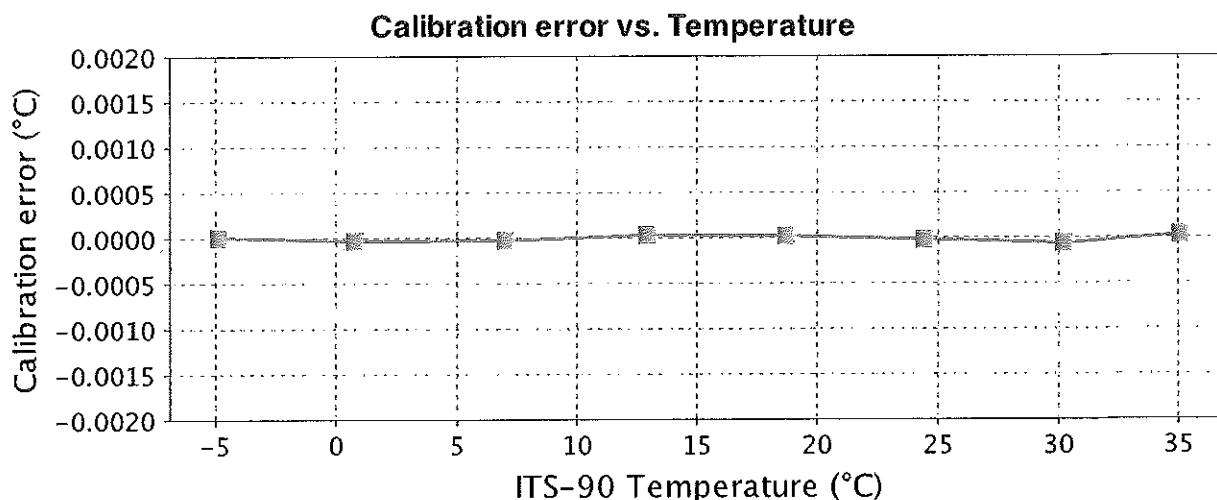

Calibration Date: 2026-06-25
Issue Date: 2026-06-25
Calibration ID: 94016

Operator: 
kthakkar

Approver: 
jwang



Pressure Calibration Certificate

RBRlegato³ C.T.D, Teledyne Webb Slocum, dry bay (1000dbar)

s/n: 243155

Instrument rating: 1000



Nominal accuracy: 0.05%FS (0.5 dbar)

Reference instrument: Mensor CPC6050 s/n: 41000CAM

Applied pressure, P_{app} (dbar)	Voltage ratio, V	Measured pressure, P_c (dbar)	Calibration error (dbar)	Coefficients
10.425	0.0208529	10.425	0.000	C0: -36.753143
110.355	0.0650072	110.383	0.028	C1: 2.260936E3
210.353	0.1091138	210.362	0.009	C2: 37.56777
310.355	0.1531836	310.367	0.012	C3: -28.237566
410.353	0.1971981	410.345	-0.008	X0: 10.0697
510.354	0.2411896	510.350	-0.004	X1: 66.05675E-3
610.356	0.2851391	610.328	-0.028	X2: -21.046235E-6
710.357	0.3290910	710.364	0.007	X3: -810.0832E-9
810.356	0.3730199	810.383	0.027	X4: -109.11245E-6
910.353	0.4169202	910.367	0.014	X5: 21.516294
1010.355	0.4608184	1010.350	-0.005	Head (mm) = 355

$$P_c = X_0 + \frac{P_m - X_0 - X_1(T - X_5) - X_2(T - X_5)^2 - X_3(T - X_5)^3}{1 + X_4(T - X_5)}$$

$$P_m = C_0 + C_1V + C_2V^2 + C_3V^3$$

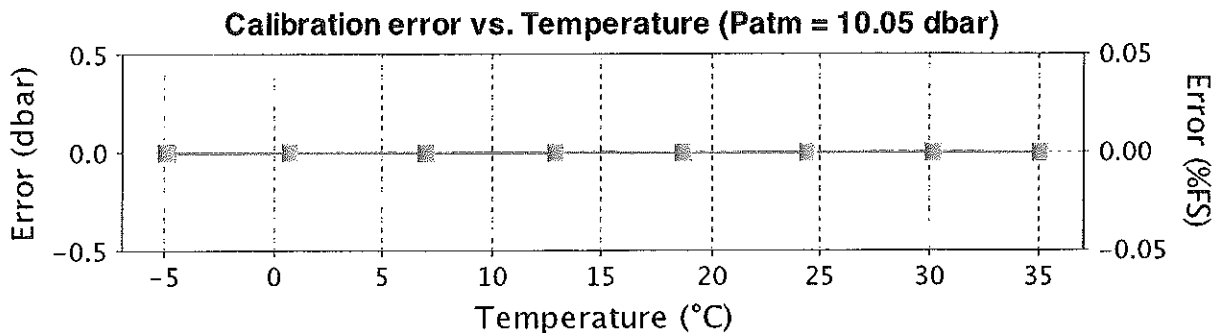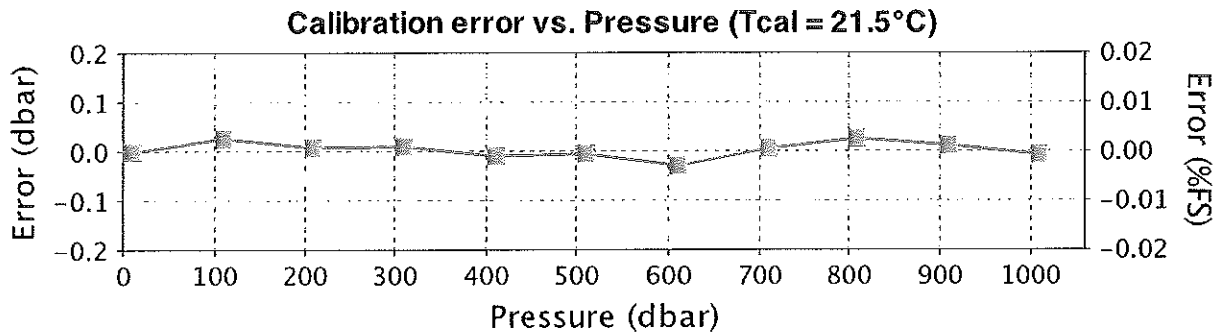

Calibration Date: 2026-06-26
Issue Date: 2026-06-29
File Name: 243155_20260626_1449P.rsk

Operator: P. J. Shah
pshah

Approver: [Signature]
slangstaff