
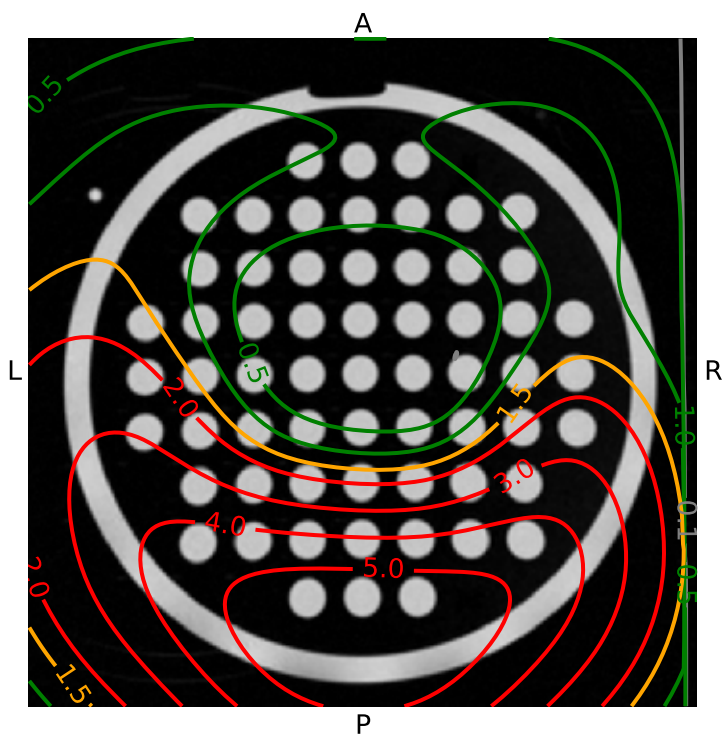
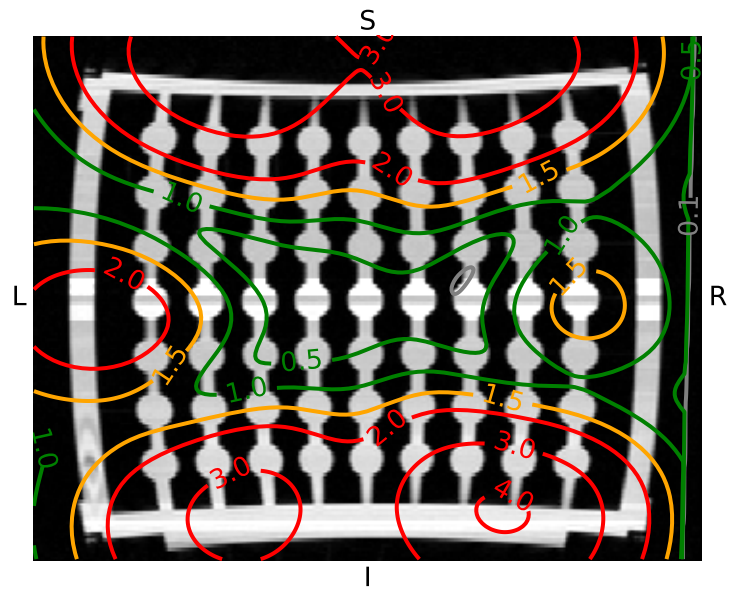


Distortion of mri.nii.gz

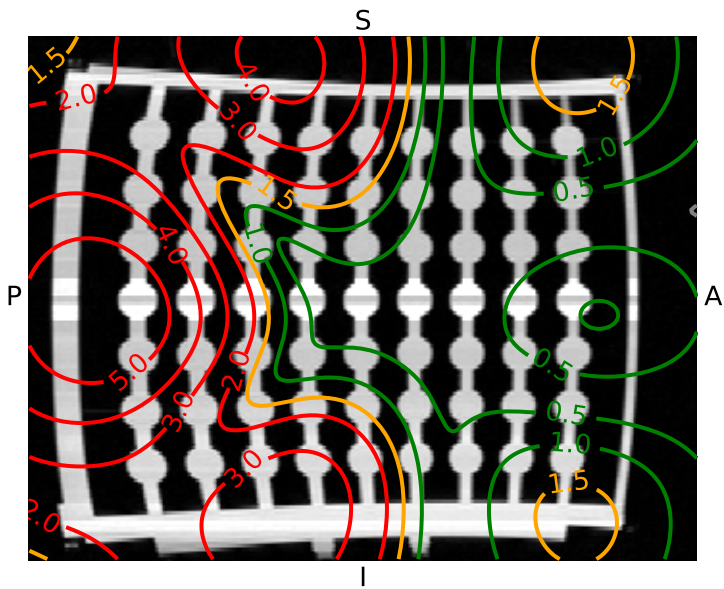

The contours show the distortion of the MRI in mm overlayed on the MRI. Distortion is quantified as the magnitude of the displacement field from the non-rigid registration of the MRI to a CT image of the phantom.

If no contours are shown distortions are <0.1 mm.