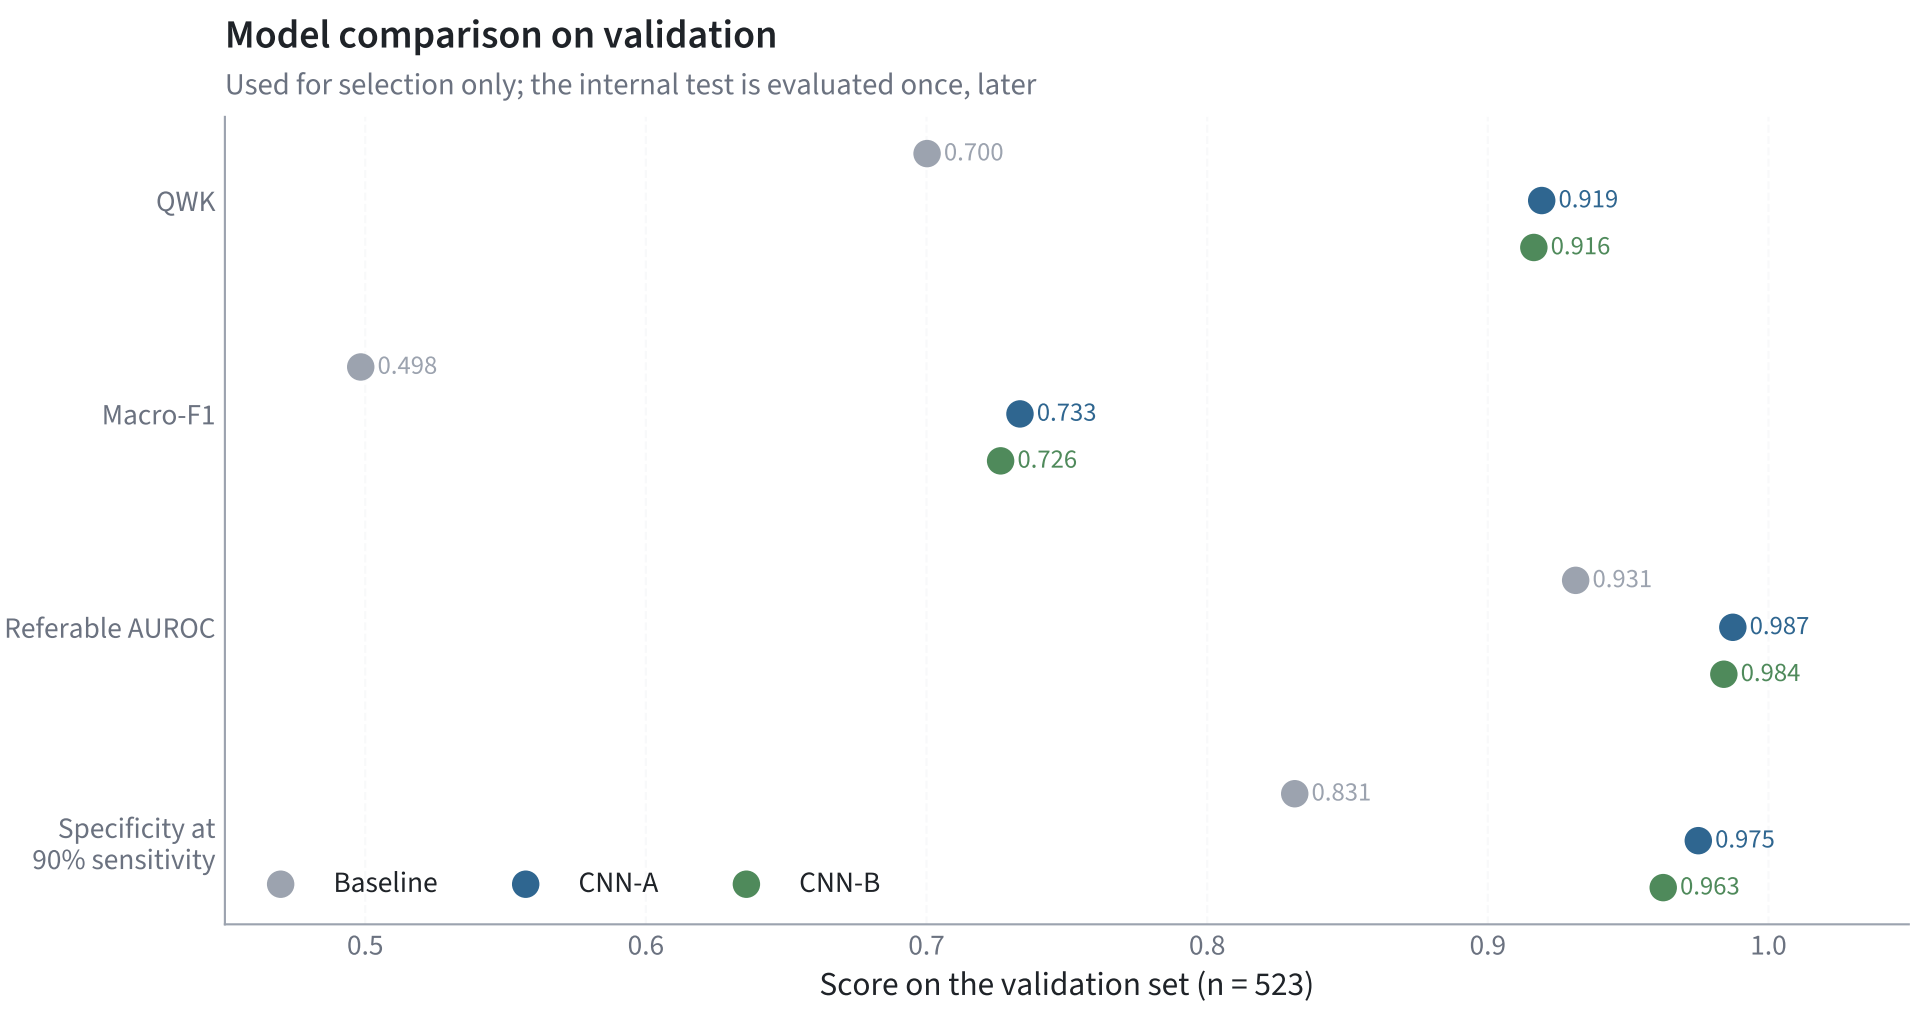
Model comparison on validation
Used for selection only; the internal test is evaluated once, later
QWK
Macro-F1
Referable AUROC
Specificity at 90% sensitivity
0.700
0.919
0.916
0.498
0.733
0.726
0.931
0.987
0.984
0.831
0.975
0.963
Baseline
CNN-A
CNN-B
0.5
0.6
0.7
0.8
0.9
1.0
Score on the validation set (n = 523)