



A. Earlier PVC used for supervised fitting
record 105, R peak at 350.305 s

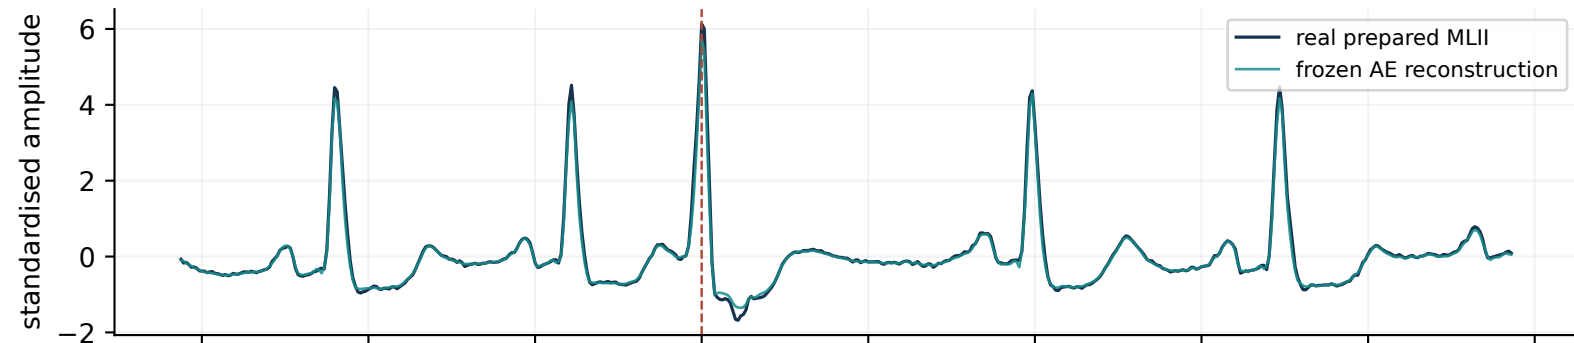

B. Later PVC reserved for temporal testing
record 105, R peak at 1461.008 s

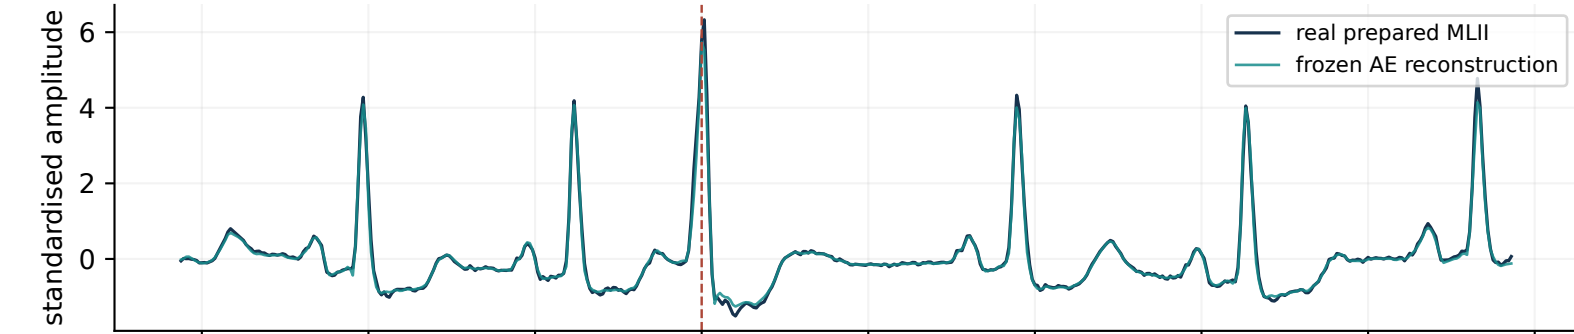

C. Later normal beat reserved for temporal testing
record 100, R peak at 1444.852 s

