



Real ECG cleaning for the two one-channel model inputs


A. Autoencoder: NSRDB 16272 / ECG1
1. Unfiltered four-second segment at 128 Hz

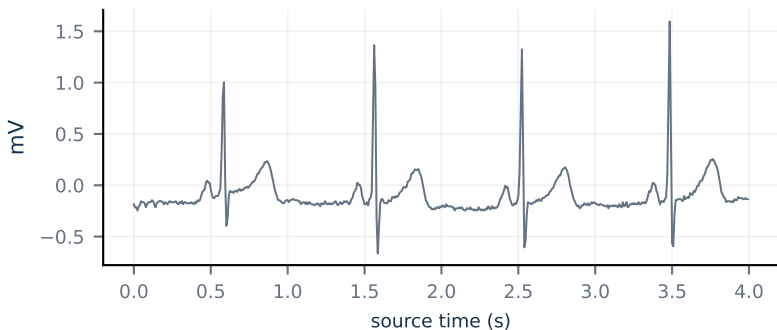


2. Filter source block; retain first four seconds

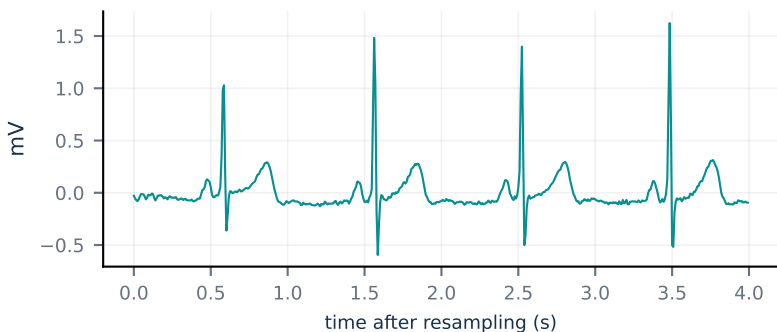


3. Actual cached input; retain archived scaling

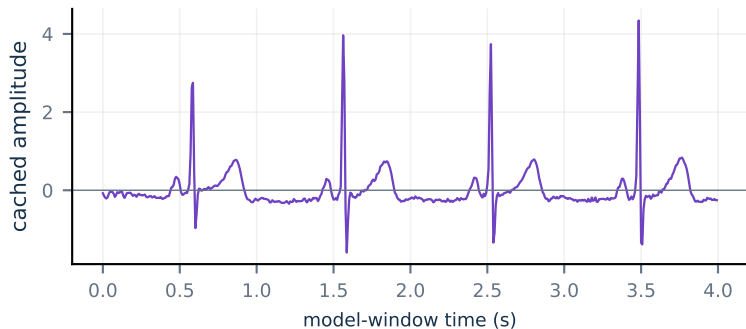

B. Detector/classifier: MITDB record 100, MLII
1. Unfiltered four-second segment at 128 Hz

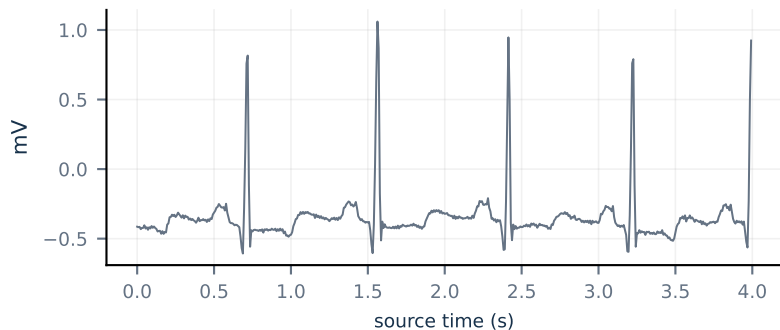

2. Filter this beat window: 0.5--50 Hz

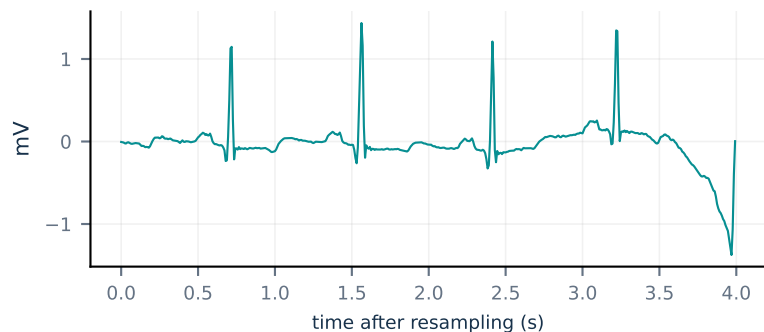

3. Standardise each R-aligned 4 s beat window

