



Supplemental Fig. S2

A

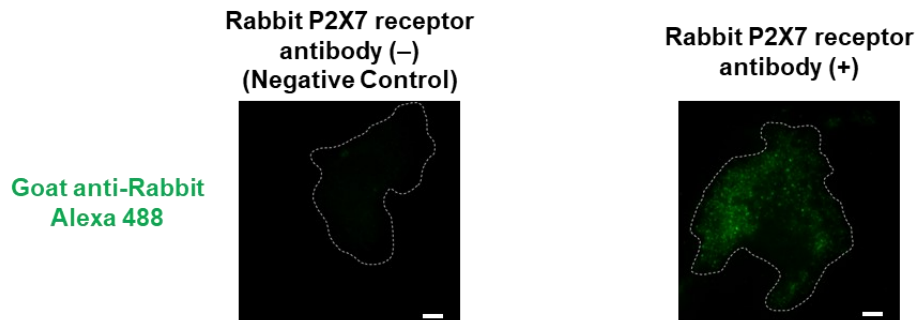

B

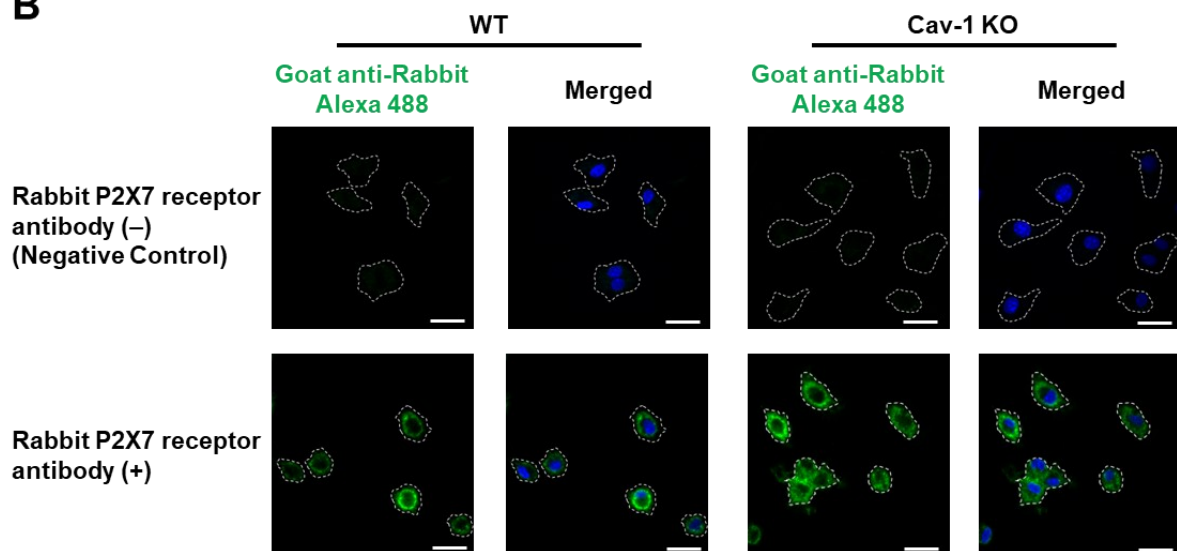

Supplemental Fig. S2: Validation of the selectivity of the anti-P2X7 receptor antibody used in TIRF and confocal microscopy.

The representative images of negative secondary antibody controls in TIRF imaging (A, for Fig. 2A-E) and confocal imaging (B, for Fig. 2I-J). Data were obtained from one isolation. Scale bar denotes 5 μm in A and 50 μm in B.