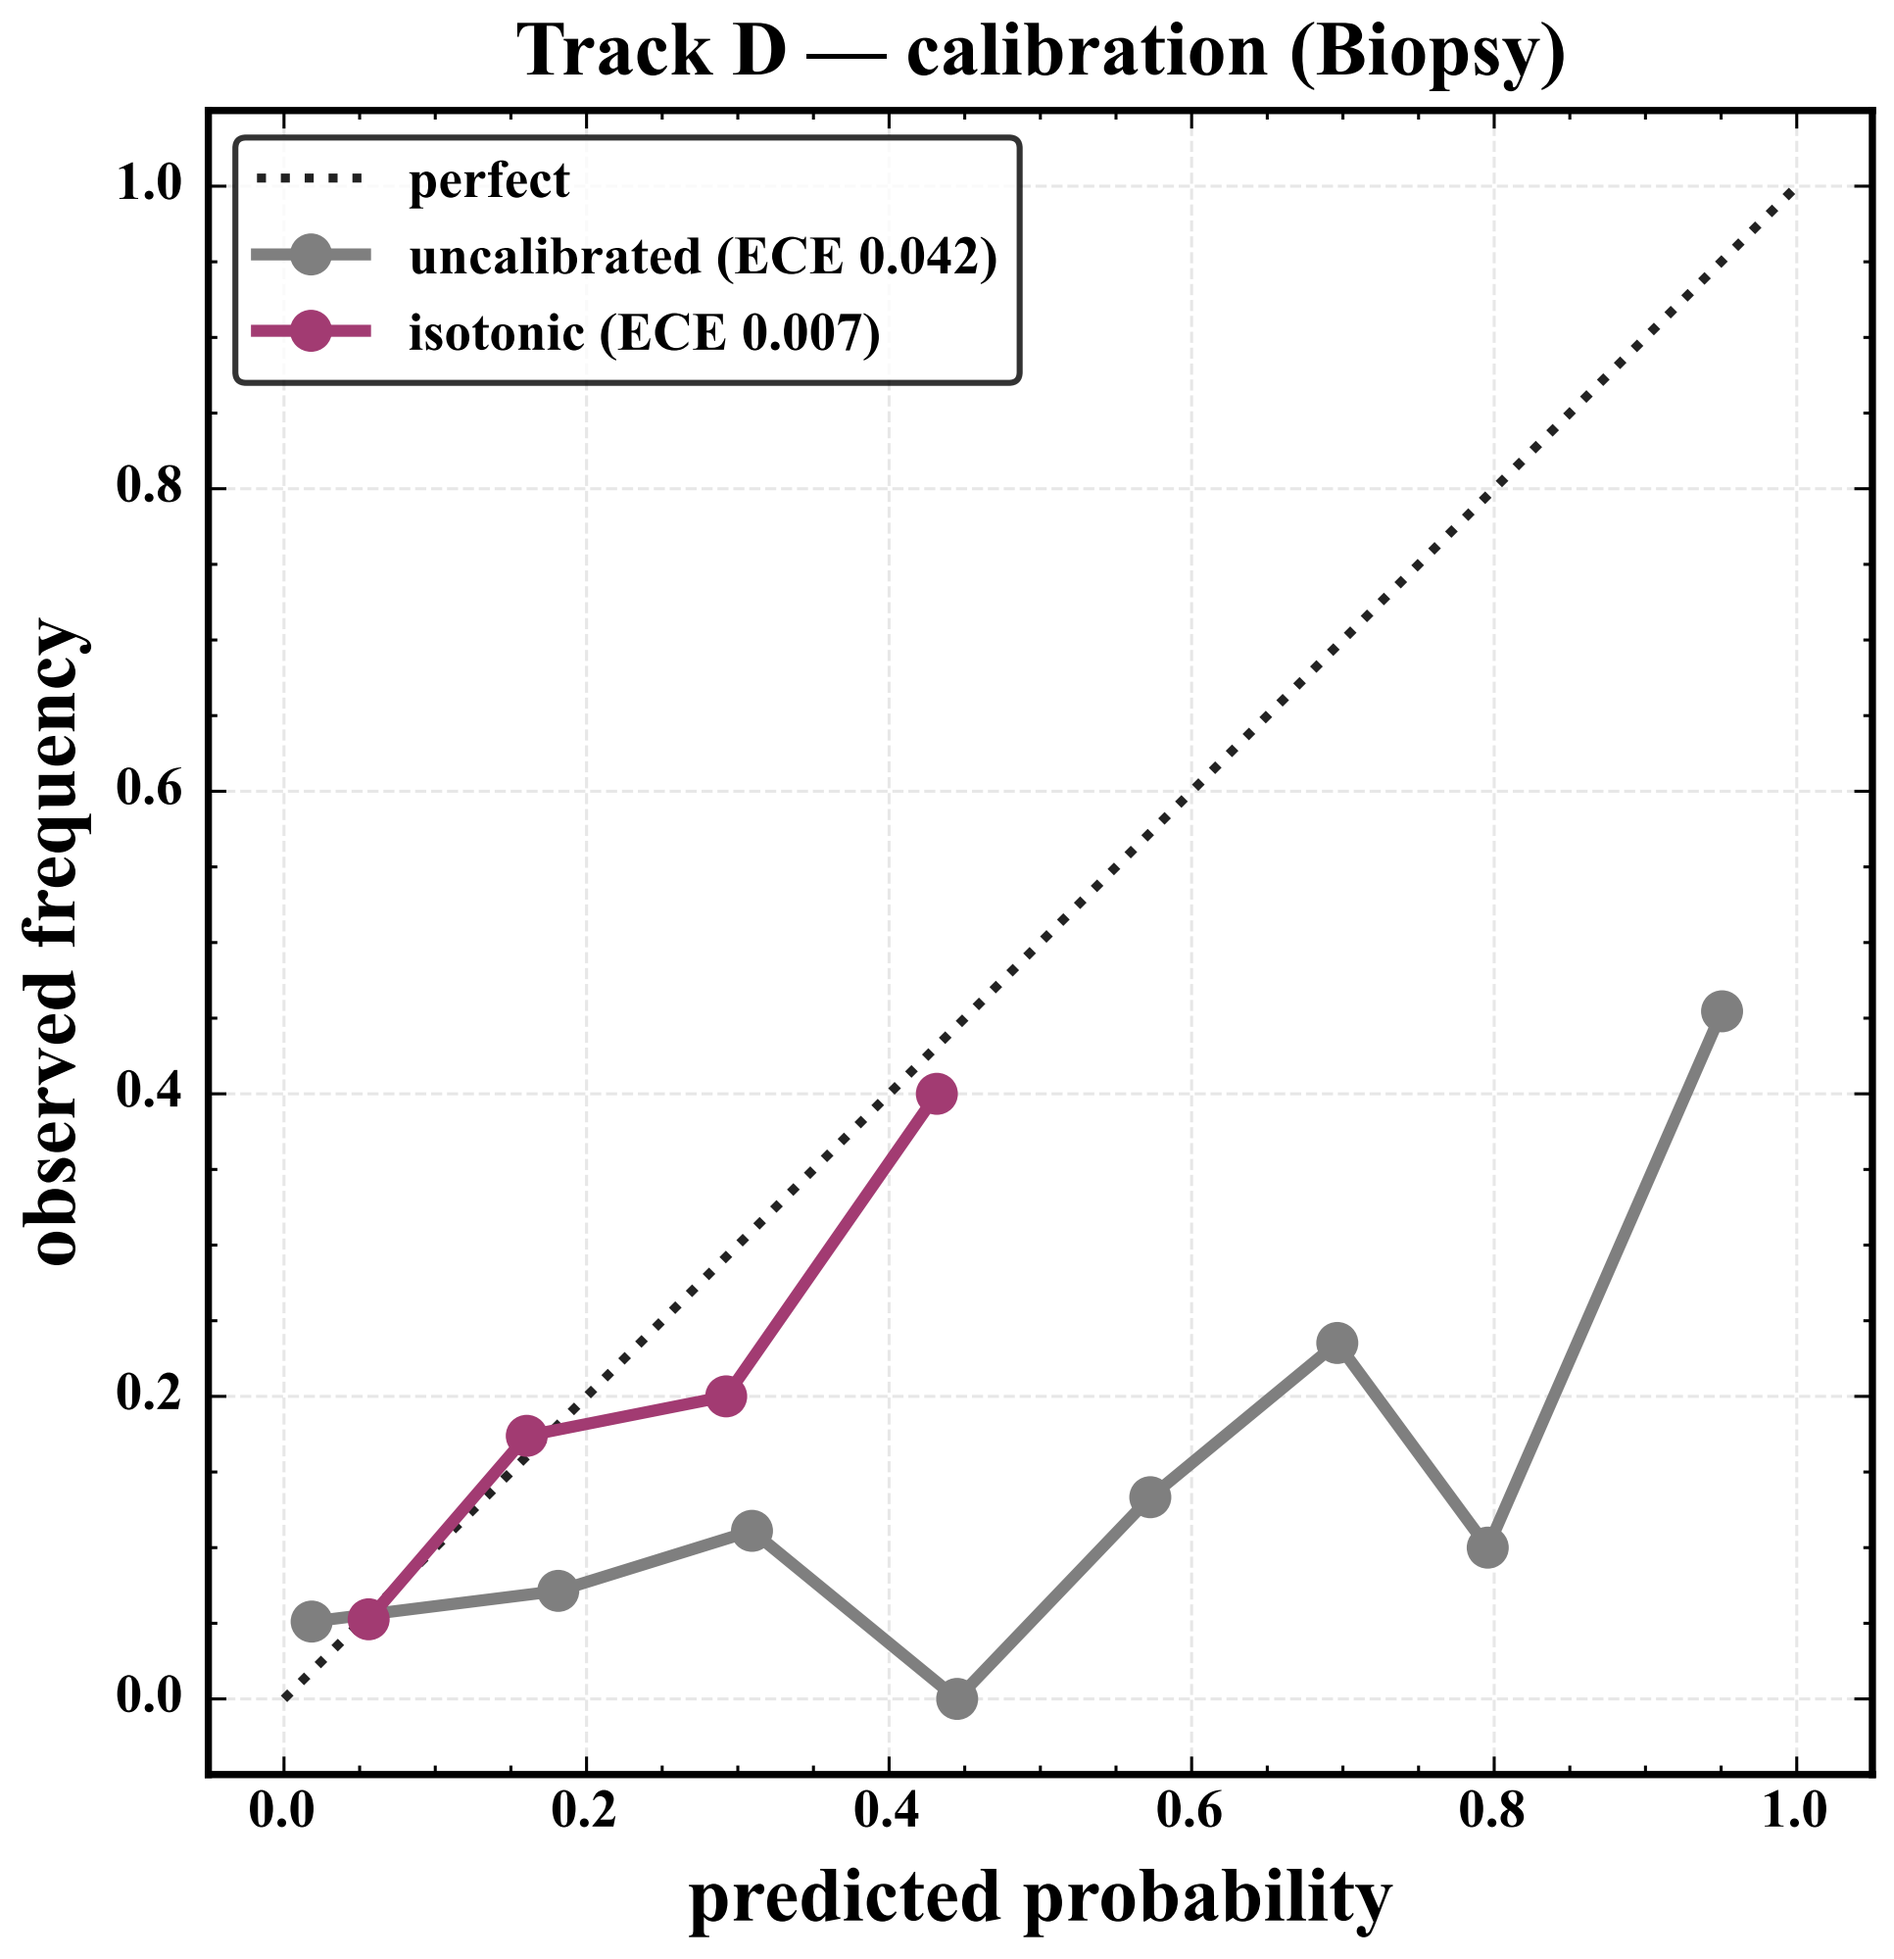
Track D — calibration (Biopsy)
perfect
uncalibrated (ECE 0.042)
isotonic (ECE 0.007)
observed frequency
predicted probability
0.0
0.2
0.4
0.6
0.8
1.0