LabelGuard AI — Label Inspection Report

STENT101 · Cardiac Stent · V1 → V2 · EU · English
Change request CHG-B38E: Sterilization update | Ruleset demo-ruleset-0.1
Approved label SHA-256: 195b101a4f1ae54529a91388… Revised label SHA-256: 420a9a72ec037f38546bcf5d…

Passed checks	Failed checks	Critical flags	Unexpected	Review flags	Expected
14	3	2	2	1	2

Outcome: REVIEW REQUIRED — do not release

Findings

LG-001 — Safety warnings: removed — **UNEXPECTED** · critical

Previous: WARNING: Do not reuse. Do not use if package is damaged.
New: —
Contract: Change request CHG-B38E explicitly protects this field.
Detected by: text, visual
Evidence: p1 text [30.0, 219.3, 315.6, 233.1]; p1 visual [24.0, 216.5, 321.1, 238.6]
Explanation: Safety warnings is missing on the revised label. Change request CHG-B38E explicitly protects this field.
Action: Verify the correct value against the source of truth and regenerate the candidate label if the change was not intended.
Rules: LG-CONTRACT-PROTECTED, LG-REQ-002

LG-002 — Unique Device Identification: modified — **UNEXPECTED** · critical

Previous: UDI: (01) 00812345678901
New: UDI: (01) 00812345678994
Contract: Change request CHG-B38E explicitly protects this field.
Detected by: barcode, text, visual
Evidence: p1 text [160.0, 339.2, 281.2, 353.0]; p1 barcode [36.5, 316.3, 133.4, 413.3]; p1 visual [264.0, 336.5, 287.0, 356.2]; p1 visual [37.4, 324.0, 132.5, 412.3]
Explanation: Unique Device Identification changed from 'UDI: (01) 00812345678901' to 'UDI: (01) 00812345678994'. Change request CHG-B38E explicitly protects this field. Barcode payload: 0100812345678901 → 0100812345678994.
Action: Verify the correct value against the source of truth and regenerate the candidate label if the change was not intended.
Rules: LG-CONTRACT-PROTECTED

LG-003 — Logo: moved — **REQUIRES_REVIEW** · minor

Previous: x=270.0, y=55.0
New: x=288.0, y=55.0
Contract: This field is not covered by the change request; insufficient evidence to accept the change.
Detected by: symbol, visual
Evidence: p1 symbol [288.0, 55.0, 378.0, 100.0]; p1 visual [266.4, 51.4, 378.7, 104.2]
Explanation: Logo moved (Shifted by (18.0, 0.0) pt). This field is not covered by the change request; insufficient evidence to accept the change.
Action: Reviewer to inspect the highlighted region and confirm whether the change is acceptable; document the rationale.
Rules: —


LG-004 — Sterilization statement: modified — **EXPECTED** · informational


Previous: Sterilized using ethylene oxide
New: Sterilized using irradiation
Contract: Change request CHG-B38E allows this field to change to 'radiation'.
Detected by: text, visual
Evidence: p1 text [140.0, 149.2, 254.5, 163.0]; p1 visual [205.0, 146.4, 280.8, 168.0]
Explanation: Sterilization statement changed from 'Sterilized using ethylene oxide' to 'Sterilized using irradiation'. Change request CHG-B38E allows this field to change to 'radiation'.
Action: No action required; confirm that the new value is correct for the target market.
Rules: LG-CONTRACT-ALLOWED

LG-005 — Sterilization symbol: modified — **EXPECTED** · informational

Previous: sterile_eo
New: sterile_radiation
Contract: Change request CHG-B38E allows this field to change to 'radiation'.
Detected by: symbol, visual
Evidence: p1 symbol [30.0, 130.0, 126.0, 190.0]; p1 visual [59.5, 158.4, 97.4, 184.3]
Explanation: Sterilization symbol changed from 'sterile_eo' to 'sterile_radiation'. Change request CHG-B38E allows this field to change to 'radiation'.
Action: No action required; confirm that the new value is correct for the target market.
Rules: LG-CONTRACT-ALLOWED

Visual comparison (approved → revised)

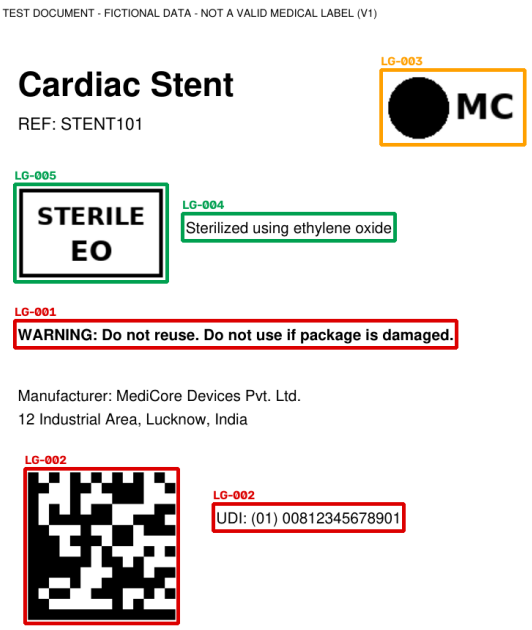

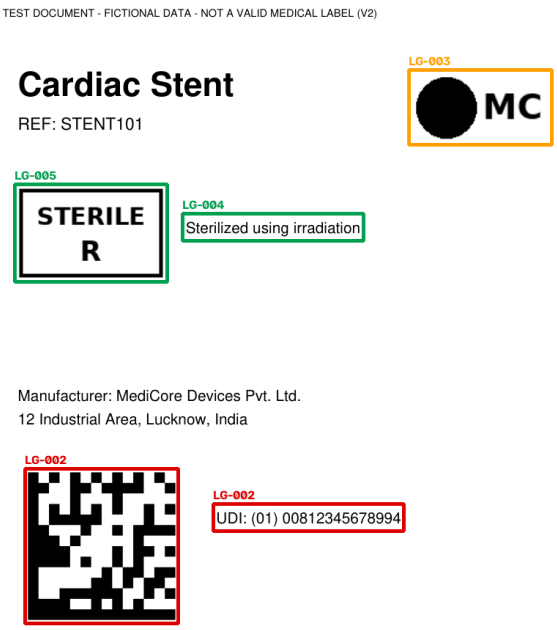

Validation checks

Check	Result	Detail
Requested change applied: Sterilization symbol	PASS	sterile_eo → sterile_radiation
Requested change applied: Sterilization statement	PASS	Sterilized using ethylene oxide → Sterilized using irradiation
Protected field unchanged: Unique Device Identification	FAIL	Unique Device Identification changed from 'UDI: (01) 00812345678901' to 'UDI: (01) 0081234
Protected field unchanged: Product identifier	PASS	No difference detected
Protected field unchanged: Manufacturer details	PASS	No difference detected
Protected field unchanged: Safety warnings	FAIL	Safety warnings is missing on the revised label. Change request CHG-B38E explicitly protec
Required element present: Unique Device Identification	PASS	
Required element present: Safety warnings	FAIL	Not found on revised label
Required element present: Manufacturer details	PASS	
Required element present: Sterilization symbol	PASS	
Required element present: Product identifier	PASS	
[approved] Barcode decodes to a GS1 GTIN	PASS	0100812345678901
[approved] GTIN check digit valid	PASS	00812345678901
[approved] Barcode matches printed UDI	PASS	barcode=00812345678901 printed=00812345678901
[revised] Barcode decodes to a GS1 GTIN	PASS	0100812345678994
[revised] GTIN check digit valid	PASS	00812345678994

[revised] Barcode matches printed UDI	PASS	barcode=00812345678994 printed=00812345678994

Review & approval history

No reviewer decision recorded yet.

Demo/test rules for prototype purposes only. Not a regulatory determination. The prototype validates against the supplied change contract and configured reference rules; it does not establish regulatory compliance. Approval must follow the organisation's controlled quality process.