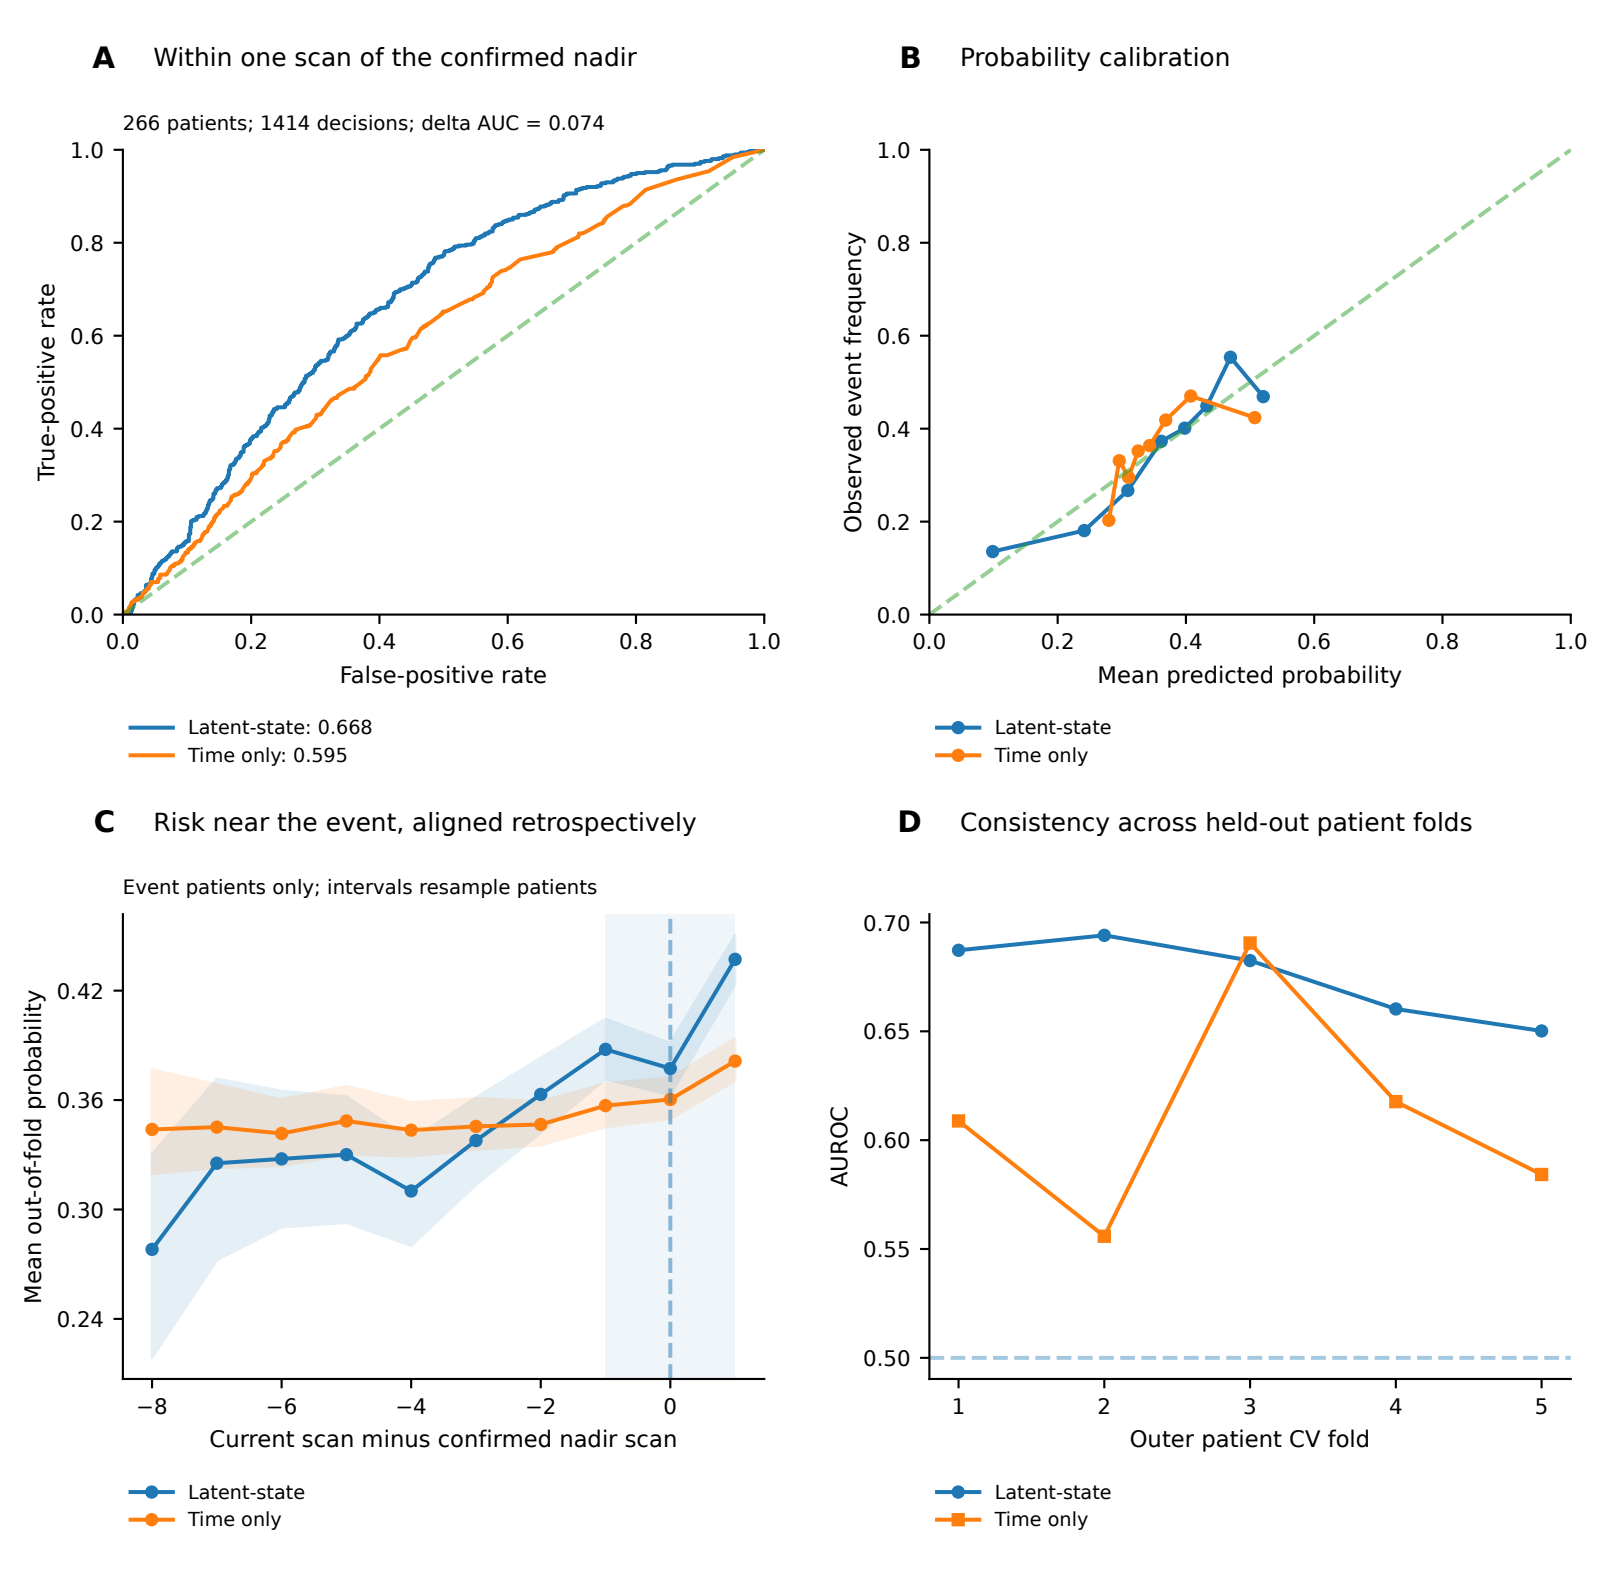
A
Within one scan of the confirmed nadir
266 patients; 1414 decisions; delta AUC = 0.074
True-positive rate
False-positive rate
Latent-state: 0.668
Time only: 0.595
B
Probability calibration
Observed event frequency
Mean predicted probability
Latent-state
Time only
C
Risk near the event, aligned retrospectively
Event patients only; intervals resample patients
Mean out-of-fold probability
Current scan minus confirmed nadir scan
Latent-state
Time only
D
Consistency across held-out patient folds
AUROC
Outer patient CV fold
Latent-state
Time only