


RETI^{animal}[®]

RETI-port/scan21

Made in Germany


mouse table · especially for examinations of animals

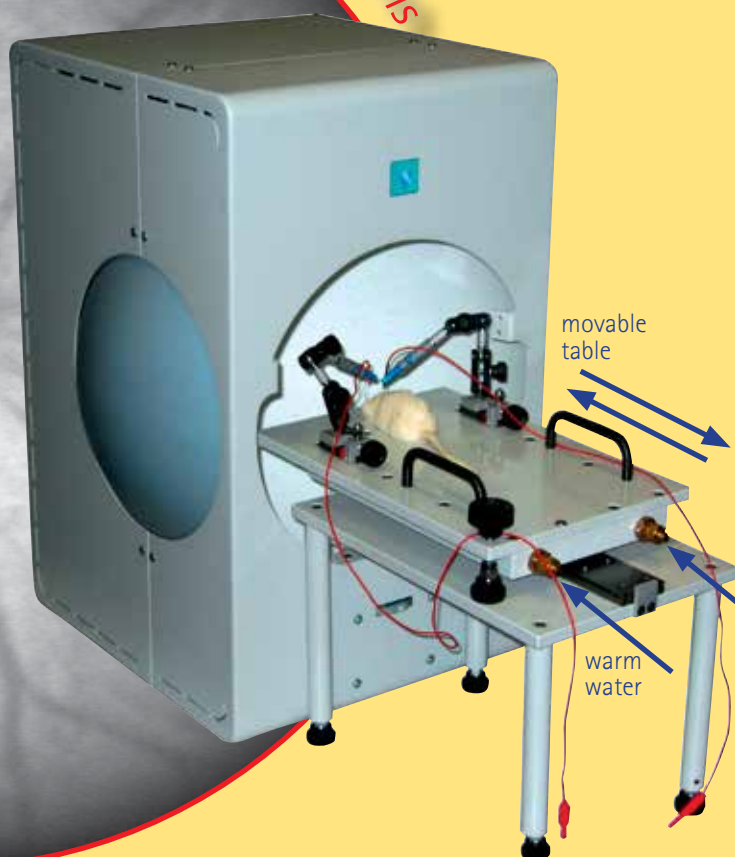

application



infrared monitoring

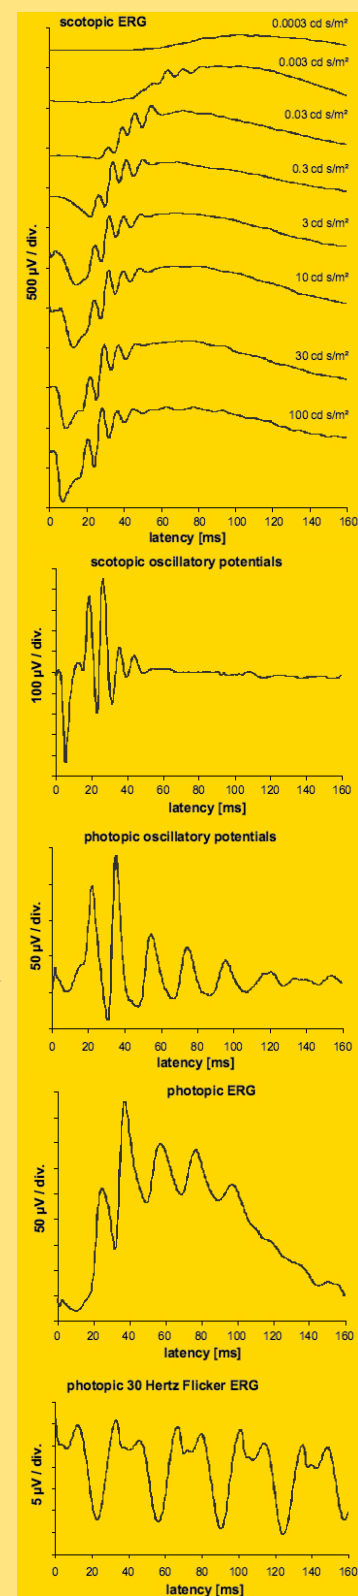

ROLAND CONSULT
Electrophysiology and Imaging

RETI^{animal}®

ISCEV Standard RETI-port/scan21

Made in Germany

Especially for examinations of animals, ROLAND CONSULT provides their customers with some tools. The Mouse Table is a heatable examination table for small animals. It is placed in front of a ROLAND CONSULT Ganzfeld and has two free moveable electrode holders. After the animal and the electrodes are placed, the table can be slid into the Ganzfeld.

Ganzfeld Q450 SC (super color)

- LEDs for Flash and Backlight: white and 5 different colors royal blue: 455nm, blue: 470nm, green 525nm, amber 590nm and red 625nm LED's for advanced flash and backlight
- ISCEV standard and more
- Full field globe d=400mm
- All function full computer controlled, USB connection
- Flash and Backlight with white LED:
Intensity Standard flash 3,0 cds/m²;
interval from - 40dB to +5dB in steps of 5
Background 25 cd/m², 100cd/m², 450cd/m²
- ON-OFF Response white Flash Time from 100ms-500ms in steps of 50ms
- Flash and Backlight with color LEDs
Flash intensity from -45 dB to 0dB in steps of 5 dB
Background 10 cd/m², 15 cd/m², 20cd/m², 25cd/m², 50cd/m²
- Option Xenon: Ganzfeld Q450 SCX
Xenon tube for white High Flash (option)
Intensity 10cds/m², 30cds/m², 100cds/m²
- Integrated infrared camera

Animal table with thermostat:

- Mouse table: Size: 20 x 30 cm, other sizes are possible!
Heating platform with warm water connection to keep the animal warm

Operating unit:

- Windows 7 or higher
- PC Processor: Intel i5 or better
- DVDRW for database backup
- Keyboard, mouse
- 24" TFT monitor
- Color printer
- Bio signal amplifier 4 channel
- Digital controlled amplifier
- Impedance 2 x 100 MOhm
- Noise <4µV(SS)
- Common mode reaction <110 dB
- Sensitivity 10µV/Div to 2 mV/Div
- High pass 0,02 Hz to 1 kHz
- Low pass 20 Hz to 10 kHz

Distributor:

UV-LEDs optional

Wavelength: 360nm
Flash intensity range up to 0,000005 mWs/m² up to 7,2 mWs/m²
adjustable in steps of 0,000005 mWs/m²
Up to 4,8 mWs/m² adjustable in steps of 0,000005 mWs/m² UV-
Background light
Range: Up to 480 mW/m² adjustable in steps of 1 mW/m²

Option: RETImap® connected with RETI^{animal}® system

Technical Data

Laser Scanning System:

Field of view:

35° x 35°

Digital image size:

512 x 512 Pixel

Digital image depth:

12 bit max. image frequency: 15 Hz

Optical resolution: 30 µm

Laser Sources:

IR: SLD 920 nm (IR Image)

Blue: 488 nm

(FA-Fluorescein Angiography / GFP)

Stimulation System: DLP projector


Field of View: 25° x 25°

Brightness: ca. 200 cd/m²

Vertical frequency: 60 Hz

Resolution: 800 x 600 pixel

Test Protocols: focal ERG,
multifocal ERG, Flash VEP
and Pattern VEP

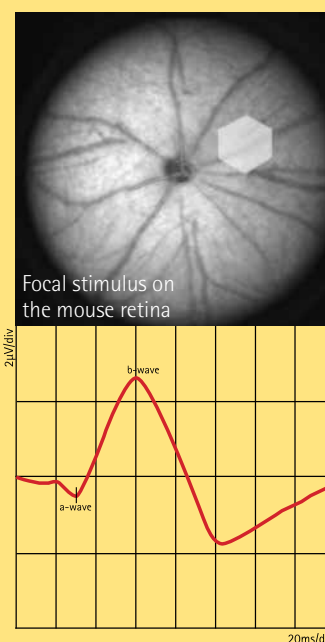

ROLAND CONSULT
Electrophysiology and Imaging



Roland Consult Stasche & Finger GmbH
Heidelberger Straße 7, 14772 Brandenburg an der Havel,
Germany
Phone: +49 (0)3381.8901034, Fax: +49 (0)3381.8902994
www.roland-consult.de, e-mail: info@roland-consult.de