Singulator™ 200 QuickStart Guide

Power on the instrument, then the tablet and complete the calibration prior to use. For details, see the Singulator™ 200 System *'Singulator 200 Manual'.*

1. Select **Left** or **Right** Sample Bay as desired, *then* select the User and log in (Fig.1).
2. From the '**User Home Screen'**, Select '**Run a Protocol'** (Fig. 2).

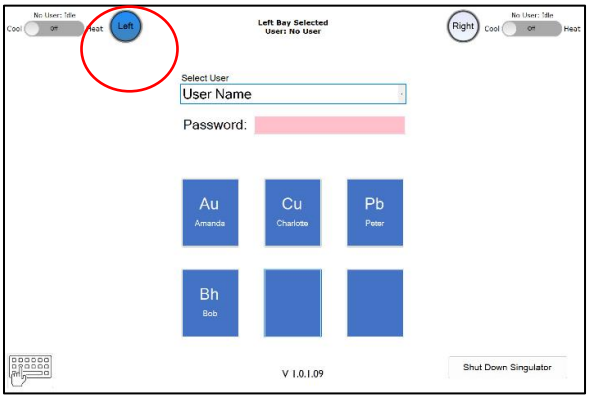


*Figure 1. User Log In Screen. Select **Left** or **Right** Sample Bay, **then** select User and then enter password.*

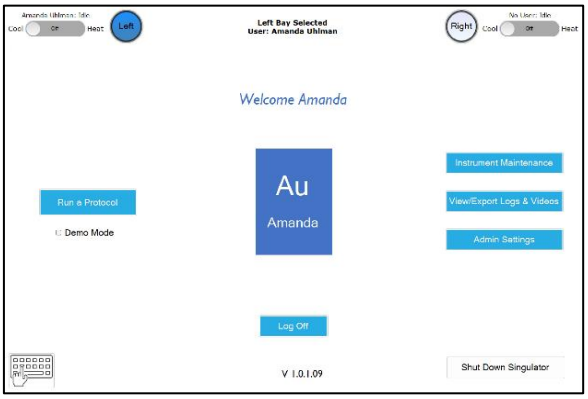


Figure 2. User Home Screen. Select 'Run a Protocol' to proceed to a run or choose 'Instrument Maintenance'.

3. On the '**Select Protocol**' screen, click '**Cells'** or '**Nuclei'** (Fig. 3).
4. If desired, Pre-cool or Pre-heat the Sample Bay by sliding the toggle to '**Cool'** or '**Heat'** and tap the icon to initiate the pre-cooling or pre-heating (Fig. 4).

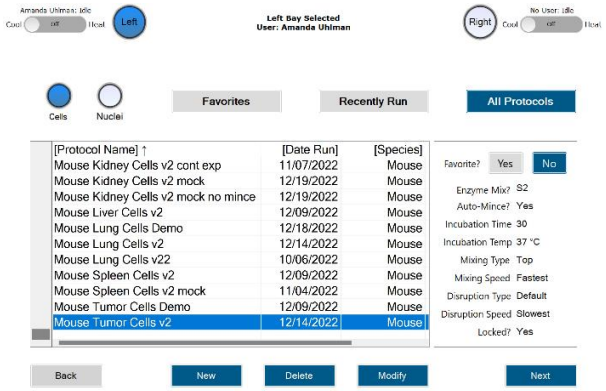


Figure 3. Select Protocol Screen showing all cell protocols. Precooling selected, but not activated.




Figure 4. Precool or Preheat slider. Top, Heat selected but not activated. Middle, Heat activated after center of slider clicked. Bottom, heating complete.

5. Select the desired protocol and click '**Next'**.
6. (OPTIONAL) On the '**Run Notes**' screen (Fig. 5), enter information as desired. Select '**Next'**.

> If the Singulator has not reached the pre-set temperature, a pop-up box (Fig. 6) will show a progress bar with time remaining. **Wait** until the system is at the set temperature (the pop-up box disappears), select '**Skip'** to proceed with the run immediately**,** or '**Cancel Run'**.

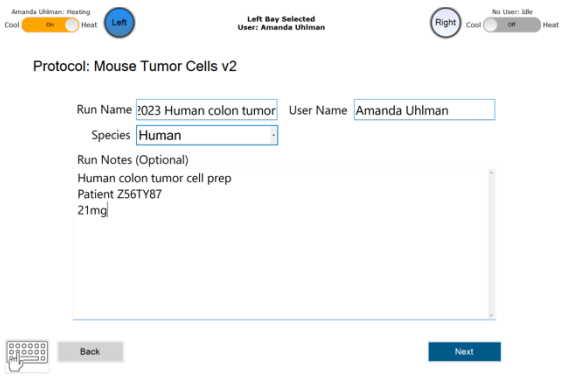


Figure 5. Run Notes Screen. Information will be saved in the run log (optional).

7. **Cell Isolations**: In the appropriate **left** or **right** Single-Shot Mechanism, place a 15 mL conical

For Research Use Only. Not for human or animal diagnostic or therapeutic use.

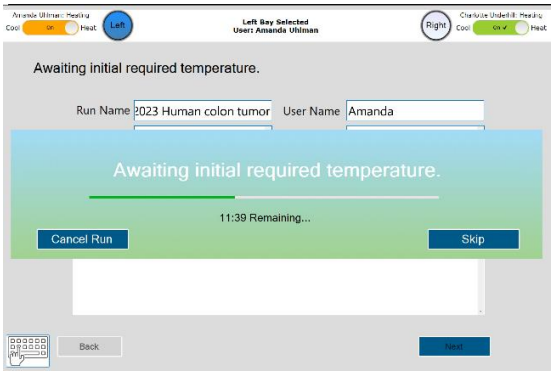


Figure 6. Pop-up box warning that the requested temperature has not been reached.

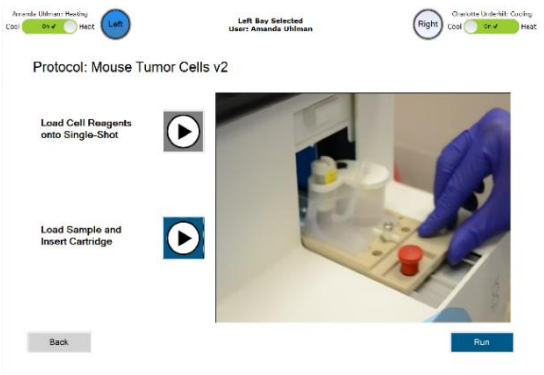


Figure 7. Instruction Screen for starting a cell run.

tube with 6 mL buffer in the LEFT position and a tube with 3 mL of enzyme cocktail in the RIGHT position, slide the red knob up until locked in place. Remove the cartridge cap, place the sample into the Dissociation Chamber, replace the cap. Place the cartridge onto the Cartridge Tray, rotate the lock counterclockwise, and slide the Cartridge Tray into the instrument until the red knob clicks in place (Fig. 7).

Nuclei Isolations: Check reagent levels in the Reagent Chiller. Remove the cartridge cap, place the sample into the Dissociation Chamber, and replace the cap. Place the cartridge onto the Cartridge Tray, lock, and slide the Cartridge Tray into the instrument until the red knob clicks into place (Fig. 7). For using the Single Shot to load reagents for nuclei, refer to the User Manual.

QUICK TIP

WARNING Do not hold the red knob while inserting the Cartridge Tray. Push the Cartridge Tray from behind until the red knob drops. Never insert fingers past the chamber door.

8. Press **Run** to execute the protocol. A '**Run Time Screen'** will appear (Fig. 8)
9. When the run finishes, the '**Run Complete**' screen (Fig. 9) will appear. Raise the door, lift the red knob, and slide the Cartridge Tray out of the instrument. Close the door. Rotate the cartridge lock clockwise and remove the cartridge from the Cartridge Tray.

CAUTION Do NOT attempt to open the instrument door until the "Run Completed" alert appears.

10. Selecting '**Finish'** will take you back to the '**User Home Screen**'.



Figure 8. Run Time Screen showing protocol selected, progress bar, run log, and the ABORT button.

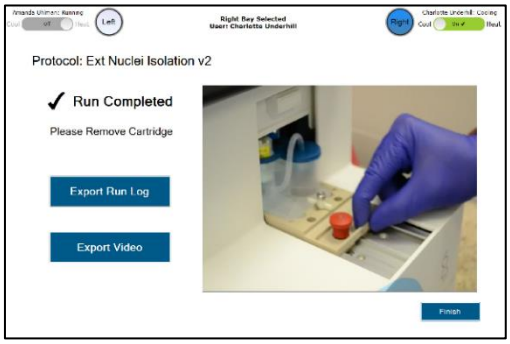


Figure 9. Run Complete screen. Video will show how to remove the cartridge.

For Research Use Only. Not for human or animal diagnostic or therapeutic use.