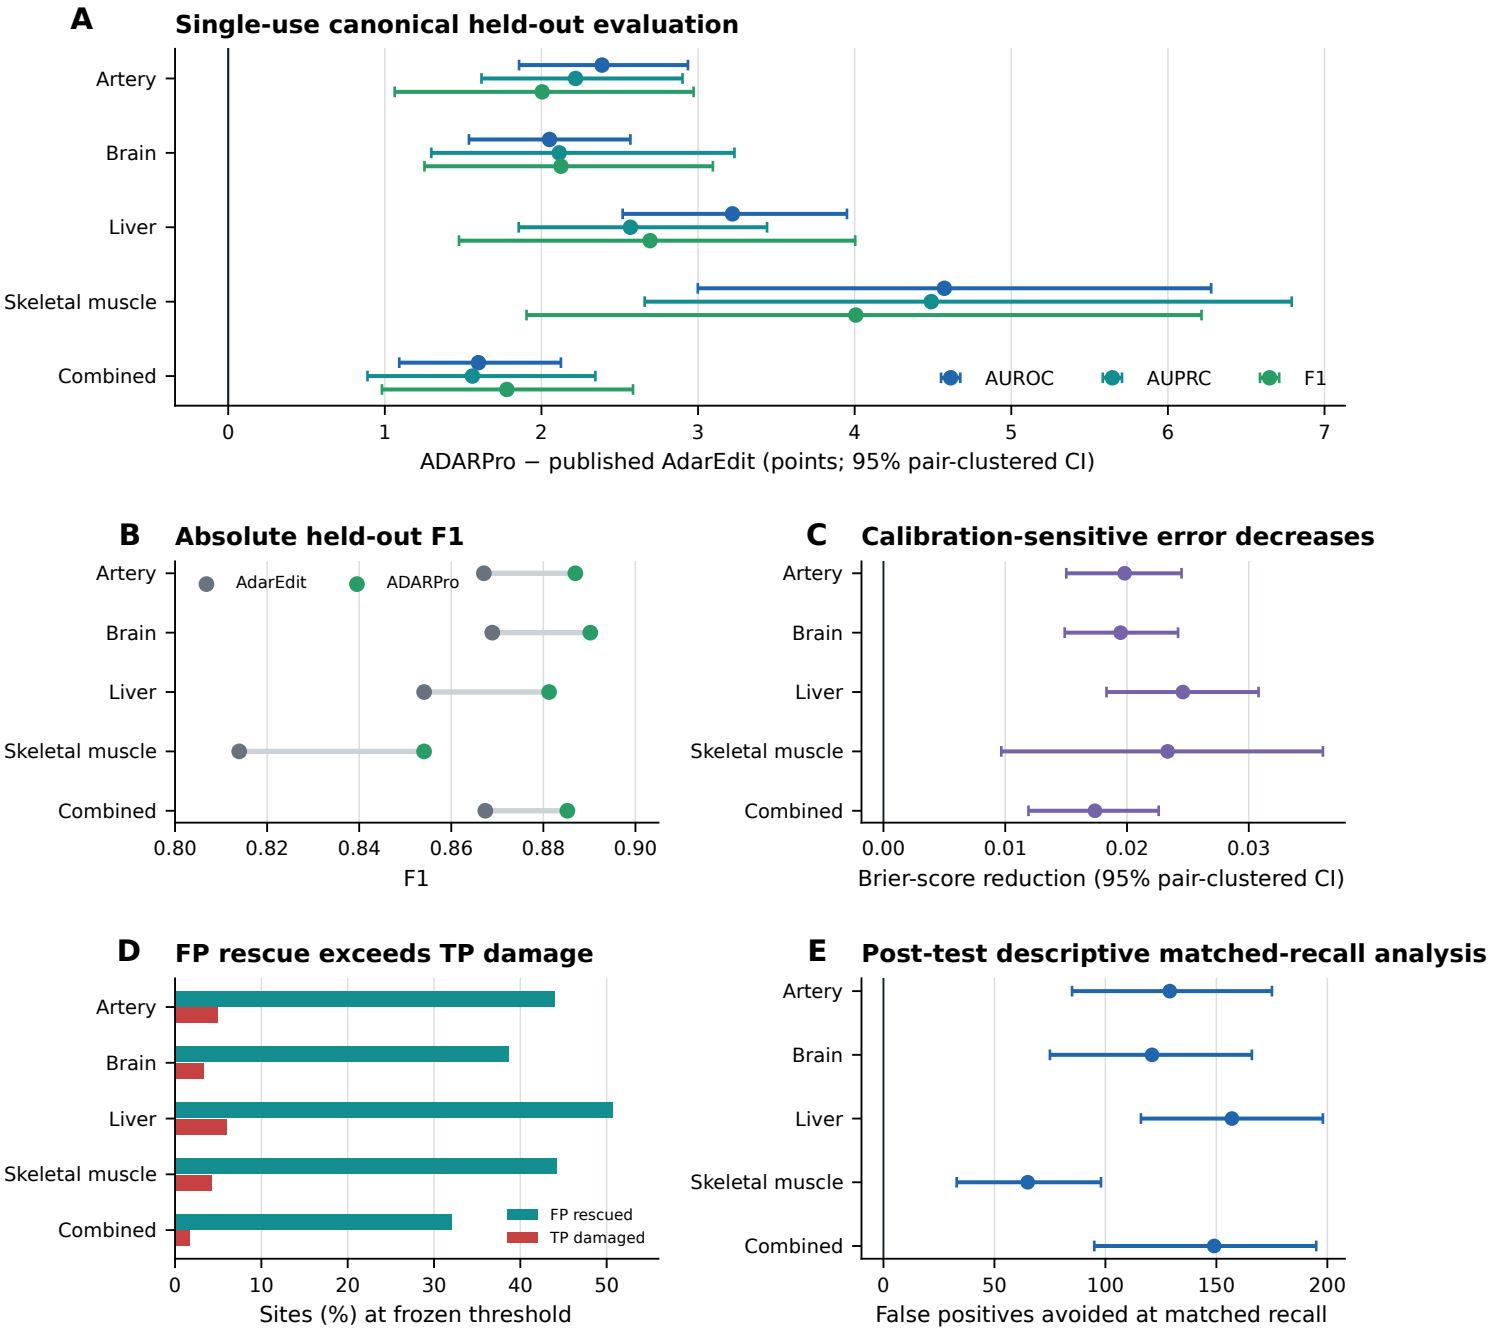
A
Single-use canonical held-out evaluation
Artery
Brain
Liver
Skeletal muscle
Combined
AUROC
AUPRC
F1
0
1
2
3
4
5
6
7
ADARPro − published AdarEdit (points; 95% pair-clustered CI)
B
Absolute held-out F1
AdarEdit
ADARPro
0.80
0.82
0.84
0.86
0.88
0.90
F1
C
Calibration-sensitive error decreases
0.00
0.01
0.02
0.03
Brier-score reduction (95% pair-clustered CI)
D
FP rescue exceeds TP damage
FP rescued
TP damaged
0
10
20
30
40
50
Sites (%) at frozen threshold
E
Post-test descriptive matched-recall analysis
0
50
100
150
200
False positives avoided at matched recall