


Date: New Acquisition: 81_2 (Manual) 03 July 2019 15:08:43 Cal: Named Calibration "190619_CHCApexA" by MALDI Solutions Admin on 19 June 2019 16:01:24 (Original)

Shin adzu MALDI-8020: Tuning Linear, Power 60, P Ext a: 66000.00 (b n 628)

Processed data (averaged: 32.5 mv (sum=824.1 mV), Smoothed=33, profiles # 1-200)

B S A

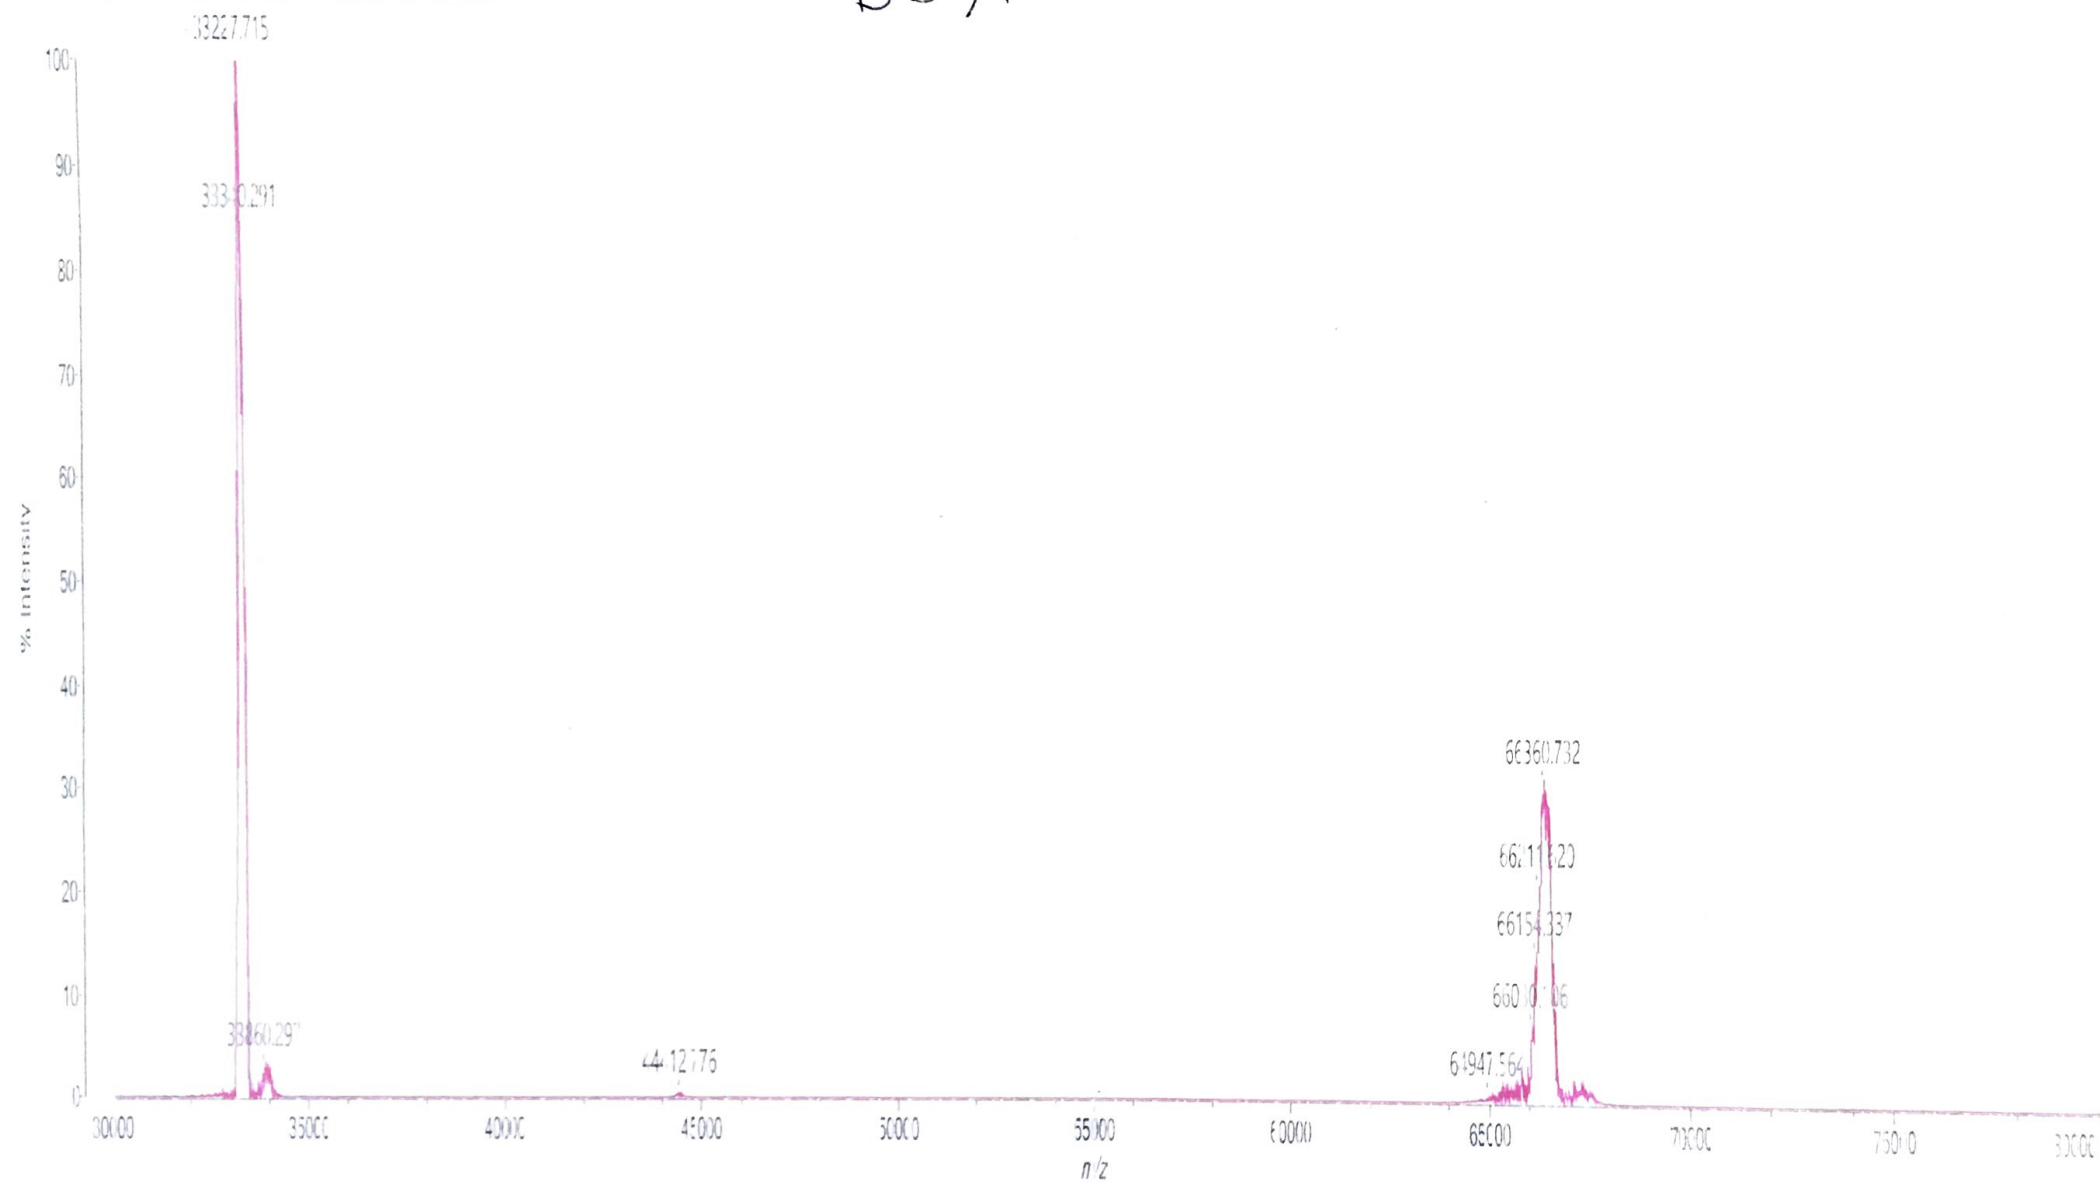


Data: New Acquisition 79142 (Manual) 19 July 2019 15:01:04. Cal: Named Calibration "150619_CHCA_pecA" by MA.DISolutionsAdmin on 19 June 2019 16:01:24 (Original)

Shimadzu MALDI-8020: Tuning: Linear, Power 30, P Ext at 14500.00 (bin 25.2)

Processed data (averaged): 49.7 mV [sum=1256.3 mV] Smoothed = 30, profiles # 1 - 210


lysozyme

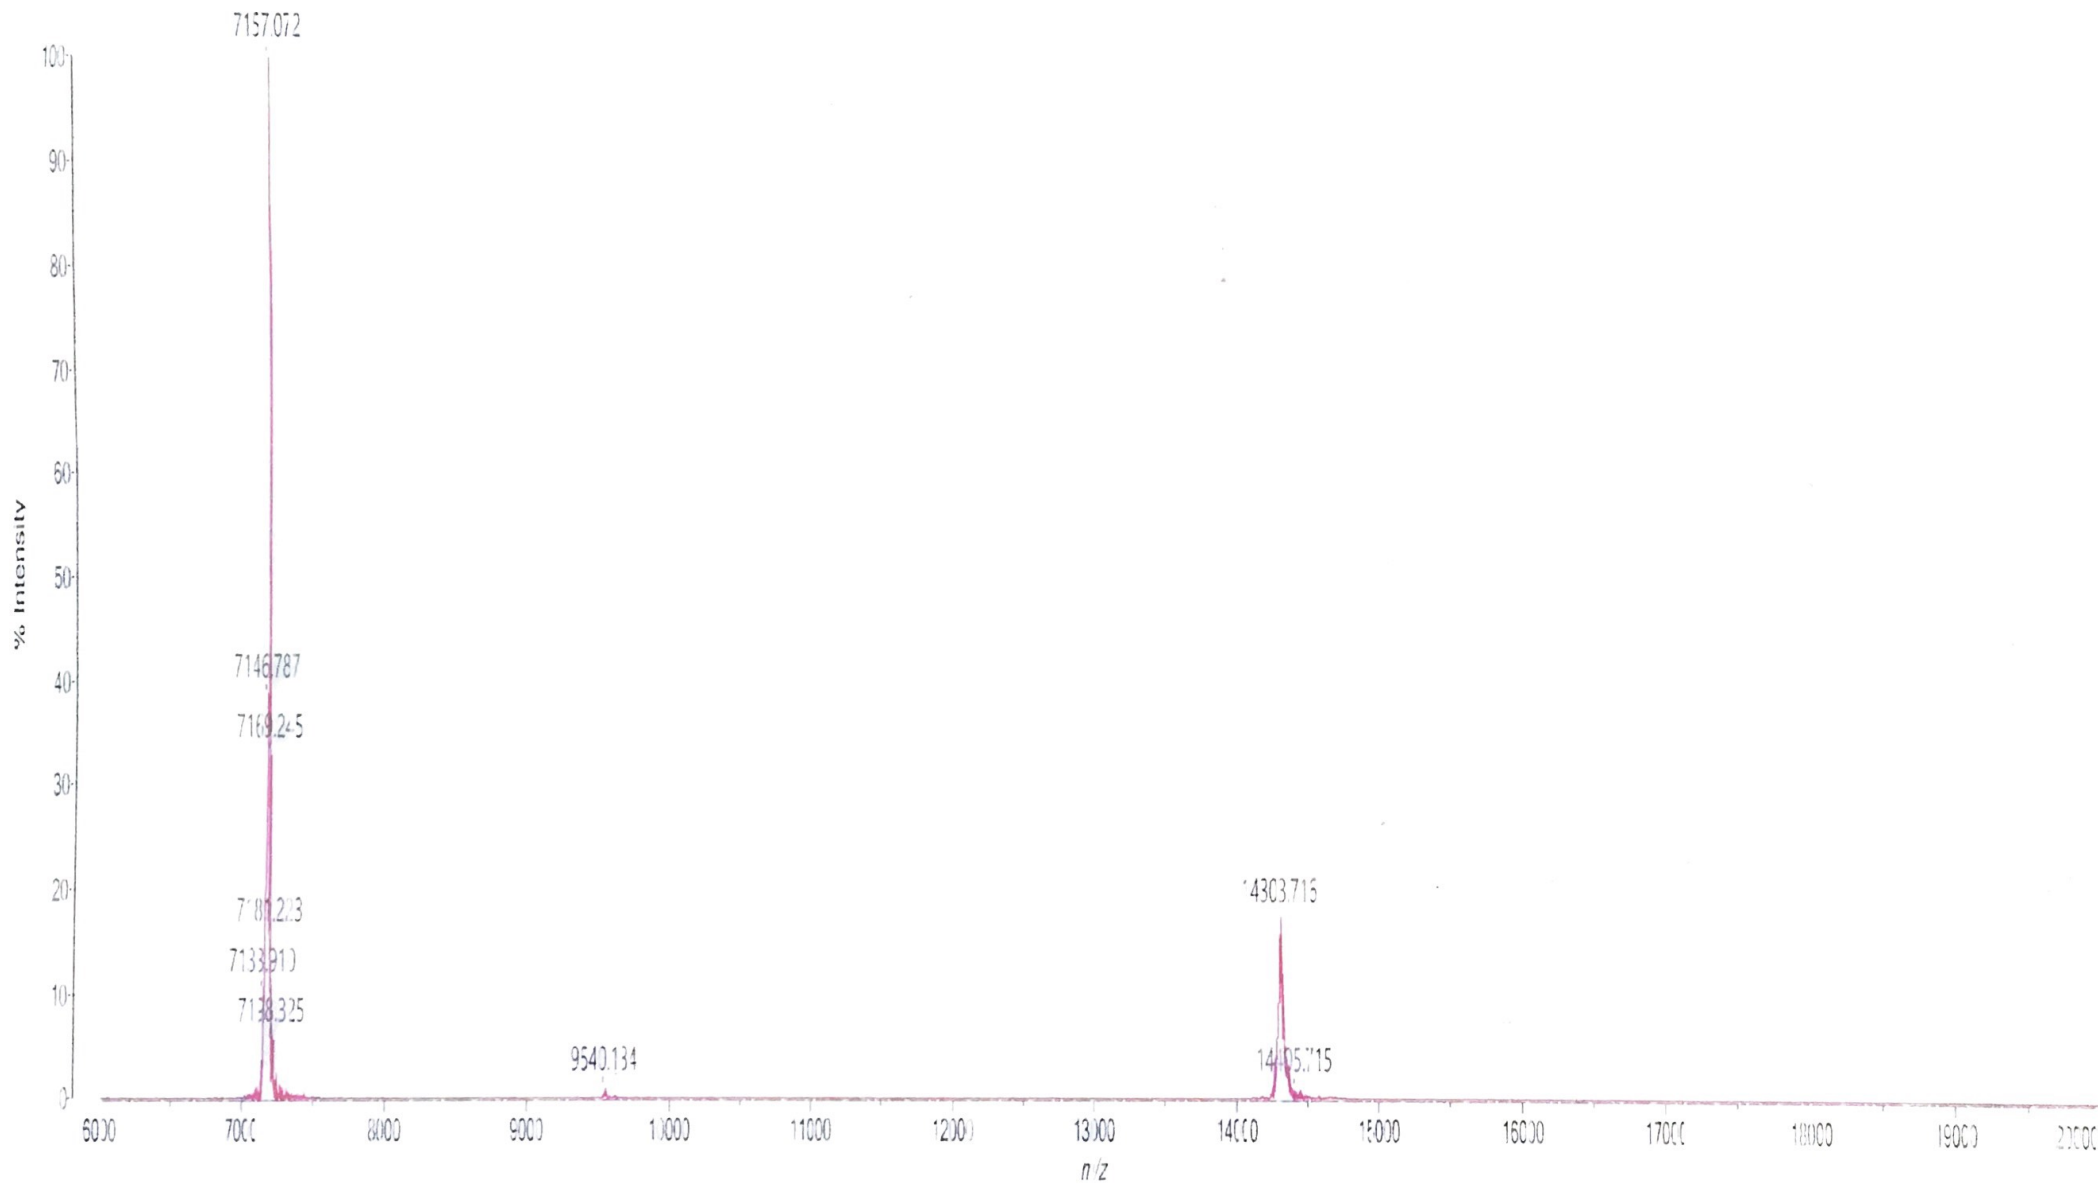

Date: New Acquisition: 8C12 (Manual) 09 July 2019 15:07:00 Cal: Named Calibration "190619_CHCAppA" by: MALDI Solutions Admin on 19 June 2019 16:01:24 Original
Shimadzu MALDI-8020: Furing Linear, Power 60, P Extra: 26000.00 (bin 354)

Processed data (averaged): 23.3 mV (sum=589.6 mV) Smoothed: 30, profile: # 1 - 200

YUH

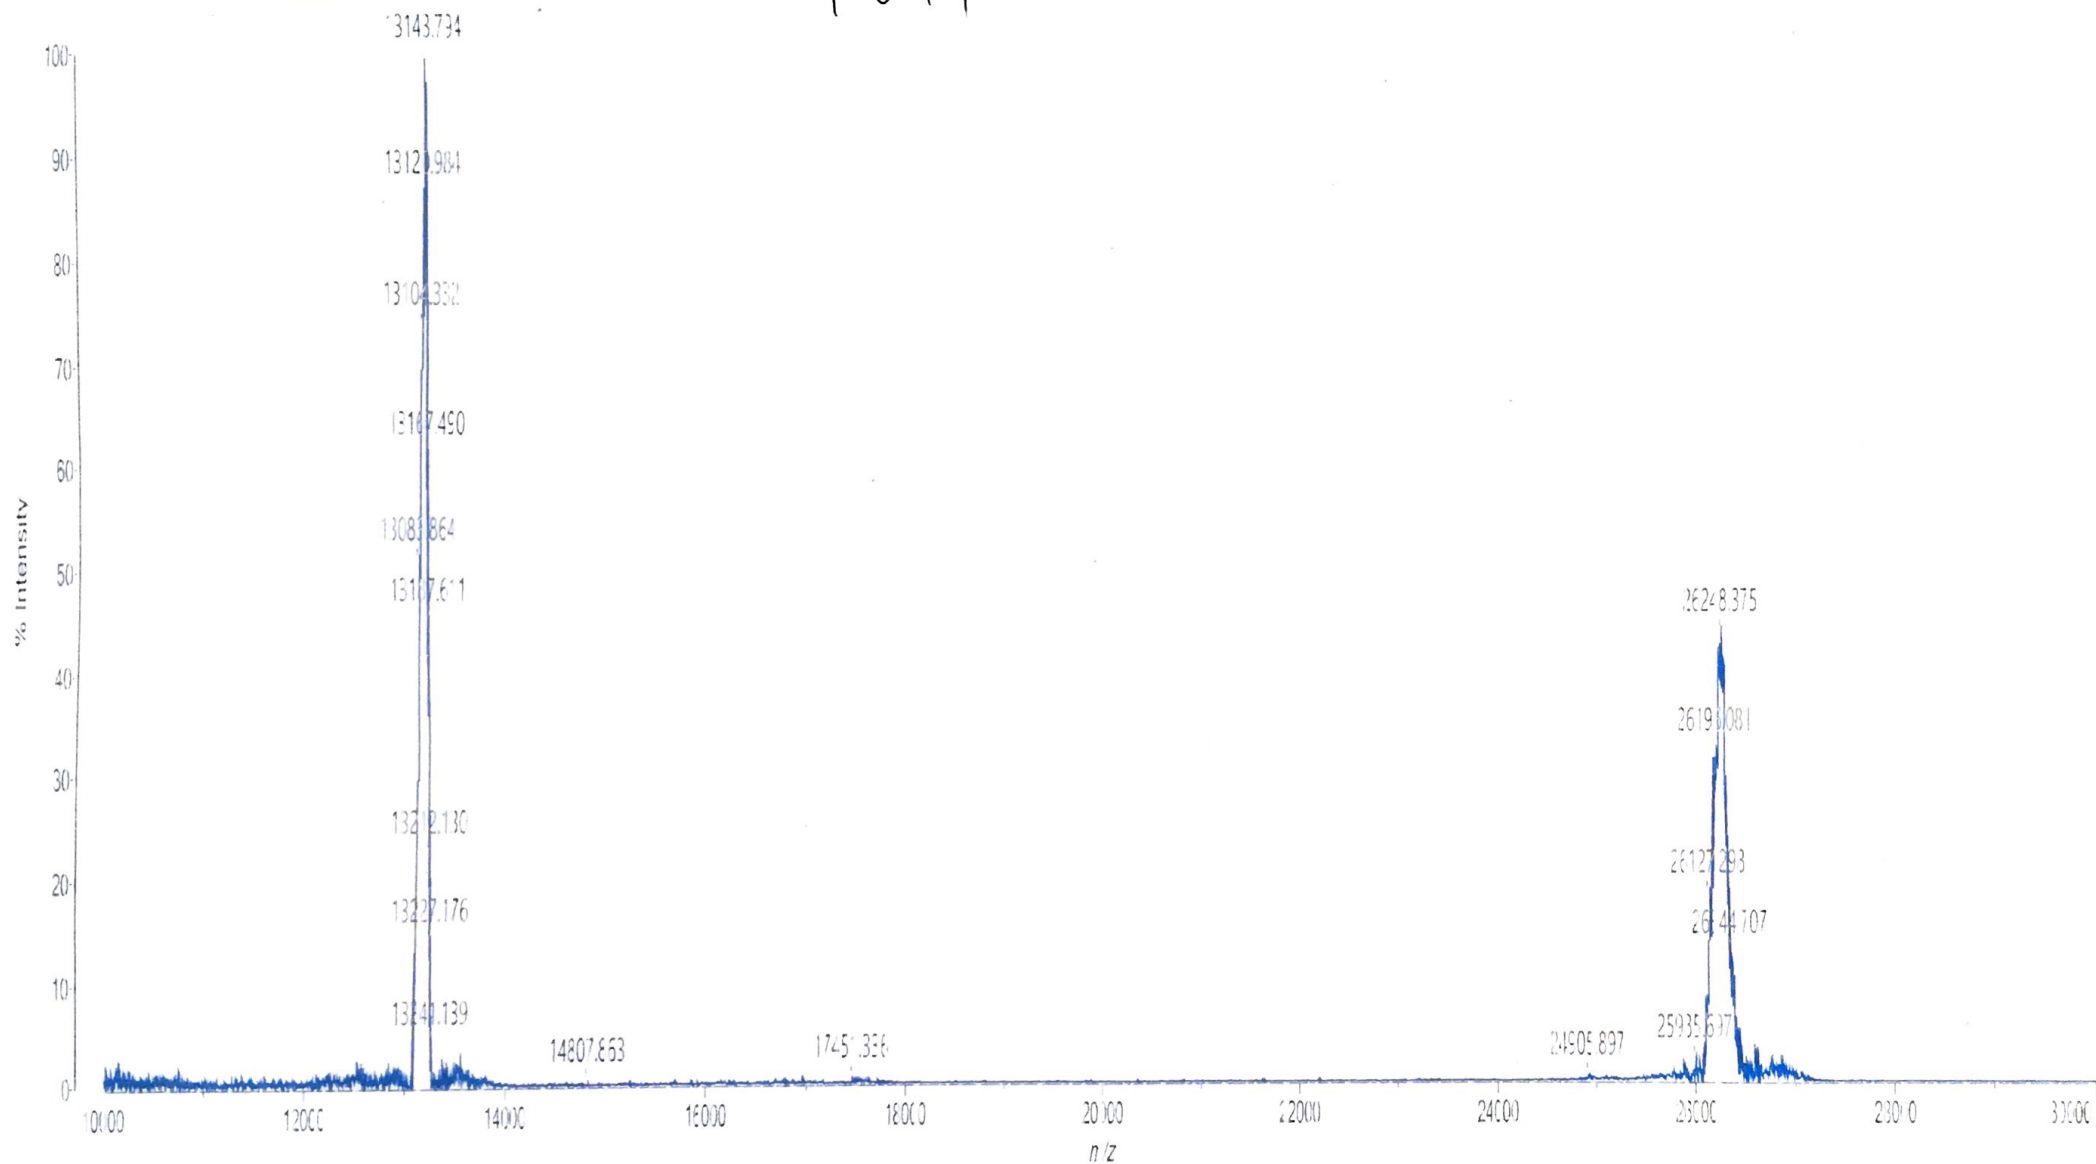


2H 15N Ub

Date: New Acquisition 78152 (Manual) 19 July 2019 14:51:51 Cal: Name: Calibration "150513_CHCA_RepA" by MA.DI.Solutions Admin on 19 June 2019 16:01:24 (Original)

Shimadzu MALDI-8020: Turin; Linear; Power 30; P Ext a: 860000 (b: 220)


Processed data (averaged): 22.5 mv (sum=572.1 mV) Smoothed: 3; profile: # 1 - 200

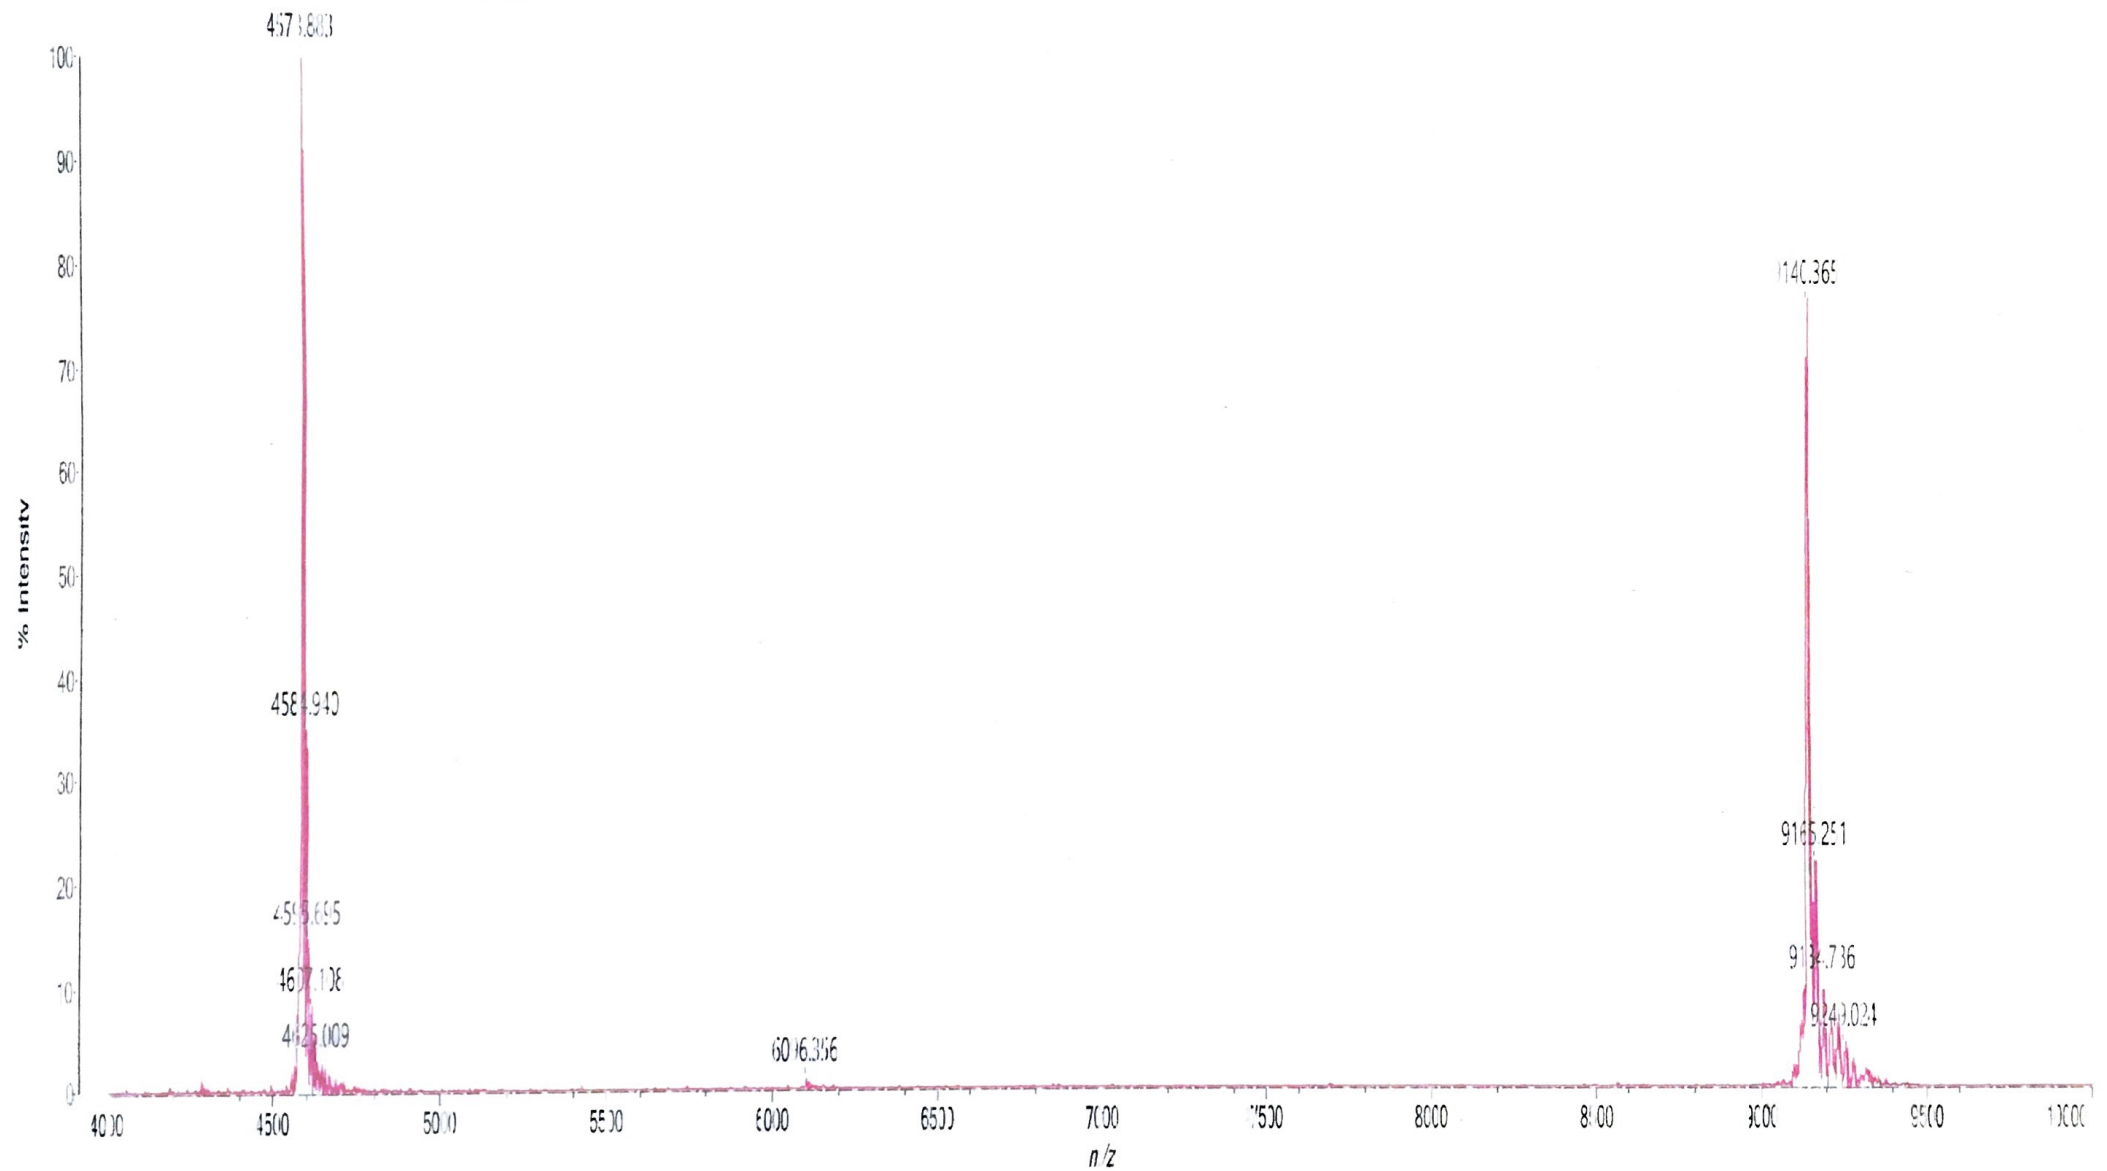

¹⁵N 26

Data: New Acquisition 77.F2 (Manual) 09 July 2019 14:50:52 Cal:Named Calibration "190619_CHCApepA" by MALDI Solutions Admin on 19 June 2019 16:01:24 (Original)
Shimadzu MALDI-8020: Tuning Linear, Power 30, P Ext at 8600.00 (bin 226)

Processed data (averaged) - 3.8 mV (sum=95.4 mV), Smoothed = 30, profiles # 1 - 200

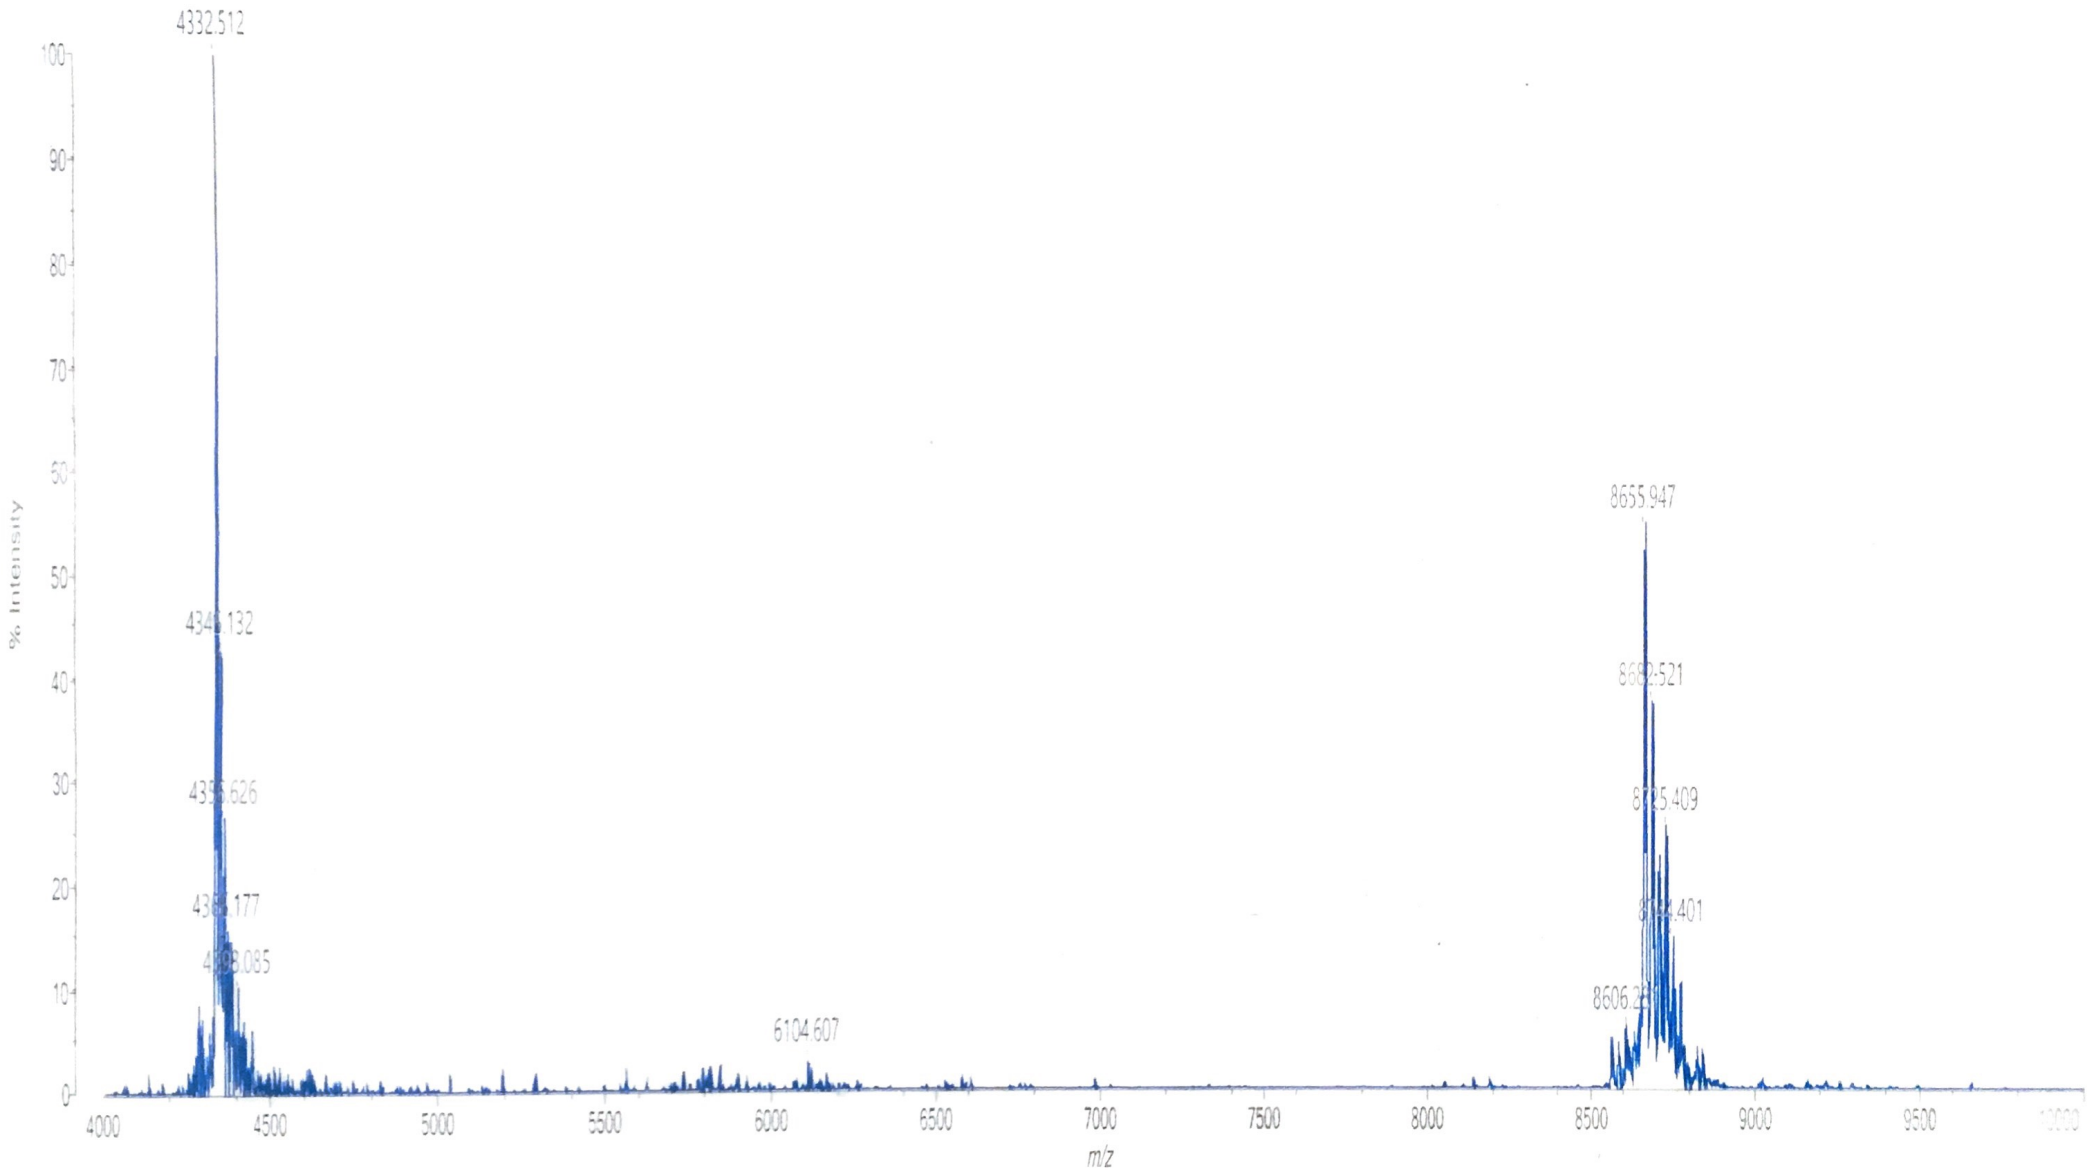


Ub

Data: New Acquisition 76:E2 (Manual) 09 July 2019 14:47:15 Cal:Named Calibration "190619_CHCApepA" by MALDI Solutions Admin on 19 June 2019 16:01:24 (Original)


Shimadzu MALDI-8020; Tuning: Linear, Power 30, P.Ext at 8600.00 (bin 226)

Processed data (averaged): 72.7 mV (sum=1837.9 mV), Smoothed = 30, profiles # 1 - 200

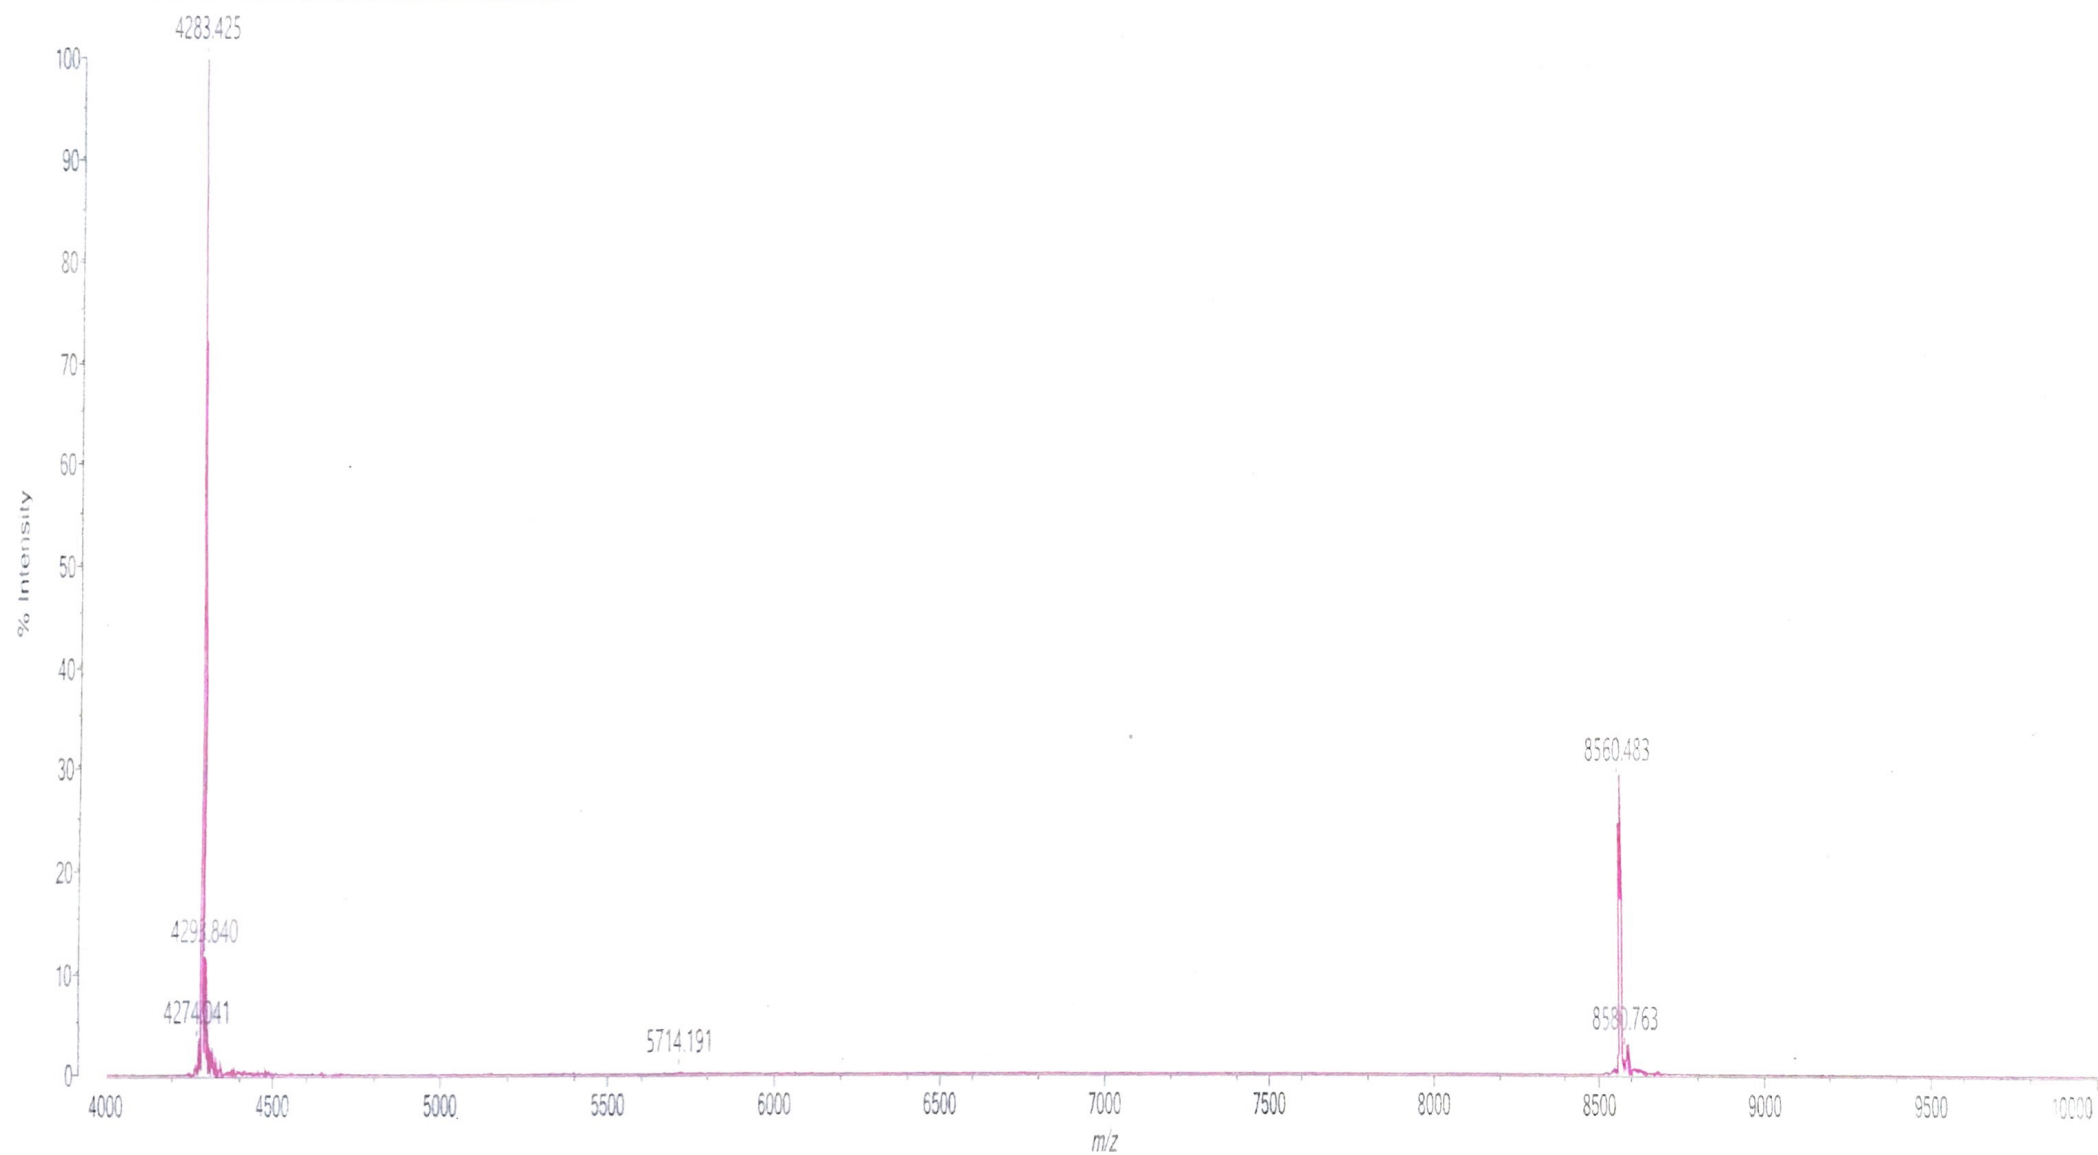

APF R トリプシン処理 24h

Data: New Acquisition 75.D2 (Manual) 09 July 2019 14:38:48 Cal:Named Calibration "190619_CHCApepA" by MALDI Solutions Admin on 19 June 2019 16:01:24 (Original)
Shimadzu MALDI-8020: Tuning Linear, Power 30, P.Ext at 700.00 (bin 64)
Processed data (averaged): 1433.6 mV (sum=36267.5 mV), Smoothed = 30, profiles # 1 - 200

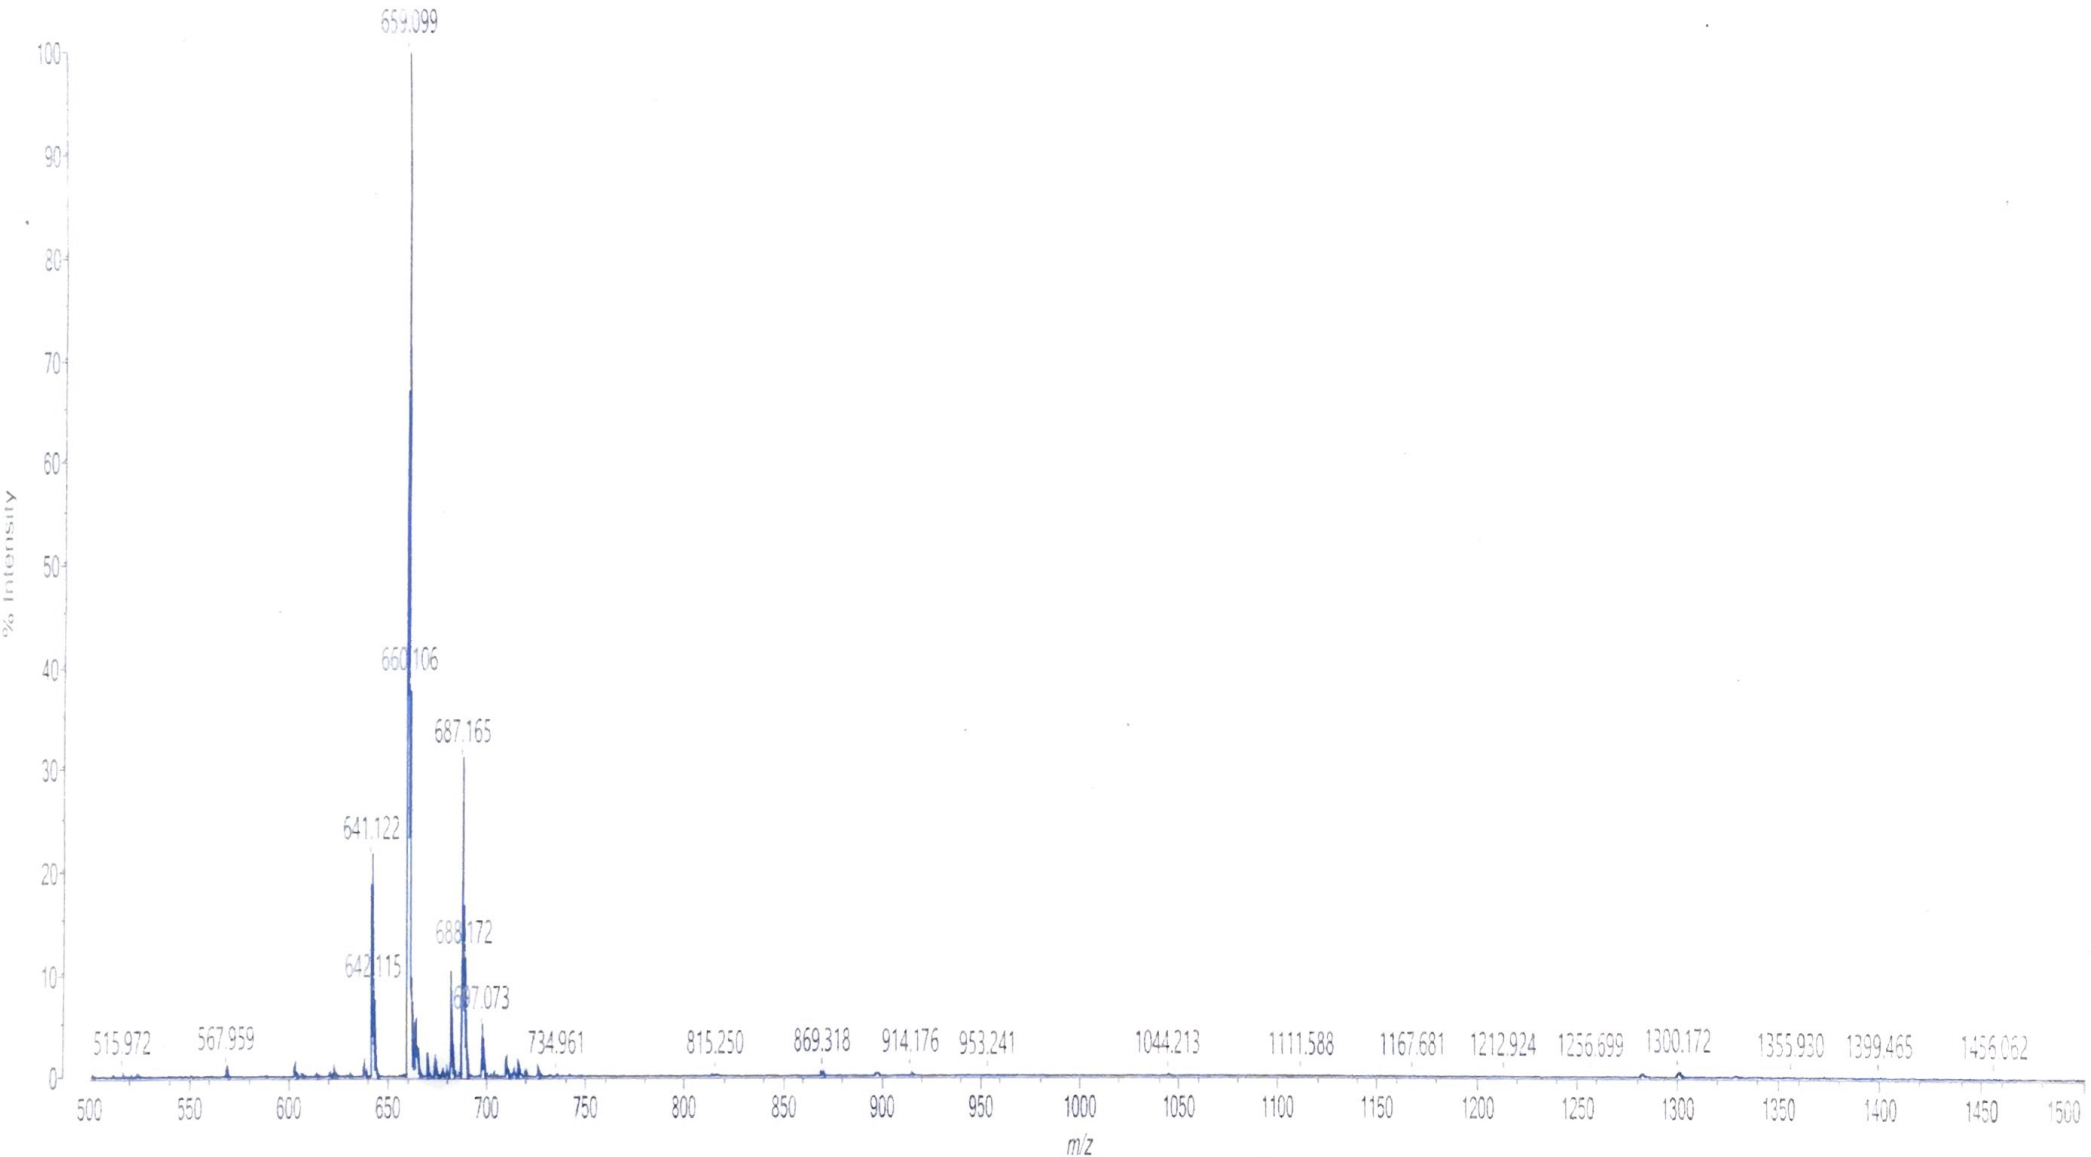


107-91 B 1170-203 (60-716)

Data: New Acquisition 74:C2 (Manual) 09 July 2019 14:37:03 Cal:Named Calibration "190619_CHCApepA" by MALDI Solutions Admin on 19 June 2019 16:01:24 (Original)

Shimadzu MALDI-8020. Tuning Linear, Power 30. P Ext at 700.00 (bin 64)

Processed data (averaged) : 614.7 mV [sum=15550.5 mV], Smoothed = 30, profiles # 1 - 200

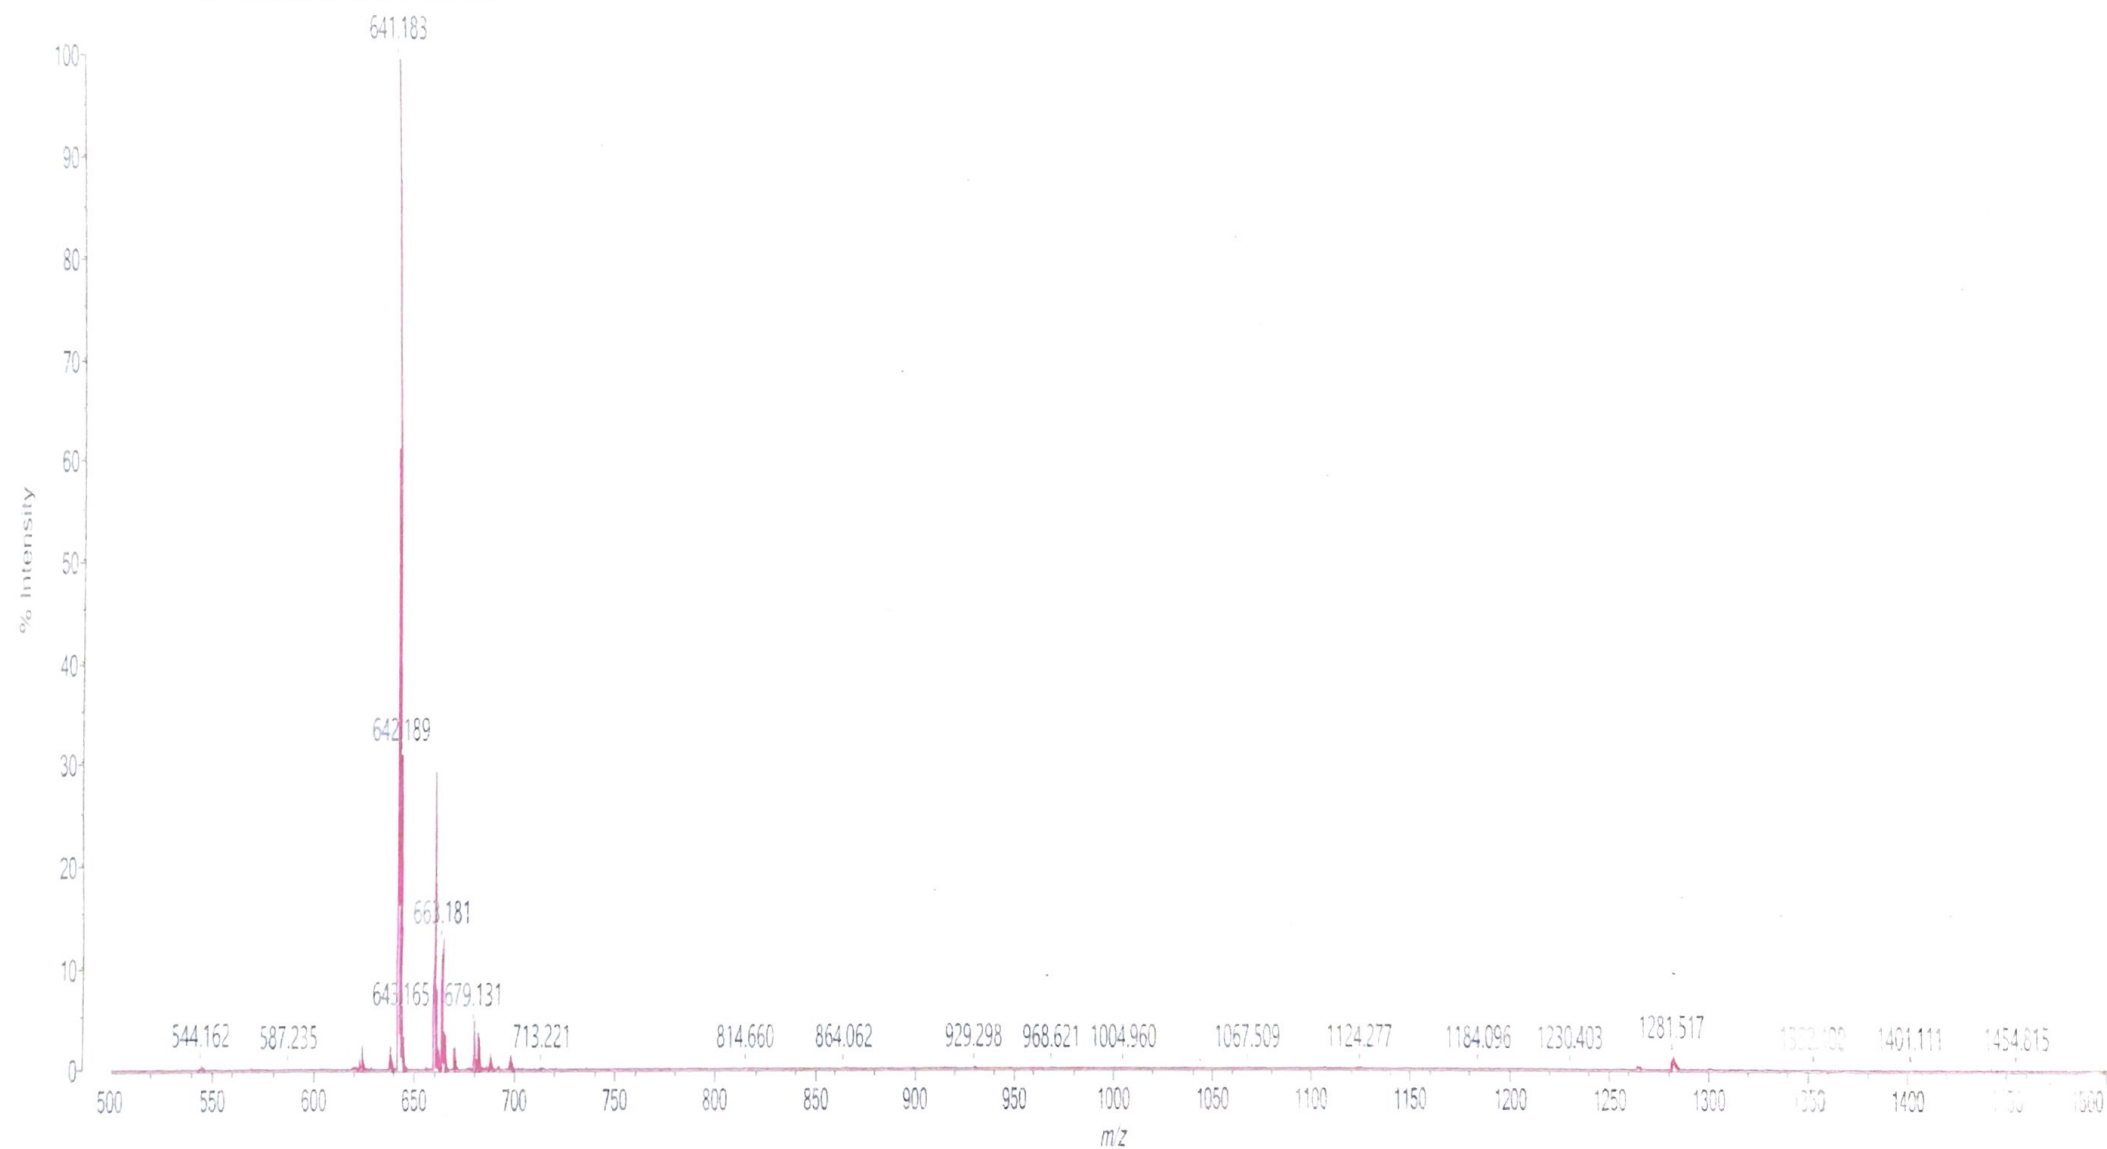


10791A

Data: New Acquisition 72:A2 (Manual) 09 July 2019 14:22:17 Cal:Named Calibration "190619_CHCApepA" by MALDI Solutions Admin on 19 June 2019 16:01:24 (Original)

Shimadzu MALDI-8020: Tuning Linear, Power 30, P Ext at 700.00 (bin 64)

Processed data (averaged): 2459.5 mV (sum=62220.5 mV), Smoothed = 30, profiles # 1 - 200

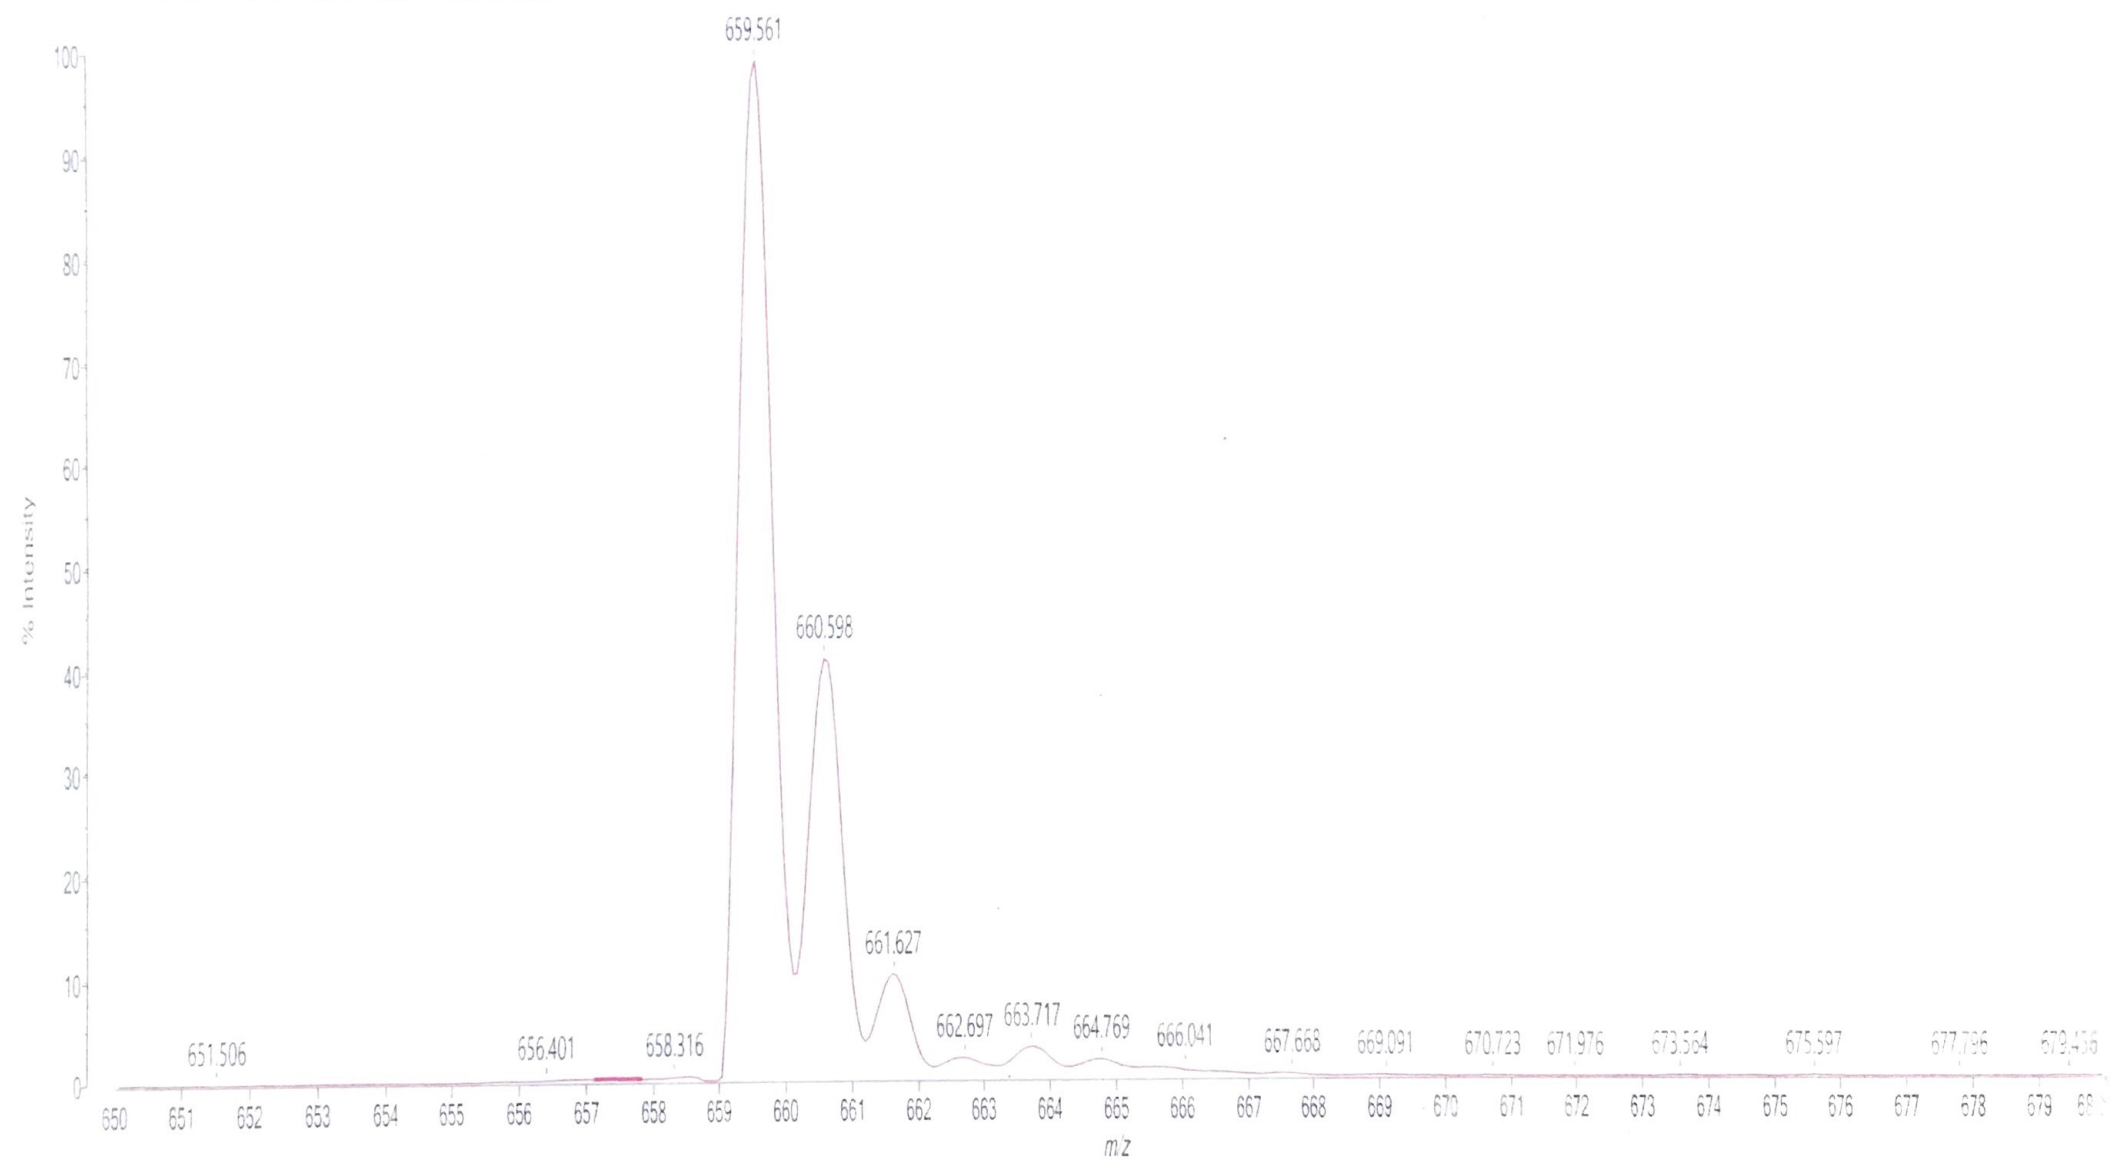


10704K A

Data: New Acquisition 72:A2 (Manual) 09 July 2019 14:22:17 Cal:Named Calibration "190619_CHCApepA" by MALDI Solutions Admin on 19 June 2019 16:01:24 (Original)

Shimadzu MALDI-8020: Tuning: Linear, Power 30, P.Ext at 700.00 (bin 64)

Processed data (averaged): 3560.9 mV [sum=90084.6 mV], Smoothed = 30, profiles # 1 - 200

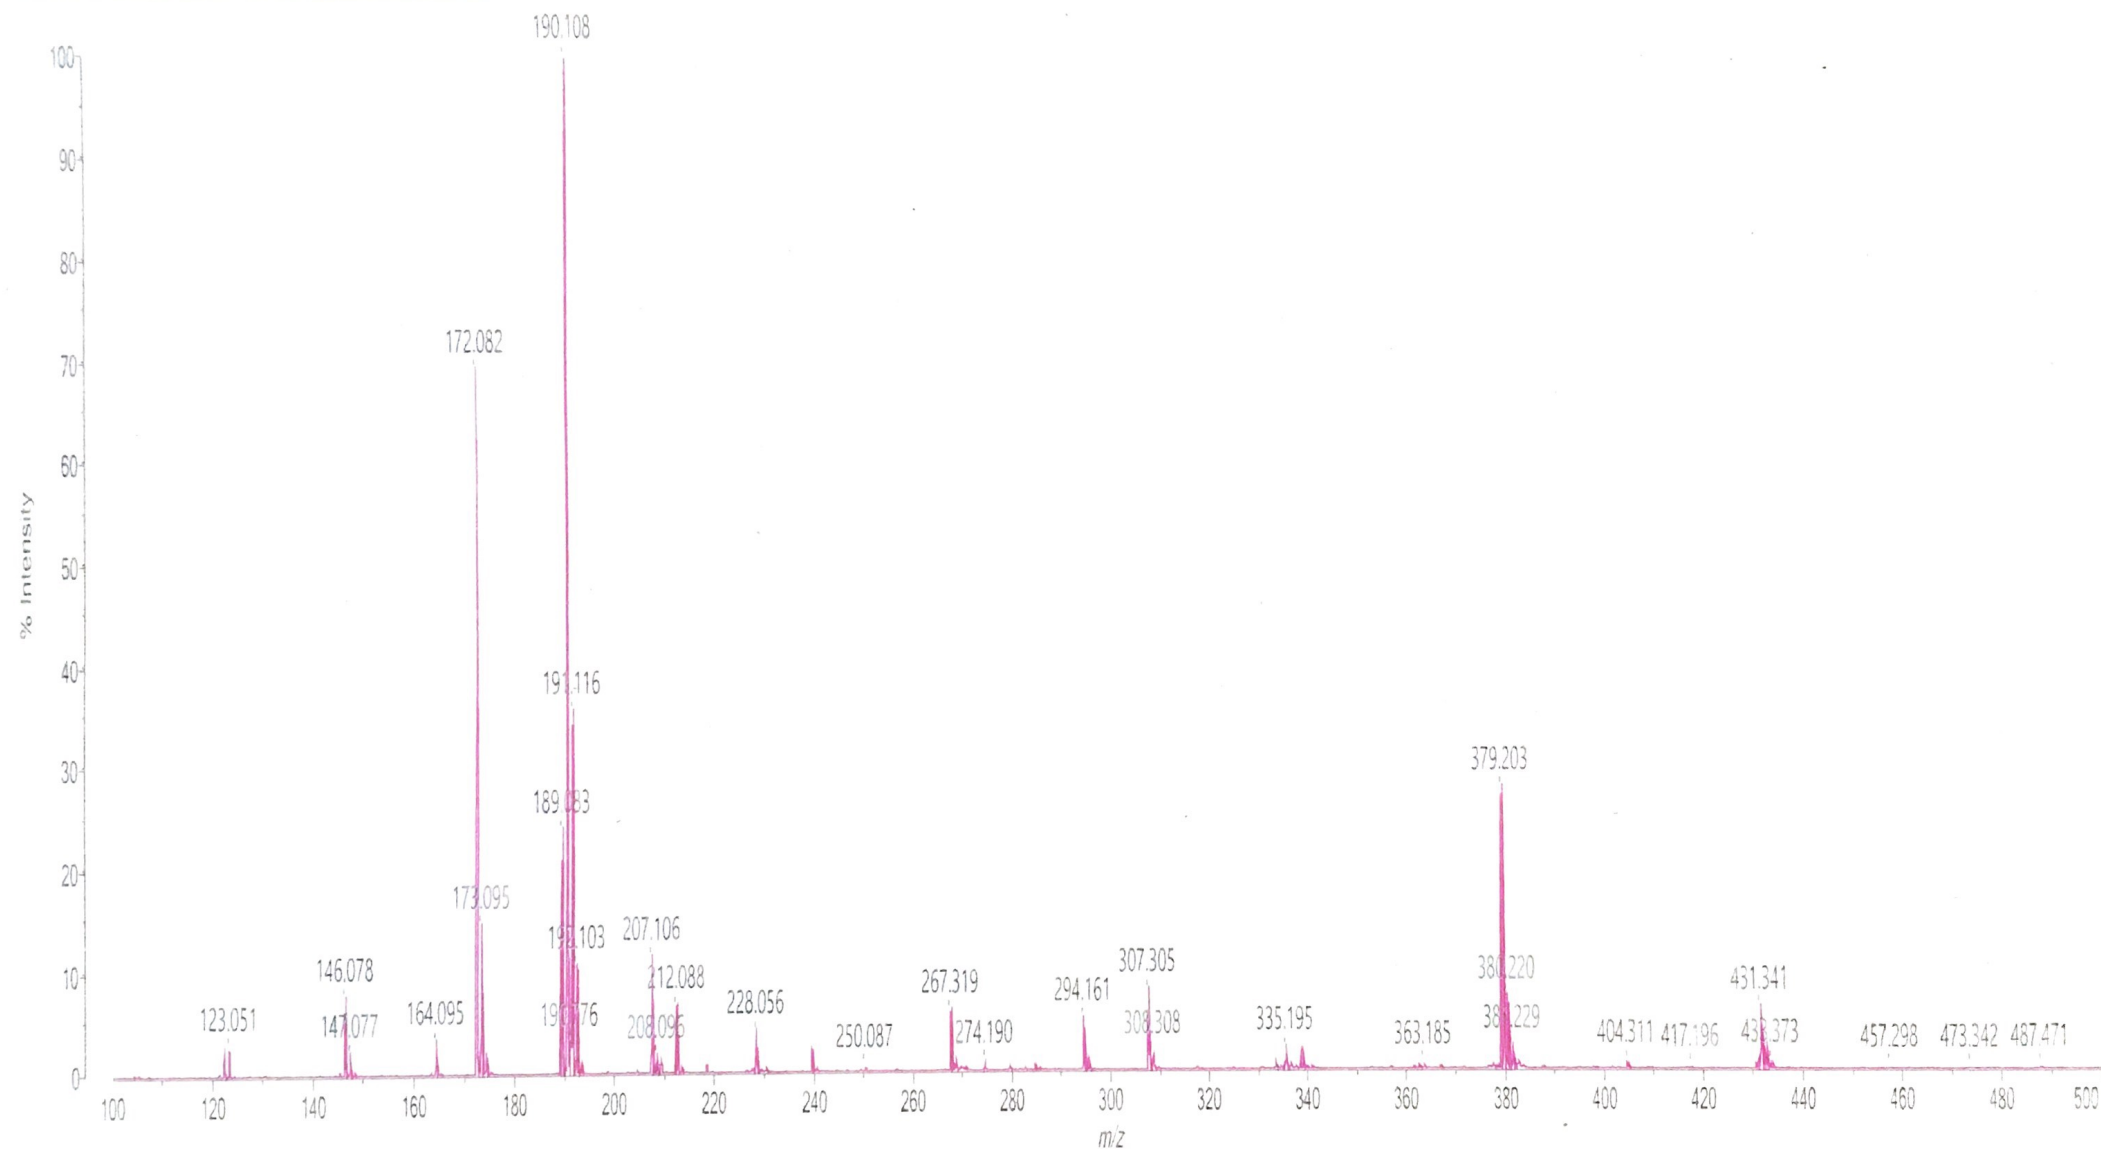

107041A

Data: New Acquisition 72:A2 (Manual) 09 July 2019 14:22:17 Cal:Named Calibration "190619_CHCApepA" by MALDI Solutions Admin on 19 June 2019 16:01:24 (Original)

Shimadzu MALDI-8020: Tuning: Linear, Power 30, P.Ext at 700.00 (bin 64)

Processed data (averaged): 2459.5 mV [sum=62220.5 mV], Smoothed = 30, profiles # 1 - 200

