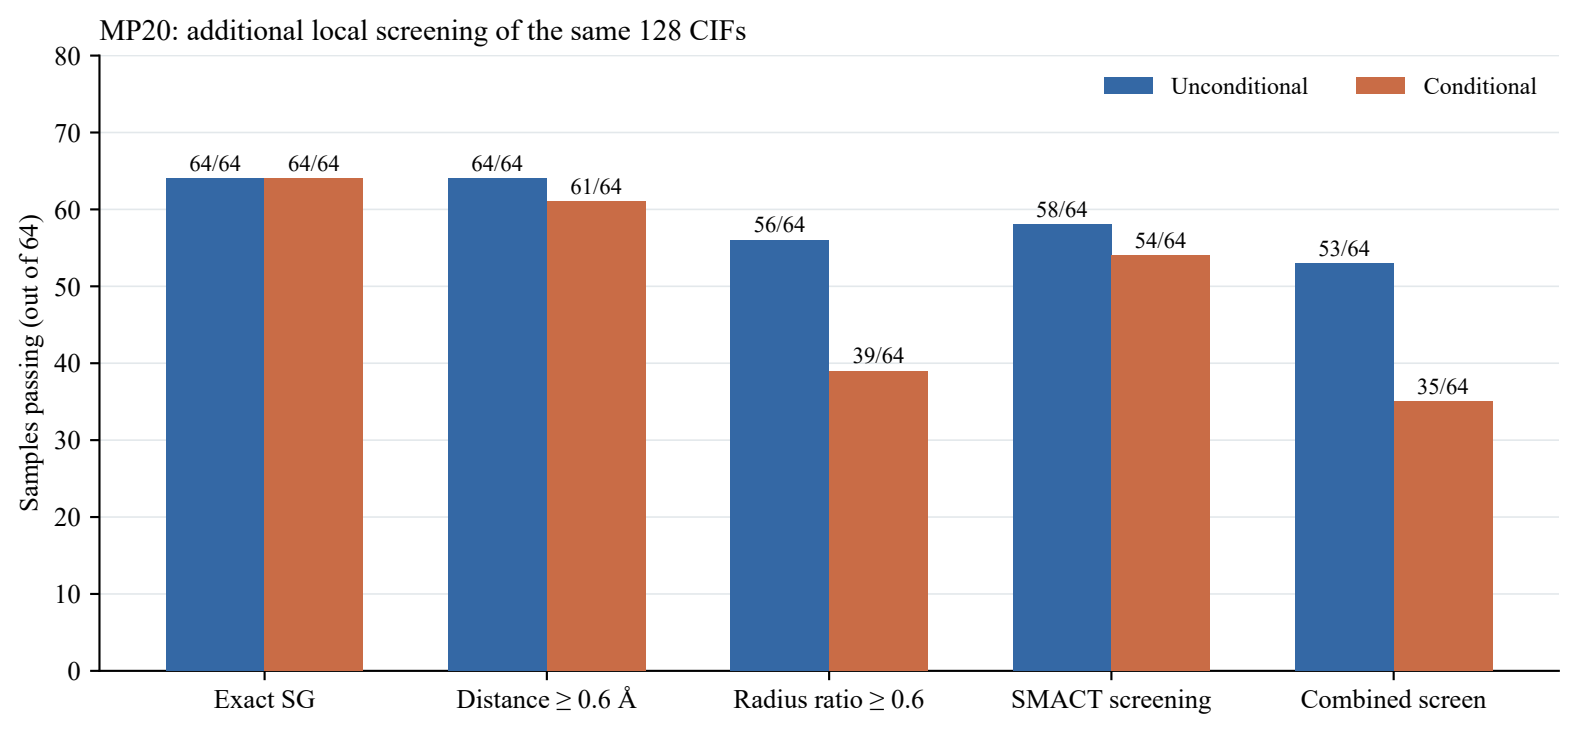
MP20: additional local screening of the same 128 CIFs
Unconditional
Conditional
Samples passing (out of 64)
0
10
20
30
40
50
60
70
80
64/64
64/64
64/64
61/64
56/64
39/64
58/64
54/64
53/64
35/64
Exact SG
Distance ≥ 0.6 Å
Radius ratio ≥ 0.6
SMACT screening
Combined screen