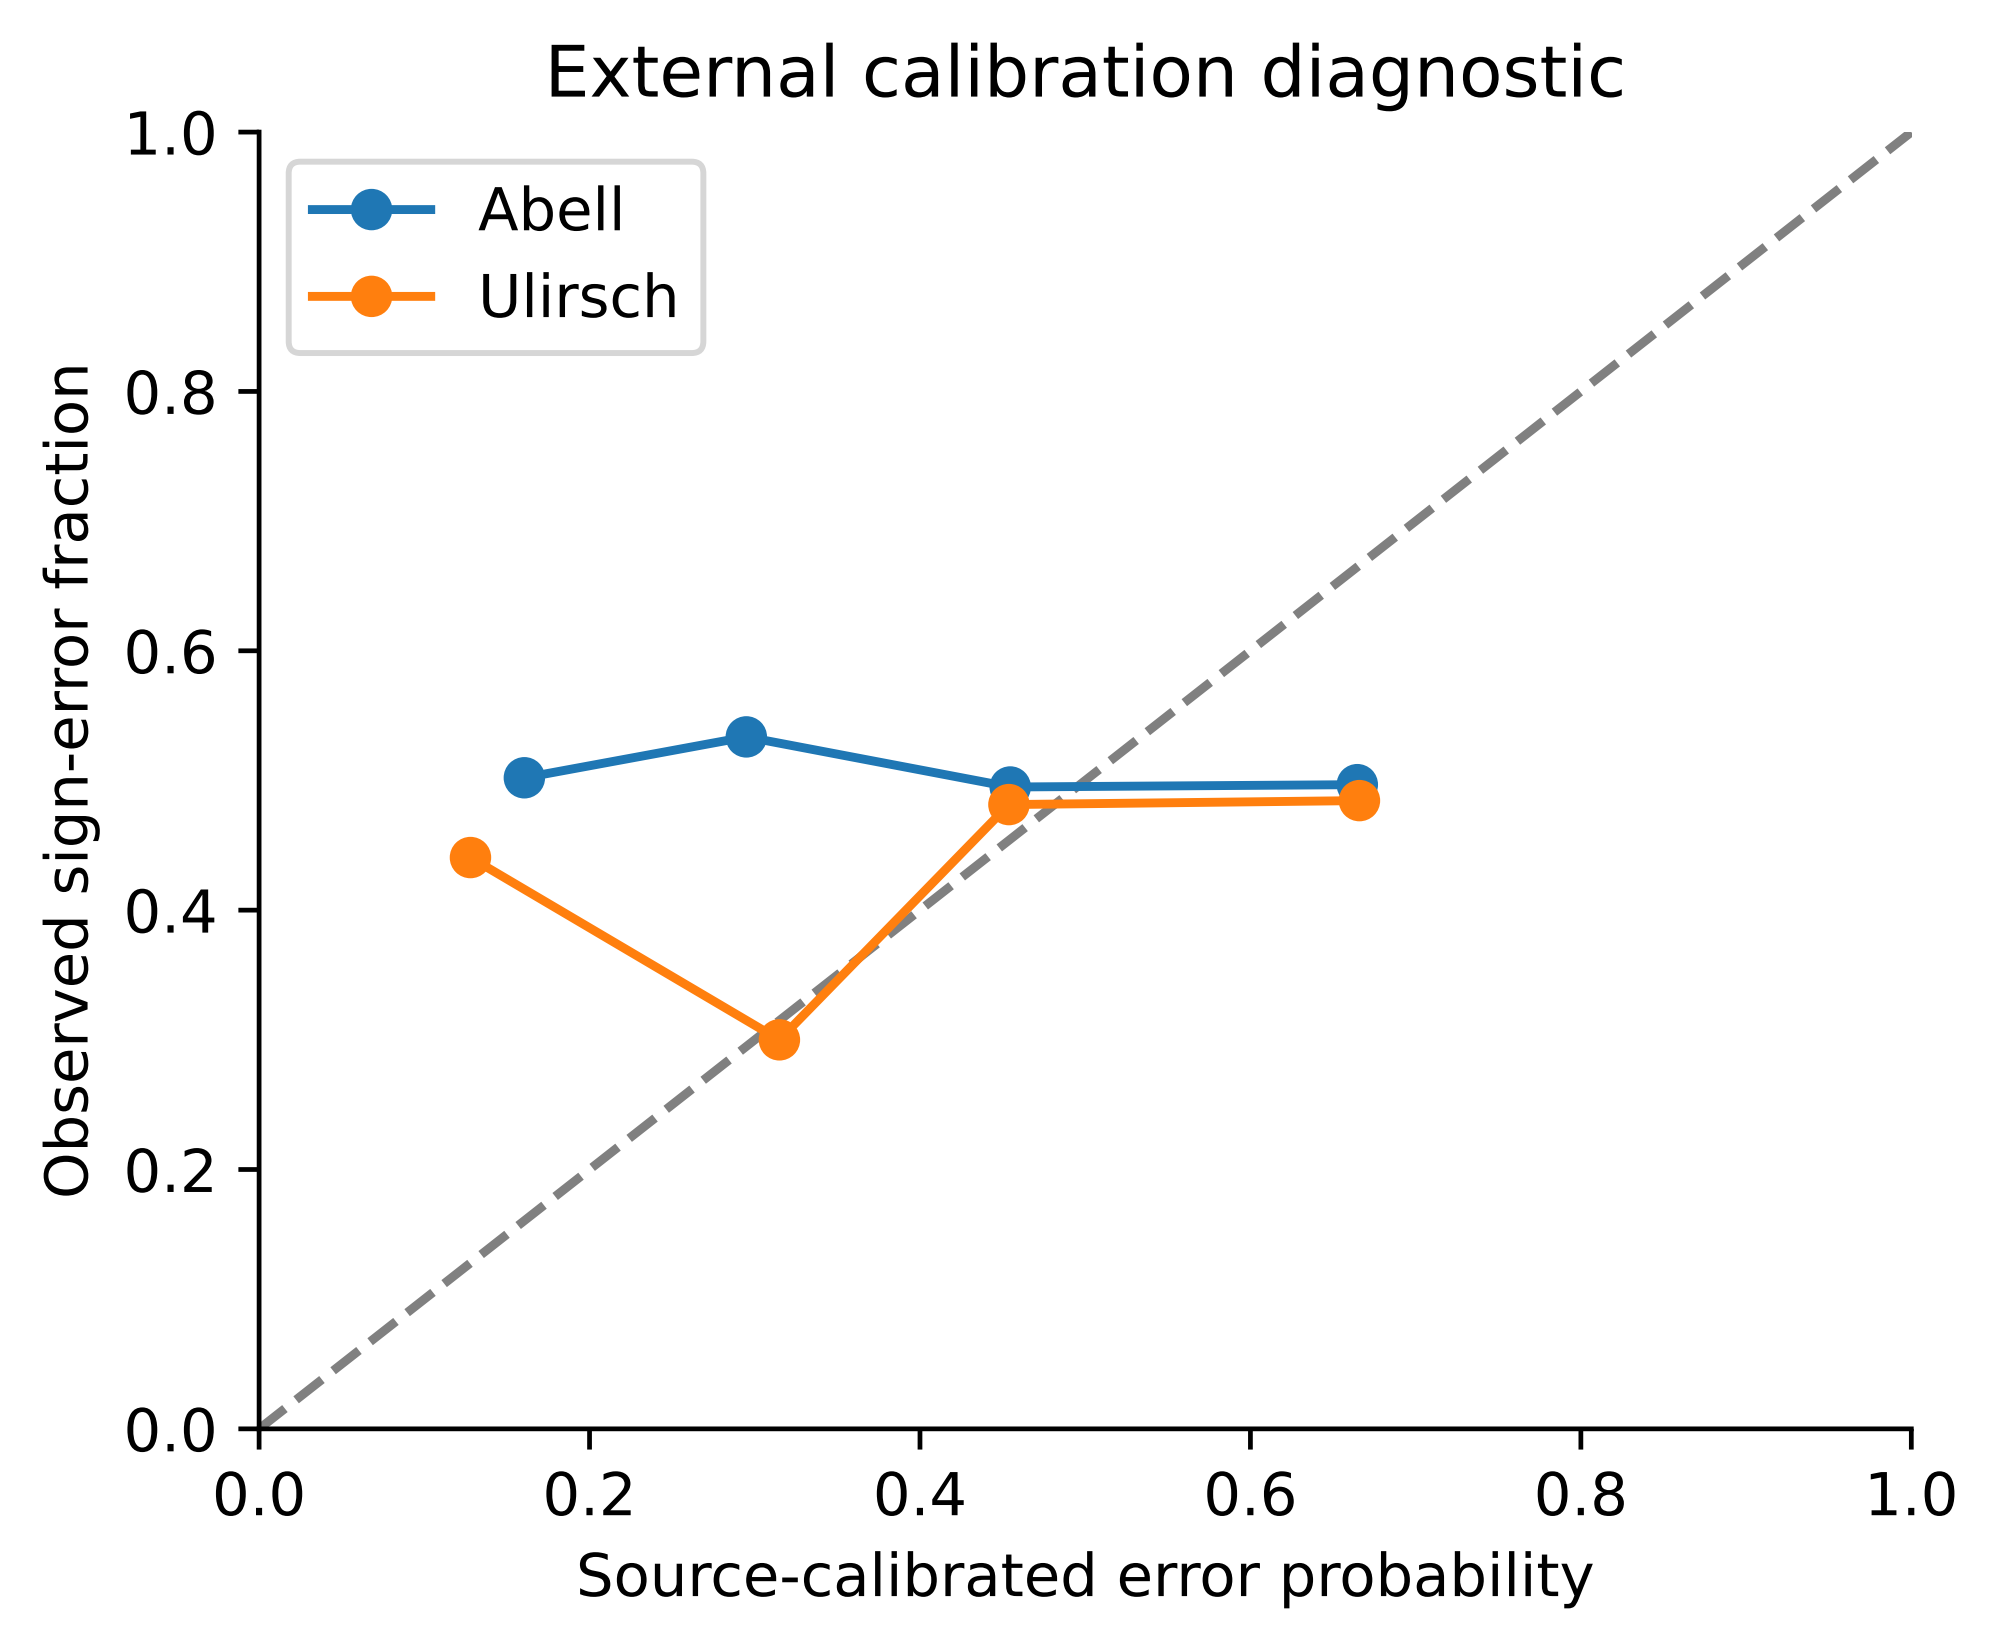
External calibration diagnostic
Abell
Ulirsch
Observed sign-error fraction
Source-calibrated error probability
0.0
0.2
0.4
0.6
0.8
1.0