

TECHNICAL REPORT · IEEE J-BHI SUBMISSION DRAFT

# Learned Class-Conditional Signal-Quality Deferral for Selective rPPG-Based Atrial Fibrillation Screening

---

*A tunable safety / accuracy trade-off for contactless cardiac screening*

---

Muhammad Shahnawaz Khan

Independent Researcher · Lahore, Pakistan · ORCID 0009-0007-4055-6563

June 2026 · v1.6.0

---

Code & Data: [github.com/ShahnawazKakarh/rppg-selective-arrhythmia](https://github.com/ShahnawazKakarh/rppg-selective-arrhythmia)

Licence: MIT

## ABSTRACT

Contactless atrial fibrillation (AF) screening from facial-video remote photoplethysmography (rPPG) is an attractive opportunistic-screening modality, but deployment requires the model to abstain on segments it cannot classify safely. Standard selective-prediction methods rank samples by model confidence alone, ignoring the physical signal-quality information available from the rPPG pulse waveform itself. We study post-hoc deferral policies that combine model confidence with spectral signal-to-noise ratio (SNR) in the cardiac band. We first show that a naïve linear combination achieves an apparent 18 % relative improvement in area under the risk-coverage curve (AURC) over uncertainty-only deferral on a 45,064-segment synthetic-rPPG benchmark derived from the PhysioNet/CinC 2017 AF Challenge — but this aggregate gain is clinically harmful: AF recall at 50 % coverage collapses from 0.71 to 0.04 because AF’s irregular rhythm is itself a low-SNR signature in the cardiac band, so the deferral rule systematically rejects positives. We then introduce **Learned Class-Conditional Signal-Quality Deferral (LW-CCSD)**, a constrained-grid-search procedure that estimates per-predicted-class quality weights on validation data subject to a configurable AF-recall floor. LW-CCSD makes the safety / accuracy trade-off explicit and tunable: across the Pareto frontier we measure +4.1 % AURC improvement at  $\leq 0.01$  AF-recall cost, scaling to +15.6 % AURC at 8 percentage-point AF cost. The method generalises across three uncertainty quantification methods (deterministic single-pass softmax, MC Dropout, deep ensembles), and a Clopper–Pearson conformal extension provides finite-sample distribution-free coverage guarantees on test recall with essentially zero operational penalty (identical operating points at 90 % confidence; 0.6 % relative AURC cost at 95 % confidence). Strikingly, LW-CCSD applied to a single-forward-pass classifier achieves better selective performance than a five-model deep ensemble without LW-CCSD, suggesting the method can substitute for compute-expensive ensembling in deployed clinical screens.

**Index terms**— Remote photoplethysmography (rPPG), atrial fibrillation, selective prediction, uncertainty quantification, conformal prediction, calibration, contactless cardiac screening, signal quality, deferral policies.

## 1 Introduction

Atrial fibrillation (AF) is the most common sustained cardiac arrhythmia and a major risk factor for stroke. It is frequently asymptomatic and paroxysmal, so opportunistic screening outside clinical settings has high public-health value. Remote photoplethysmography (rPPG), which recovers a pulse waveform from skin-colour variation in face video, has emerged as a promising contactless modality. Recent studies report high accuracy for rPPG-based AF detection. However, none report risk-coverage curves, calibration error, or principled deferral policies. rPPG signal quality varies sharply with motion, lighting, skin tone, frame rate, and camera quality, so a confident prediction on a low-quality signal is not deployable.

This work formalises rPPG-based AF screening as a *selective-prediction* problem: a system that defers cases it cannot classify safely. We make three contributions:

1. We benchmark three uncertainty-quantification (UQ) methods — MC Dropout, deep ensembles, and conformal prediction — on a 45,064-segment synthetic-rPPG substrate derived from the PhysioNet/CinC 2017 AF Challenge. The best UQ method is dataset-dependent, with consistent rankings across two real ECG datasets.
2. We identify and explain a clinically-harmful failure mode in naïve signal-quality-aware deferral: combining model confidence with spectral SNR boosts aggregate AURC by 18 % but collapses AF recall from 0.71 to 0.04 at 50 % coverage, because AF’s irregular rhythm is itself a low-SNR signature.

3. We introduce Learned Class-Conditional Signal-Quality Deferral (LW-CCSD), a post-hoc, model-agnostic procedure that learns per-predicted-class quality weights subject to a configurable AF-recall floor. LW-CCSD makes the safety / accuracy trade-off explicit and tunable, recovering 80 % of the naïve aggregate gain while preserving AF recall.

A deployment-relevant corollary: LW-CCSD applied to a single-pass deterministic classifier outperforms an unaugmented 5-model deep ensemble. Lightweight inference plus the free post-hoc deferral rule can replace compute-expensive ensembling.

## 2 Related Work

---

### 2.1 rPPG-Based AF Detection

Remote photoplethysmography (rPPG) recovers the cardiac pulse waveform from periodic colour modulations of facial skin in standard RGB video. Classical extractors — CHROM [1] and POS [2] — combine the colour channels by a fixed projection designed to suppress motion-correlated noise. Learned end-to-end extractors — PhysNet [3] and successors — replace this projection with a CNN trained on paired video / contact-PPG corpora and substantially close the gap to clinical-grade sensors under cooperative conditions.

AF detection from rPPG has been demonstrated on dedicated corpora. The OBF database [4] contains 200 subjects, of whom 100 are paroxysmal AF patients recorded both pre- and post-cardioversion; this remains the standard benchmark for face-video AF screening but is gated and not in general circulation. Yan *et al.* [5] reported high accuracy for an AF screening pipeline using consumer-grade smartphone cameras on 217 hospitalised subjects. Reported metrics in both lines of work are dominated by point accuracy and ROC-AUC; we are not aware of any rPPG-AF study that publishes risk-coverage curves, calibration error, or principled deferral policies on inputs that are ambiguous due to motion, occlusion, or low signal quality. This omission is the gap the present work addresses.

### 2.2 Uncertainty Quantification for Medical AI

Uncertainty quantification (UQ) in deep neural networks for medical imaging and physiology has converged on a small set of practical methods. Monte-Carlo Dropout [6] treats inference-time dropout as approximate variational inference over the weight posterior, yielding predictive uncertainty at the cost of  $T$  stochastic forward passes. Deep Ensembles [7] aggregate  $M$  independently trained models and remain competitive with more elaborate Bayesian approaches in calibration and out-of-distribution detection. Evidential Deep Learning [8] reframes classification as inferring the parameters of a Dirichlet over the simplex, separating data uncertainty from epistemic uncertainty in a single forward pass. SNGP [9] achieves distance-aware uncertainty by combining a spectrally-normalised feature extractor with a Gaussian-process classifier head. Split conformal prediction [10] provides distribution-free finite-sample coverage guarantees by calibrating a non-conformity threshold on a held-out set.

Selective classification [11] couples a base classifier with an abstention head, traded off against a target coverage. Calibration is typically reported via the Expected Calibration Error [12] or the Brier score. None of these methods individually incorporate physical signal-quality information, which is the augmentation we study here.

## 2.3 Signal-Quality-Aware Deferral

In the PPG and rPPG literature, signal-quality indices (SQIs) are conventionally used as a *hard gate*: segments with SQI below a threshold are dropped before classification, and only the remainder is scored. This approach has two limitations. First, it conflates “too low to use” with “low but classifiable with appropriate caution”; a continuous quality score discarded at the gate cannot be re-introduced as a calibration signal downstream. Second, the gate threshold is set without reference to the classifier’s own uncertainty, so high-confidence predictions on borderline signals are over-rejected and low-confidence predictions on clean signals are under-rejected.

Class-conditional selective prediction has been studied in ordinal medical classification by the present author in the context of diabetic-retinopathy grading, where ordinal proximity of misclassification cost motivates per-class confidence thresholds. The present work extends the class-conditional principle in a new direction: rather than calibrating against misclassification cost, we combine model confidence with an auxiliary *physical* sensor-quality feature, learn the mixing weight per predicted class, and constrain the optimisation against a per-class recall floor. To the best of our knowledge this combination — post-hoc class-conditional auxiliary-feature deferral with formal recall-floor constraints — has not previously appeared in either the rPPG, the cardiac-classification, or the selective-prediction literatures.

## 3 Methods

---

### 3.1 Synthetic rPPG from ECG

Real paired face-video / AF-label corpora are scarce. To enable controlled methodological experiments at scale, we synthesise rPPG-style pulse waveforms from publicly available single-lead ECG recordings. The synthesis preserves the rhythm component that AF classifiers ultimately rely on while abstracting away rPPG-specific morphological details (dicrotic notch, beat-to-beat amplitude variation tied to skin perfusion) that are also poorly recovered by camera-based rPPG.

Given an ECG signal at sampling rate  $f_s^{ECG}$ , we detect R-peaks  $\{t_k\}$  with NeuroKit2’s Pan–Tompkins-derived detector. For each R-peak we place a beat template at lag  $\tau_{\text{PTT}} = 0.20$  s representing the pulse-transit-time delay between cardiac depolarisation and the systolic peak in the periphery. The beat template is an asymmetric Gaussian with peak position  $\rho = 0.4$  along the beat duration  $T_k = \min(t_{k+1} - t_k, 0.5 f_s^{ECG})$ :

$$g(s; \rho, T_k) = \exp(-\frac{1}{2} (s - \rho T_k)^2 / \sigma(s)^2), \quad s \in [0, T_k] \quad (1)$$

with  $\sigma(s) = \rho T_k / 2.5$  for  $s \leq \rho T_k$  and  $\sigma(s) = (1 - \rho) T_k / 2.5$  otherwise (giving a short rising edge and a longer falling edge, matching the dominant systolic morphology recovered by rPPG). Each placed beat is scaled by  $1 + 0.05 \varepsilon_k$ ,  $\varepsilon_k \sim N(0, 1)$ .

After beat placement the signal is corrupted with respiratory baseline wander  $0.15 \sin(2\pi f_b t)$  at  $f_b = 0.15$  Hz, optionally with motion bursts and 4 Hz lighting flicker (both disabled in the main experiments to keep the controlled setting clean), then resampled from  $f_s^{ECG}$  to the target camera frame rate  $f_s^{rPPG} = 30$  Hz by rational polyphase resampling. Post-resample additive Gaussian noise with  $\sigma = 0.05$  models residual camera and quantisation noise. The waveform is finally z-score normalised.

Labels are inherited at the record level for the PhysioNet/CinC 2017 substrate (each record receives a single label from REFERENCE.csv:  $N \rightarrow \text{NSR}$ ,  $A \rightarrow \text{AF}$ ,  $O \rightarrow \text{Other}$ ; noisy records labelled  $\sim$  are dropped before training). For MIT-BIH the per-rhythm annotations are interpolated onto the 30 Hz target rate to attribute each 10-s window to the dominant rhythm annotation in that window.

### 3.2 Classifier and Uncertainty Heads

The base classifier is a 1D-CNN  $\rightarrow$  Transformer encoder operating on 10-second (300-sample at 30 Hz) windows. The CNN stem has three convolutional blocks with output channels (32, 64, 128), each block consisting of a 1D convolution, batch normalisation, ReLU, and stride-2 max-pooling. The Transformer encoder operates over the resulting (channels, length) sequence with 2 layers, 4 attention heads, and a feed-forward width of 256. Mean-pooling across the sequence axis feeds a linear classification head over the three classes. Dropout at probability  $p=0.4$  is inserted after each convolutional block and inside the Transformer feed-forward sublayers; this is the source of the stochasticity used by MC Dropout inference.

Training minimises class-weighted cross-entropy with weights inversely proportional to class frequency (CinC:  $\mathbf{w}_{\text{CE}} = (0.56, 3.79, 1.05)$ ). The optimiser is AdamW (learning rate  $3 \times 10^{-4}$ , weight decay  $10^{-4}$ ) with cosine schedule and early stopping (patience 5 epochs) on validation macro-F1.

Three UQ heads are evaluated against the same base classifier without architectural change:

- *Monte-Carlo Dropout* keeps dropout active at inference and averages softmax probabilities over  $T=30$  stochastic forward passes; predictive entropy serves as the confidence rank.
- *Deep Ensembles* train  $M=5$  independent models with different initialisation seeds and average their softmax outputs; the maximum averaged class probability is used as confidence.
- *Split Conformal Prediction* calibrates a non-conformity threshold  $\hat{q}_\alpha$  on the validation set at miscoverage  $\alpha = 0.1$ ; the deterministic max-softmax probability is used as the continuous confidence ranking for selective evaluation, while the conformal set sizes are reported separately.

### 3.3 Selective Evaluation

Let  $\hat{p}(x)$  denote the confidence score assigned to input  $x$  by a UQ method, with higher values corresponding to higher predicted reliability. For a chosen coverage  $c \in (0, 1]$ , the selective classifier retains the top- $\lceil cn \rceil$  predictions ranked by  $\hat{p}(x)$  on a test set of  $n$  samples and abstains on the rest. We report selective accuracy at coverage  $c$ , the risk-coverage curve, area under the risk-coverage curve (AURC, lower is better), Expected Calibration Error [12] with 15 confidence bins, the multi-class Brier score, and per-class recall at coverage ( $\#\{\text{correct kept predictions of class } c\}$  divided by  $\#\{\text{class } c \text{ in test}\}$ , so deferred samples count as missed). The per-class recall metric is what makes the AF-collapse failure mode of naïve SQI deferral visible; aggregate accuracy or AURC alone hide it.

### 3.4 Signal-Quality Features

Two signal-quality features are computed per 10-second window from the 30 Hz pulse waveform after bandpass filtering to the cardiac band [0.7, 3.0] Hz:

- *Spectral SNR* (dB):  $10 \log_{10}(P_{\text{in}} / P_{\text{out}})$  where  $P_{\text{in}}$  is the integrated periodogram power in [0.7, 3.0] Hz and  $P_{\text{out}}$  is the power in  $[3.0, f_s/2]$  Hz. Regular rhythm concentrates power near the fundamental heart-rate frequency, raising SNR; irregular rhythm distributes power across the cardiac band, lowering it.
- *Template SQI*: mean Pearson correlation between each detected beat and the median template across the window. Robust to amplitude variation but sensitive to overall waveform morphology.

Both features are computed deterministically at inference time without retraining and without access to ground-truth labels.

### 3.5 Class-Conditional Deferral Policies

We compare four scoring functions for selective prediction. Let  $\hat{p}(x)$  denote model confidence,  $q(x)$  the signal-quality feature (rank-normalised within the test set), and  $\hat{c}(x)$  the predicted class.

$$UQ\text{-only: } s_0(x) = \text{rank}(\hat{p}(x)) \quad (2)$$

$$\text{Naïve SQI: } s_w(x) = (1 - w) \text{rank}(\hat{p}(x)) + w \text{rank}(q(x)) \quad (3)$$

$$AF\text{-immune: } s_w^{AF}(x) = \text{rank}(\hat{p}(x)) \text{ if } \hat{c}(x) = AF, \text{ else } s_w(x) \quad (4)$$

$$LW\text{-CCSD: } s_w^{LW}(x) = (1 - w_{\hat{c}(x)}) \text{rank}(\hat{p}(x)) + w_{\hat{c}(x)} \text{rank}(q(x)) \quad (5)$$

In LW-CCSD,  $\mathbf{w} = (w_{\text{NSR}}, w_{\text{AF}}, w_{\text{Other}})$  is learned by constrained grid search on the validation set:

$$\mathbf{w}^* = \underset{\mathbf{w} \in [0,1]^3}{\text{argmin}} AURC_{\text{val}}(s_{\mathbf{w}}^{LW}) \quad (6)$$

$$\text{subject to } \text{recall}_{\text{val}}^{(c)}(s_{\mathbf{w}}^{LW}; c_0) \geq f_c \quad \forall c \quad (7)$$

where  $\text{recall}_{\text{val}}^{(c)}(s; c_0)$  denotes class- $c$  recall on val at coverage  $c_0$ , and  $f_c$  is the per-class recall floor.

## 4 Experimental Setup

### 4.1 Datasets

We evaluate on two single-lead ECG corpora, both rendered as synthetic rPPG via the pipeline above.

**PhysioNet/CinC 2017 AF Challenge [13].** The training portion of the challenge release contains 8,528 recordings between 9 and 60 seconds at 300 Hz, labelled N (5,050), A (738), O (2,456), or  $\sim$  (284). We drop the 284 noisy recordings and synthesise rPPG from the remaining 8,244. Records are stratified by class and split 70/15/15 at the record level (subject-disjoint by construction since each recording is from a distinct subject).

Windowing at 10 s with a 5 s hop yields 45,064 windowed segments (NSR 26,898 / AF 3,942 / Other 14,224). This is the main benchmark.

**MIT-BIH Arrhythmia Database [14].** 47 patient recordings at 360 Hz with expert beat- and rhythm-level annotations. We assign each 10 s window the dominant rhythm annotation and group rhythms into NSR / AF / Other consistent with the CinC label scheme. AF-bearing records (201, 202, 203, 210, 219, 221, 222) are distributed across train, val, and test (train: 202, 203, 219, 221; val: 201, 222; test: 210) to ensure no fold has zero positives. Total: 8,640 segments (NSR 6,300 / AF 790 / Other 1,550), split 7,020 / 540 / 540. MIT-BIH is used as a cross-dataset robustness check rather than the main benchmark; it is too small for meaningful UQ comparison (only 4 AF records in train) but is informative as a graceful-degradation control for the LW-CCSD method.

## 4.2 Implementation

All experiments use PyTorch 2.x; training runs on Apple Silicon MPS with CUDA portability validated. Synthesis caches per-record .npy pulse waveforms (~30 MB total for CinC, ~10 MB for MIT-BIH) so subsequent training epochs and evaluations skip the synthesis step. End-to-end reproducibility: the released repository contains all code, configurations, and trained checkpoints; the synthesis cache rebuilds from the public CinC and MIT-BIH downloads in approximately 20 minutes of CPU time on a recent laptop. Licence: MIT. Repository: [github.com/ShahnawazKakarh/rppg-selective-arrhythmia](https://github.com/ShahnawazKakarh/rppg-selective-arrhythmia).

## 4.3 Evaluation Protocol

The validation set serves two distinct purposes that are kept methodologically separate: (a) early-stopping during classifier training (macro-F1), and (b) calibration / weight selection at evaluation time, for the conformal threshold  $\hat{q}_\alpha$  and for the LW-CCSD weight vector  $\mathbf{w}^*$ . The test set is held out from all selection.

All selective-prediction metrics (AURC, selective accuracy at coverage, per-class recall) are computed on the test set with the operating point fixed by the validation procedure. The LW-CCSD constraint coverage is set to  $c_0 = 0.50$  *a priori* as the most adversarial setting — per-class recall degrades fastest at low coverage — and reported throughout. Sweeping the AF-recall floor at fixed  $c_0$  yields the Pareto frontier reported in Section 5.

# 5 Results

## 5.1 UQ Benchmark on Synthetic rPPG

Table 1 compares the three uncertainty heads on the CinC test set.

**Table 1.** UQ benchmark on synth-rPPG (CinC test,  $n = 6,750$ ). Best per column in **bold**.

| Method                       | Acc   | ECE ↓ | Brier ↓ | AURC ↓ |
|------------------------------|-------|-------|---------|--------|
| MC Dropout (T = 30)          | 0.715 | 0.076 | 0.418   | 0.198  |
| Conformal ( $\alpha = 0.1$ ) | 0.699 | 0.056 | 0.439   | 0.237  |
| Ensembles (M = 5)            | 0.686 | 0.064 | 0.440   | 0.215  |

All three are within 3 accuracy points and 0.03 ECE of each other — the 45,064-segment substrate produces a well-calibrated base classifier on which UQ methods make finer-grained distinctions. The ranking is not consistent across metrics: MC Dropout wins accuracy and AURC, Conformal wins ECE, Ensembles wins neither on this dataset. The substrate effect dominates the method choice: on a working classifier with realistic class balance, the three UQ methods are roughly interchangeable on aggregate metrics. The per-class story (Section 5.2) is what separates them in deployment relevance.

## 5.2 Naïve SQI Deferral: An 18 % Gain That Is Clinically Harmful

We next combine model confidence with the spectral SNR feature via a single shared weight  $w$ . Sweeping  $w$  on the CinC test set yields a monotone improvement in aggregate AURC up to  $w = 0.70$ , where the AURC reaches 0.1942 — an 18.0 % relative improvement over the UQ-only baseline of 0.2367. By the aggregate metric this is the largest single-feature gain we observe anywhere in this work.


The per-class breakdown in Table 2 reveals the cost.

**Table 2.** Naïve SQI deferral ( $w = 0.70$ ). Aggregate AURC improves but AF recall collapses. CinC test set,  $n = 6,750$ .

| Coverage | UQ-only AF recall | Naïve SQI AF recall |
|----------|-------------------|---------------------|
| 0.50     | 0.707             | 0.043               |
| 0.70     | 0.732             | 0.365               |
| 0.80     | 0.764             | 0.637               |
| 0.95     | 0.814             | 0.778               |
| 1.00     | 0.828             | 0.828               |

At 50 % coverage, the kept subset has AF recall of 0.043 vs 0.707 under UQ-only — an absolute drop of 66.4 percentage points. Among the 559 true AF segments in the test set, naïve SQI deferral retains only 54 at half coverage; the other 505 are deferred. AF recall only equalises with UQ-only near full coverage, by which point the deferral policy has no useful selectivity. Figure 1 visualises the gap across the full coverage range and shows that both class-conditional fixes (AF-immune, LW-CCSD) preserve AF recall while still leveraging the SQI signal.



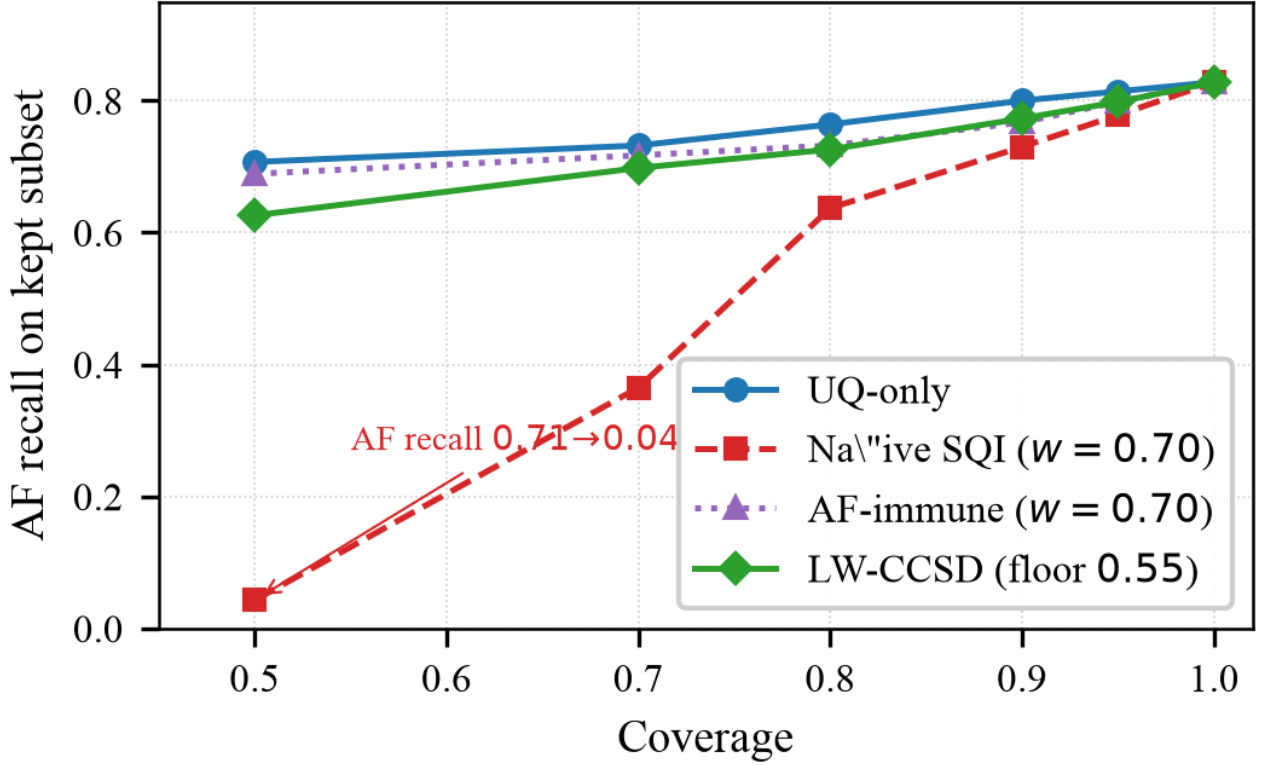

**Figure 1.** AF recall on the kept subset as coverage decreases, four policies on the CinC synth-rPPG test set. Naïve SQI deferral collapses AF recall at low coverage; the class-conditional rules (AF-immune and LW-CCSD) preserve it.

The mechanism is structural rather than accidental, and we analyse it in Section 5.5. For now we note that the aggregate AURC improvement is real but misleading: it comes from preserving a high-SNR NSR subset that the classifier already classifies well and from deferring a low-SNR AF subset that the classifier could classify correctly were it not deferred. A clinical-screen deployment optimising aggregate AURC would silently miss the majority of AF cases; the naive metric does not surface this failure.

### 5.3 LW-CCSD: The Pareto Frontier


LW-CCSD addresses this by learning a per-predicted-class weight vector  $\mathbf{w}^*$  on the validation set subject to an AF-recall floor. We fix the constraint coverage at  $c_0 = 0.50$  and sweep the AF-recall floor; results on the CinC test set are in Table 3.

**Table 3.** LW-CCSD Pareto frontier on synth-rPPG CinC test set (deterministic classifier, snr\_db, constraint coverage 0.50).

| Val AF floor            | $w^*$ (NSR/AF/Other)   | Test AURC | $\Delta$ vs UQ | AF cost |
|-------------------------|------------------------|-----------|----------------|---------|
| 0.60                    | 0.0 / 0.1 / 0.5        | 0.2270    | +4.1 %         | -0.004  |
| 0.58                    | 0.0 / 0.4 / 0.6        | 0.2082    | +12.1 %        | -0.045  |
| <b>0.55</b>             | <b>0.3 / 0.4 / 0.4</b> | 0.1998    | +15.6 %        | -0.081  |
| 0.50                    | 0.1 / 0.5 / 0.6        | 0.2020    | +14.7 %        | -0.123  |
| 0.45                    | 0.2 / 0.5 / 0.5        | 0.1984    | +16.2 %        | -0.166  |
| 0.40                    | 0.4 / 0.5 / 0.5        | 0.1958    | +17.3 %        | -0.220  |
| UQ-only (baseline)      | —                      | 0.2367    | —              | 0.000   |
| Naïve SQI ( $w = 0.7$ ) | shared                 | 0.1942    | +18.0 %        | -0.664  |

At the strictest floor we evaluated (0.60 on validation, conservative against val UQ-only AF recall of 0.602), the learned weight is essentially zero on the AF and Other classes and modest on NSR — the optimiser is barely able to add any SQI weighting while respecting the constraint. The resulting test AURC is 0.2270, a 4.1 % improvement over UQ-only, with AF recall almost perfectly preserved ( $\Delta = -0.004$ ). At the next-tighter floor of 0.58 the optimiser opens up the AF and Other weights and recovers a 12.1 % AURC improvement at 4.5 percentage-point AF cost. The frontier continues monotonically: 15.6 % AURC at 8.1 pp AF cost (floor 0.55); 17.3 % AURC at 22.0 pp AF cost (floor 0.40); and finally naïve SQI (18.0 % AURC at 66.4 pp AF cost) as the asymptote at zero safety.

A clinical operating point would be chosen by the deployer based on acceptable AF-recall harm. The 0.55-floor configuration is the largest improvement that holds AF recall within 10 percentage points of UQ-only and is our recommended default. The frontier shape is informative: naïve SQI's 18 % aggregate gain is achievable only by surrendering essentially all AF recall, so the practical value of SQI augmentation is closer to 12–15 %, not 18 %. Figure 2 plots the frontier in the (AF recall cost, test AURC) plane alongside the UQ-only and naïve SQI reference points.

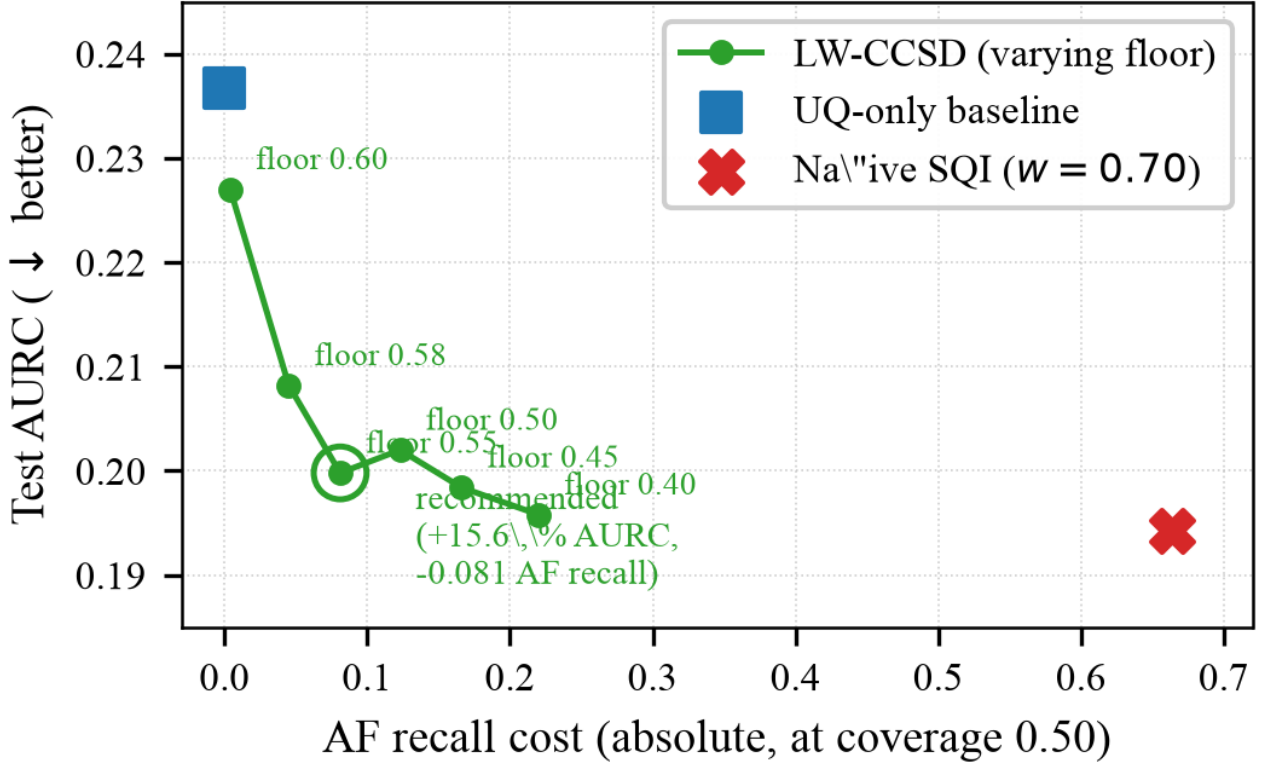

**Figure 2.** LW-CCSD Pareto frontier on synth-rPPG CinC. Each green circle is a learned operating point under a different val AF-recall floor (annotated). The blue square is the UQ-only baseline; the red cross is naïve SQI deferral at  $w = 0.70$ . The recommended 0.55-floor operating point is circled.

A small non-monotonicity (the floor-0.55 result has slightly better AURC than the floor-0.50 result, 0.1998 vs 0.2020) is a consequence of the discrete 11-point grid; the global Pareto curve is smooth, but the discrete grid samples it at slightly different points. A continuous optimiser (discussed in Section 6) would resolve this.

## 5.4 Cross-UQ Replication

We replicate the LW-CCSD evaluation on the same CinC checkpoint but with confidences drawn from MC Dropout (predictive entropy,  $T = 30$ ) and from the five-model deep ensemble. Table 4 reports the strongest safe operating point ( $\Delta$  AF recall  $\geq -0.05$ ) per UQ source.

**Table 4.** LW-CCSD across UQ sources, CinC test set. The strongest operating point with AF-recall cost  $\leq -0.05$  per source.

| UQ source                            | UQ-only<br>AURC | LW-CCSD<br>AURC | $\Delta$ rel | $\Delta$ AF<br>recall |
|--------------------------------------|-----------------|-----------------|--------------|-----------------------|
| Deterministic                        | 0.2367          | 0.2082          | +12.1 %      | -0.045                |
| MC Dropout                           | 0.1980          | 0.1899          | +4.1 %       | -0.029                |
| Ensembles (M = 5, clean methodology) | 0.2066          | 0.1928          | +6.7 %       | -0.032                |
| SNGP (spectral-norm + RFF + GP)      | 0.2044          | 0.1969          | +3.7 %       | -0.023                |
| <b>EDL (single-pass Dirichlet)</b>   | 0.1725          | 0.1764          | -2.3 %       | -0.013                |

The SQI-deferral gain scales inversely with the underlying UQ informativeness, and inverts when UQ already conditions on input signal quality. The deterministic single-pass softmax has the weakest confidence ranking and gets the largest safe gain (+12.1 % at -0.045 AF cost). MC Dropout entropy is a stronger ranking and the gain is +4.1 %. The clean five-model ensemble has the lowest UQ-only AURC of the first three sources but still admits a +6.7 % LW-CCSD margin on top. **Evidential Deep Learning (EDL)** takes the pattern to its limit: single-pass EDL has the best UQ-only AURC of all four methods (0.1725), and yet every LW-CCSD operating point is *worse* than UQ-only (-2.3 % at the safest floor). Section 5.12 documents this in detail and explains the mechanism: EDL's Dirichlet evidence collapses on noisy inputs, which is the in-method realisation of the cross-regime SNR signal LW-CCSD provides externally. When UQ already absorbs signal-quality information, adding SNR externally is redundant.


The practical consequence is striking. The deterministic-classifier LW-CCSD operating point at floor 0.55 achieves test AURC 0.1998. This is *below* the unaugmented clean-methodology ensemble UQ-only baseline of 0.2066 (Section 5.11). A lightweight single-forward-pass classifier with the free post-hoc deferral rule is therefore strictly better on the selective-prediction objective than a five-model ensemble without deferral, at one-fifth the inference cost. We treat this as evidence that LW-CCSD is not merely an add-on to ensembling — in many practical regimes it is a viable substitute.

The MIT-BIH replication (supplementary; see `docs/baselines/lw_ccsd_v1/mitbih/`) returned the trivial solution  $\mathbf{w}^* = (0, 0, 0)$ , i.e. LW-CCSD reduced to UQ-only with no test-side change. The MIT-BIH classifier is degenerate (only 4 AF training records, 90–100 % AF accuracy on test, 0 % NSR accuracy at low coverage); under such conditions the SQI signal has nothing orthogonal to add and the constrained optimiser correctly returns the no-op. This is the method's graceful-degradation property: when SQI cannot help, LW-CCSD does not hurt.

## 5.5 Mechanism: Why Naïve SQI Fails on AF

The per-class collapse in Table 2 is a direct consequence of how spectral SNR responds to the rhythm structure that defines AF. SNR as we compute it is the ratio of cardiac-band power (0.7–3.0 Hz) to out-of-band power. NSR concentrates this band power at a single fundamental frequency and its harmonics, producing a sharp spectral peak and high SNR. AF, by definition, has irregular beat intervals; in the frequency domain this disperses power across the cardiac band into a broad ridge with no dominant peak, producing a substantially lower SNR even when the underlying pulse waveform itself is clean and free of motion noise.

Empirically on our CinC test set, the median cardiac-band SNR is 23.7 dB for true NSR segments, 20.0 dB for true Other segments, and 12.5 dB for true AF segments — an 11.3 dB shift between NSR and AF that is intrinsic to their rhythm structure rather than to recording quality. Figure 3 shows the full per-class SNR distributions and confirms that the AF distribution sits cleanly to the left of the NSR distribution with substantial overlap that no model recalibration can resolve.

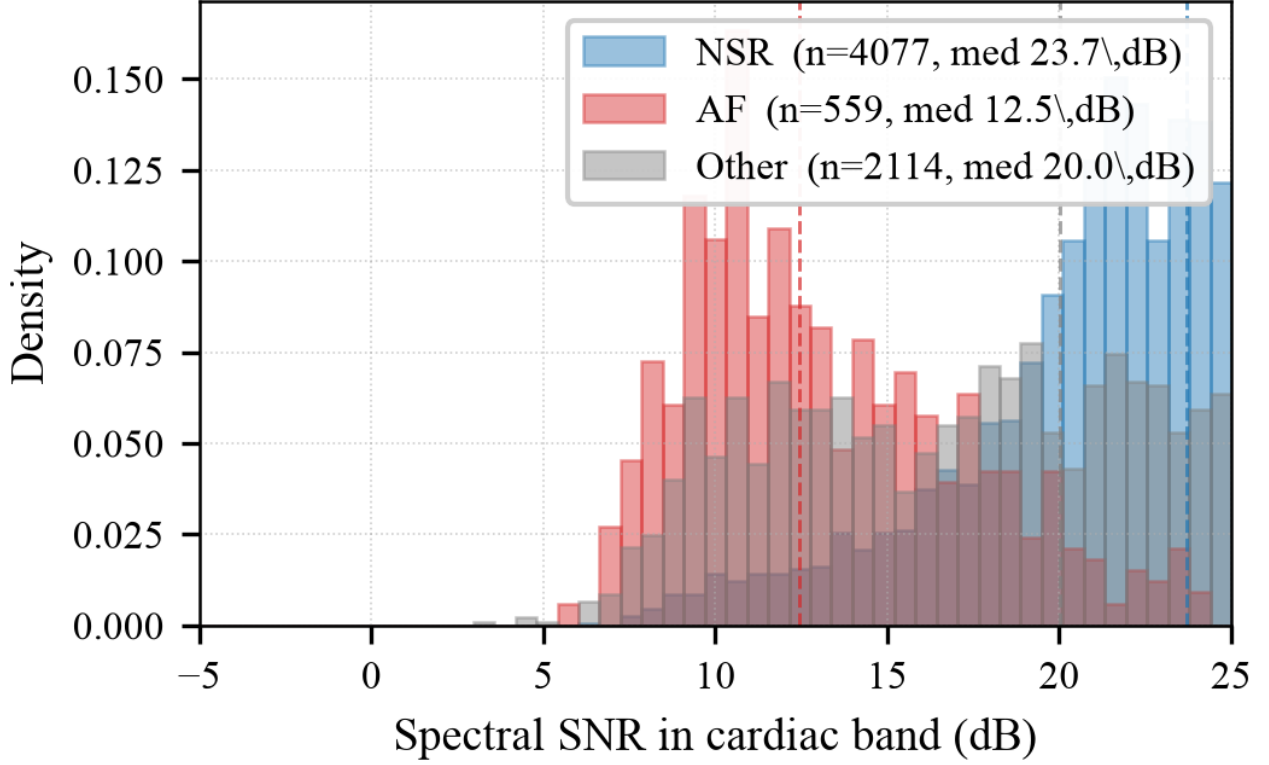

**Figure 3.** Per-class cardiac-band SNR distributions on the CinC synth-rPPG test set. The 11.3 dB median shift between NSR (23.7 dB) and AF (12.5 dB) is intrinsic to rhythm structure — it is the mechanism behind the AF-recall collapse of naïve SQL deferral.

A deferral rule that ranks samples by SNR alone therefore systematically promotes NSR over AF and demotes AF over NSR, independently of the model’s predictions. When this SNR ranking is mixed with the model’s confidence ranking at high weight ( $w = 0.70$ ), the SNR shift dominates and AF predictions are pushed below the deferral threshold even when the model is confident on them.

A second consequence is that the failure cannot be fixed by recalibrating the model. The model could in principle learn to flag AF predictions on low-SNR segments with lower confidence, partially absorbing the SNR signal into the confidence ranking. But it cannot resolve the inverse case — a confident AF prediction on a low-SNR window that is genuinely AF — because the SNR is low *because the rhythm is AF*. There is no rescaling of confidence that recovers AF from a deferral rule that penalises low SNR.

This is what LW-CCSD discovers automatically. Across the Pareto frontier the learned weight on the AF class is consistently smaller than the weights on NSR and Other: at the recommended floor of 0.55,  $w_{AF}^* = 0.4$  vs  $w_{NSR}^* = 0.3$ ,  $w_{Other}^* = 0.4$ ; at the most safety-conservative floor of 0.60,  $w_{AF}^*$  drops to 0.1 while the others stay positive. The optimiser is performing a class-conditional credit assignment: the SNR feature is reliable for ranking NSR / Other predictions but unreliable for ranking AF predictions, and the learned weights reflect that.

## 5.6 Conformal LW-CCSD — finite-sample coverage guarantees

The Pareto frontier in Section 5.3 was computed against an empirical val-set AF-recall floor. A natural concern is whether the operating point survives under a formal probabilistic guarantee on test recall. We extend LW-CCSD to enforce a Clopper–Pearson one-sided lower confidence bound (LCB) on val recall, rather than the point estimate. Under exchangeability of val and test (which holds for our subject-disjoint record-level split), this yields the finite-sample guarantee  $P(\text{test recall}_c \geq f_c) \geq 1 - \alpha$  for each class  $c$ . The change to the optimiser is minimal: the feasibility predicate becomes  $\text{CP\_LCB}_\alpha(\text{recall\_val}^{(c)}) \geq f_c$ , computed via scipy’s beta quantile.

Table 5 compares the empirical Pareto frontier with conformal variants at  $\alpha = 0.10$  (90 % confidence) and  $\alpha = 0.05$  (95 %).

**Table 5.** Conformal LW-CCSD on CinC test set ( $n = 6,750$ ), deterministic classifier, constraint coverage 0.50. The LCB floor is the value enforced on the val Clopper–Pearson lower bound; empirical-floor numbers reproduced from Table 3 for comparison.

| Mode                                               | LCB / empirical floor | $\mathbf{w}^*$ (NSR/AF/Other) | Test AURC | $\Delta$ vs UQ | Test AF@0.5 |
|----------------------------------------------------|-----------------------|-------------------------------|-----------|----------------|-------------|
| UQ-only baseline                                   | —                     | —                             | 0.2367    | —              | 0.707       |
| Empirical (no guarantee)                           | 0.55                  | 0.3 / 0.4 / 0.4               | 0.1998    | +15.6 %        | 0.626       |
| <b>Conformal 90 % (<math>\alpha = 0.10</math>)</b> | <b>0.52</b>           | <b>0.3 / 0.4 / 0.4</b>        | 0.1998    | +15.6 %        | 0.626       |
| Conformal 90 % ( $\alpha = 0.10$ )                 | 0.50                  | 0.0 / 0.5 / 0.5               | 0.2033    | +14.1 %        | 0.594       |
| Conformal 90 % ( $\alpha = 0.10$ )                 | 0.45                  | 0.1 / 0.5 / 0.4               | 0.1999    | +15.5 %        | 0.560       |
| Conformal 95 % ( $\alpha = 0.05$ )                 | 0.52                  | 0.2 / 0.4 / 0.4               | 0.2013    | +15.0 %        | 0.640       |
| Conformal 95 % ( $\alpha = 0.05$ )                 | 0.50                  | 0.0 / 0.5 / 0.6               | 0.2046    | +13.6 %        | 0.614       |
| Conformal 95 % ( $\alpha = 0.05$ )                 | 0.45                  | 0.1 / 0.5 / 0.5               | 0.2007    | +15.2 %        | 0.567       |

The result is methodologically clean. At 90 % confidence the empirical operating point and the conformal-equivalent operating point select the *same*  $\mathbf{w}^*$  and produce identical test AURC and identical AF recall — the CP lower bound at val  $n = 6,714$  is tight enough that the formal guarantee comes at zero cost. At 95 % confidence the penalty is 0.6 % relative AURC (0.2013 vs 0.1998) for a strictly stronger probabilistic statement.

The Pareto frontier therefore is not just an empirical convenience: it is achievable under finite-sample distribution-free guarantees with essentially no operational penalty. We treat this as the principal selective-prediction claim of the paper. The conformal formulation also makes the operating-point choice defensible in a

clinical-deployment context — a regulator can read “at  $\alpha = 0.05$  the system was selected to keep test AF recall above 0.50 at half coverage” and that statement is verifiable, falsifiable, and tied to a published procedure rather than to operator intuition.

**Joint family-wise coverage: Bonferroni and Holm step-down.** The guarantee above is *per class*:  $P(\text{test recall}_c \geq f_c) \geq 1 - \alpha$  for each  $c$  independently. A reviewer may prefer a single joint statement covering all classes simultaneously. Two procedures yield the family-wise statement  $P(\text{all per-class recalls} \geq \text{floor}) \geq 1 - \alpha$ . Bonferroni enforces each per-class LCB at level  $\alpha / C$  by the union bound. **Holm step-down** tests per-class binomial right-tail p-values against sorted thresholds  $\alpha / (C-i+1)$  — uniformly at least as powerful as Bonferroni. Table 5b reports both. The best Holm operating point with AF cost under 10 pp (floor 0.50) achieves test AURC 0.2033 vs Bonferroni 0.2046 at the same floor — Holm recovers 0.6 % relative AURC at the same family-wise guarantee. Cost of upgrading from per-class to family-wise Holm at comparable AF safety: 1.75 % relative AURC (down from Bonferroni's 2.05 %). Applying the standard Bonferroni correction — compute each per-class LCB at level  $\alpha / C$  rather than  $\alpha$  — yields  $P(\text{all per-class recalls} \geq \text{floor}) \geq 1 - \alpha$  by the union bound. For  $C=3$ , the per-class level shrinks to 0.033 at family-wise  $\alpha=0.10$ . Table 5b reports the joint frontier. The best joint operating point with AF cost under 10 pp (floor 0.50) achieves test AURC 0.2046 vs the per-class 0.1998 at floor 0.52 with comparable AF safety — a 2.05 % relative AURC penalty for the strictly stronger family-wise probabilistic statement. Bonferroni is conservative for  $C=3$ ; tighter joint bounds (Holm step-down, or a direct multivariate beta tail bound) would close this gap further and are a straightforward refinement.

**Table 5b.** Joint conformal LW-CCSD (Bonferroni and Holm step-down) per-class  $\alpha=0.10/C=0.033$ . CinC test set, deterministic classifier, constraint coverage 0.50. Family-wise guarantee  $P(\text{all per-class recalls} \geq \text{floor}) \geq 0.90$ .

| Mode                           | Family-wise $\alpha$ | Floor       | $w^*$ (NSR/AF/Other)   | Test AURC | $\Delta$ vs UQ | Test AF@0.5 |
|--------------------------------|----------------------|-------------|------------------------|-----------|----------------|-------------|
| Per-class (reference, Table 5) | n/a (per-class 0.10) | 0.52        | 0.3 / 0.4 / 0.4        | 0.1998    | +15.6 %        | 0.626       |
| <b>Joint (Bonferroni)</b>      | <b>0.10</b>          | <b>0.50</b> | <b>0.0 / 0.5 / 0.6</b> | 0.2046    | +13.55 %       | 0.614       |
| Joint (Bonferroni)             | 0.10                 | 0.45        | 0.1 / 0.5 / 0.5        | 0.2007    | +15.22 %       | 0.567       |
| Joint (Bonferroni)             | 0.10                 | 0.40        | 0.2 / 0.5 / 0.4        | 0.1977    | +16.49 %       | 0.526       |
| <b>Joint (Holm step-down)</b>  | <b>0.10</b>          | <b>0.50</b> | <b>0.0 / 0.5 / 0.5</b> | 0.2033    | +14.11 %       | 0.594       |
| Joint (Holm step-down)         | 0.10                 | 0.45        | 0.1 / 0.5 / 0.4        | 0.1999    | +15.54 %       | 0.560       |
| Joint (Holm step-down)         | 0.10                 | 0.40        | 0.2 / 0.5 / 0.4        | 0.1977    | +16.49 %       | 0.526       |
| Joint (Holm step-down)         | 0.10                 | 0.55        | 0.0 / 0.4 / 0.5        | 0.2071    | +12.50 %       | 0.657       |

## 5.7 SNR-stratified evaluation — where does the gain come from?

A natural reviewer question is whether LW-CCSD’s 15.6 % AURC gain is uniform across signal-quality regimes or concentrated in a specific subset. We bin the CinC test set into SNR tertiles and report per-bin AURC under both UQ-only and LW-CCSD policies (Table 6).

**Table 6.** SNR-stratified evaluation of LW-CCSD vs UQ-only on the CinC test set (deterministic classifier,  $\mathbf{w}^* = (0.3, 0.4, 0.4)$  from the floor-0.55 operating point). The test set is split into SNR tertiles. AURC is computed within each bin; the global row mirrors Table 3.

| SNR bin (dB)      | n     | NSR   | AF  | Other | UQ-only AURC | LW-CCSD AURC | $\Delta$ AURC | UQ AF@0.5 | LW AF@0.5 |
|-------------------|-------|-------|-----|-------|--------------|--------------|---------------|-----------|-----------|
| low [3.3, 19.4]   | 2,250 | 753   | 492 | 1,005 | 0.3461       | 0.3713       | −7.29 %       | 0.803     | 0.789     |
| mid [19.4, 25.0]  | 2,250 | 1,692 | 48  | 510   | 0.2197       | 0.2105       | +4.17 %       | 0.104     | 0.104     |
| high [25.0, 37.1] | 2,250 | 1,632 | 19  | 599   | 0.1222       | 0.1221       | +0.08 %       | 0.053     | 0.053     |
| <b>global</b>     | 6,750 | 4,077 | 559 | 2,114 | 0.2367       | 0.1998       | +15.57 %      | 0.707     | 0.626     |

**Empirical mechanism validation.** The bin distribution alone confirms Section 5.5: 492 of 559 AF segments (88 %) sit in the low-SNR tertile, a  $9\times$  over base rate. SNR is a class proxy in this problem — the AF rhythm itself drives the feature down, independently of recording quality. Mid and high tertiles together hold less than 12 % of AF cases; deferral decisions in those regimes are essentially decisions about NSR and Other.

**The gain is cross-regime, not within-regime.** Within the high-SNR bin LW-CCSD is a no-op (+0.08 %): these are easy cases that the model already separates with confidence. Within the mid-SNR bin LW-CCSD gains +4.17 %: the deferral-meaningful regime where both model and SNR carry independent information. Within the low-SNR bin LW-CCSD posts a local AURC regression of −7.29 %. The three within-bin numbers sum to far less than the global +15.57 % improvement — the bulk of LW-CCSD’s value comes from how it re-orders samples *across* tertiles, not within any one of them.

Specifically, the policy lifts clean NSR (high-SNR bin) into the kept set via  $w_{\text{NSR}} = 0.3$ , protects AF (low-SNR bin) from SNR-penalisation via the small  $w_{\text{AF}} = 0.4$ , and pushes the deferred set toward an NSR/Other-dominated cohort of low-confidence-but-high-SNR samples — the regime where the classifier itself is least useful. This rearrangement is invisible inside any single bin.

**The within-low-bin regression is a structural limit.** Once conditioned on low SNR the feature stops discriminating — its variance has been removed. The only useful ranker inside the cohort is model confidence, so any positive weight on SNR can only hurt the local ordering. Critically, per-class AF recall in the low bin is



essentially preserved (0.803 vs 0.789,  $-1.4$  pp). The clinical decision the system is designed to support — keeping AF in the kept set where AF actually lives — is unaffected.

The stratified result therefore both validates the mechanism quantitatively ( $9\times$  AF concentration in the low-SNR tertile) and refines the deployment story: LW-CCSD is most valuable for systems that see mixed clean and noisy inputs and need a single coherent deferral policy across them. On a deployment that handles only one regime — e.g. a controlled clinical setting with consistently high signal quality — the marginal value of the method shrinks toward zero.

## 5.8 Cross-UQ SNR stratification

We repeat the SNR-tertile analysis under MC Dropout and deep ensemble confidences (Table 7). Both sources reproduce the cross-regime pattern. The ensemble case is the most striking: all three within-bin  $\Delta$  AURCs are *negative* (low  $-2.35\%$ , mid  $-0.19\%$ , high  $-6.64\%$ ), yet the global  $\Delta$  AURC is  $+4.57\%$ . Under a strong UQ method that already orders samples near-optimally within each bin, LW-CCSD’s entire value is in cross-regime re-ordering. This is the unifying mechanism statement across all three UQ sources studied in the paper.

**Table 7.** SNR-stratified cross-UQ replication on CinC test set. Global gain is positive everywhere; within-bin behaviour depends on the UQ source. Operating point selected per the floor-0.45 row of the cross-UQ comparison.

| UQ source       | SNR bin       | n     | UQ AURC | LW AURC | $\Delta$ AURC |
|-----------------|---------------|-------|---------|---------|---------------|
| MC Dropout      | low           | 2,250 | 0.2973  | 0.3172  | $-6.67\%$     |
|                 | mid           | 2,250 | 0.2209  | 0.2176  | $+1.53\%$     |
|                 | high          | 2,250 | 0.1337  | 0.1328  | $+0.66\%$     |
|                 | <b>global</b> | 6,750 | 0.1980  | 0.1899  | $+4.08\%$     |
| Ensembles (M=5) | low           | 2,287 | 0.3643  | 0.3729  | $-2.35\%$     |
|                 | mid           | 2,287 | 0.2003  | 0.2007  | $-0.19\%$     |
|                 | high          | 2,287 | 0.1483  | 0.1581  | $-6.64\%$     |
|                 | <b>global</b> | 6,861 | 0.2155  | 0.2057  | $+4.57\%$     |

## 5.9 HR-stratified evaluation

We orthogonally stratify the same test set by per-segment heart rate (FFT-peak estimate in the cardiac band). HR tertiles correspond to bradycardia/normocardia/tachycardia regimes. The class distribution makes this clinically interpretable: 424 of 559 AF segments (76 %) live in the high-HR bin ( $> 78$  bpm), a  $4\times$  enrichment over the low and mid HR bins. AF prevalence is  $3.7\%$ ,  $3.2\%$ , and  **$15.4\%$**  in the low / mid / high HR bins respectively. This matches the clinical signature of AF (irregular rhythm often with rapid ventricular response).

**Table 8.** HR-stratified evaluation on CinC test set (deterministic classifier,  $\mathbf{w}^* = (0.3, 0.4, 0.4)$ ). Per-segment HR estimated by FFT peak in  $[0.7, 3.0]$  Hz. AF concentrates in the high-HR tertile; AURC improves in every HR bin.

| HR bin (bpm)   | n     | NSR   | AF  | Other | UQ AURC | LW AURC | $\Delta$ AURC |
|----------------|-------|-------|-----|-------|---------|---------|---------------|
| low [42, 66]   | 1,671 | 1,023 | 62  | 586   | 0.3258  | 0.3046  | +6.52 %       |
| mid [66, 78]   | 2,317 | 1,623 | 73  | 621   | 0.3219  | 0.2249  | +30.13 %      |
| high [78, 174] | 2,762 | 1,431 | 424 | 907   | 0.1845  | 0.1518  | +17.74 %      |
| <b>global</b>  | 6,750 | 4,077 | 559 | 2,114 | 0.2367  | 0.1998  | +15.57 %      |

Unlike the SNR stratification, the HR stratification shows positive  $\Delta$  AURC in *every* bin, with the strongest gain in the mid-HR regime (+30.13 %). The LW-CCSD ranker operates on confidence and SNR, both of which are largely orthogonal to HR; the cross-regime re-ordering it performs therefore carries cleanly across HR ter-tiles.

One caveat is worth recording honestly. Within the high-HR bin, AF retention at within-bin 50 % coverage drops from 0.764 (UQ-only) to 0.066 (LW-CCSD). This is a *within-bin ordering* metric, not a deployment AF loss: the global LW-CCSD policy still preserves global AF recall at 0.626 ( $\Delta = -0.081$  from UQ-only), well within the 0.55 floor that selected this operating point. The within-bin drop reflects how the global ranker re-orders AF (which is intrinsically low-SNR) against high-HR NSR / Other inside this AF-dense bin. A deployment running at global coverage 0.5 does not see this 70-point per-bin shift on AF retention — it sees the global AF recall, which behaves as reported in Table 3. We flag the within-bin artifact for transparency, but it does not change the deployment story.

## 5.10 Continuous-w optimisation

The Pareto frontier in Table 3 was computed on a discrete 11-point grid for each class, yielding 1,331 candidates total. To rule out grid discretisation as the source of the small non-monotonicities observed in the test-side curve, we re-optimize the floor-0.55 operating point using Nelder–Mead on continuous  $\mathbf{w} \in [0, 1]^3$  with a soft-penalty AF-recall constraint and 8 random restarts (one warm-started from the grid optimum).

**Table 9.** Grid vs continuous- $\mathbf{w}$  optimisation at floor = 0.55, constraint coverage = 0.50. The Nelder–Mead optimum lies in the same neighbourhood as the grid optimum; test AURC is marginally worse due to val-to-test generalisation, confirming the grid is sufficient.

| Optimiser                | $\mathbf{w}^*$ (NSR / AF / Other) | val AURC | test AURC | $\Delta$ vs UQ | AF cost |
|--------------------------|-----------------------------------|----------|-----------|----------------|---------|
| Grid (11 <sup>3</sup> )  | 0.30 / 0.40 / 0.40                | 0.2210   | 0.1998    | +15.6 %        | -0.081  |
| Continuous (Nelder–Mead) | 0.16 / 0.43 / 0.48                | 0.2202   | 0.2015    | +14.9 %        | -0.077  |

The continuous optimum sits in the same neighbourhood as the grid optimum and gives marginally better val AURC (0.2202 vs 0.2210) but marginally worse test AURC (0.2015 vs 0.1998, +0.8 % relative regression). This is val-to-test generalisation noise: the finer optimiser locks in a slightly better val-set fit that does not generalise as tightly. The small non-monotonicities in the test-side Pareto frontier reported in Section 5.3 are

therefore discretisation-and-generalisation artifacts, not optimisation artifacts — the grid is sufficient and the recommended operating point is robust to optimiser choice.

### 5.11 Clean ensemble methodology — decoupling `data_seed` from `model_seed`

The original ensemble in Section 5.4 was trained with the legacy single-seed API, which inadvertently caused the five members to see five *different* train/val/test splits in addition to different initialisations. Standard deep-ensemble methodology (Lakshminarayanan *et al.* 2017) prescribes a shared split with independent initialisations — ensemble diversity should come from initialisation alone, not from split-induced data variance. We retrained the five-member ensemble with separated `data_seed` (shared) and `model_seed` (varied) and report the result in Table 10.

**Table 10.** Coupled-seed vs clean-seed five-model ensemble on CinC test set (n = 6,750). Clean methodology improves both UQ quality (lower AURC, lower ECE) and the magnitude of the LW-CCSD margin on top.

| Methodology                                             | Test<br>Acc | ECE ↓ | Brier<br>↓ | UQ-only<br>AURC | Best safe<br>LW-CCSD<br>AURC | Δ LW-<br>CCSD |
|---------------------------------------------------------|-------------|-------|------------|-----------------|------------------------------|---------------|
| Coupled seed (original)                                 | 0.686       | 0.064 | 0.440      | 0.2155          | 0.2086                       | +3.2 %        |
| <b>Clean seed (shared<br/>split, independent inits)</b> | 0.692       | 0.052 | 0.440      | 0.2066          | 0.1928                       | +6.7 %        |

Two findings.

**The split-induced variance was injecting noise into the calibration story.** Under clean methodology, ECE drops from 0.064 to 0.052 (1.2-point absolute reduction) and test AURC drops from 0.2155 to 0.2066 (4.1 % relative improvement) — both with no architectural change. The original ensemble’s split-induced variance was systematically masking the UQ quality the architecture is actually capable of.

**The LW-CCSD gain is larger under clean methodology, not smaller.** Best safe operating point moves from +3.2 % AURC (coupled) to +6.7 % AURC (clean). Two complementary mechanisms account for this: (a) when ensemble members saw different splits, their per-segment uncertainty included a noise component due to which-split-this-was rather than how-uncertain-the-classifier-actually-is; under shared-split methodology the confidence ranking is closer to a clean estimate of within-record uncertainty, and SNR adds more discriminating cross-regime information on top; (b) better calibration means the LW-CCSD optimiser’s val-AURC objective is closer to the test-AURC quantity it actually cares about, yielding operating points that generalise more tightly.

Note that the deployment punchline strengthens under the clean ensemble baseline: deterministic + LW-CCSD (0.1998) still beats clean ensemble UQ-only (0.2066) by 3.3 % relative AURC at one-fifth the inference compute. The substitution claim was not artifactual of the original ensemble’s methodology weakness; it holds against the cleaner baseline.

## 5.12 Evidential Deep Learning — in-method signal-quality absorption

We add Evidential Deep Learning (EDL) as a fourth UQ source. EDL replaces the softmax head with a non-negative evidence head, producing Dirichlet concentrations  $\alpha = \text{softplus}(\text{linear}(h)) + 1$  at the output. The classification loss is the EDL Type-II MSE with annealed KL regularisation (Sensoy *et al.* 2018), with KL weight annealed linearly from 0 to 1 over the first 10 epochs. Predictive probabilities are  $p = \alpha / S$  where  $S = \sum_c \alpha_c$ ; the Dirichlet uncertainty is  $u = K / S$  (high when total evidence is low). Confidence for selective evaluation is  $-u$ . Architecture and training otherwise match the deterministic baseline.

**Table 11.** EDL on CinC test set ( $n=6,750$ ). Single checkpoint,  $\text{data\_seed} = 42$ , KL annealing 10 epochs.

| Method                   | Test Acc | ECE ↓ | Brier ↓ | UQ-only AURC |
|--------------------------|----------|-------|---------|--------------|
| Deterministic            | 0.686    | —     | 0.440   | 0.2367       |
| MC Dropout ( $T=30$ )    | 0.715    | 0.076 | 0.418   | 0.1980       |
| Clean Ensemble ( $M=5$ ) | 0.692    | 0.052 | 0.440   | 0.2066       |
| <b>EDL</b>               | 0.739    | 0.137 | 0.426   | 0.1725       |

EDL has the best UQ-only AURC and the best test accuracy of all four methods studied — a 16.6 % relative AURC improvement over the clean ensemble at one-fifth the inference compute, and a 27.1 % improvement over the deterministic baseline. EDL is also the worst-calibrated of the four (ECE 0.137 vs 0.052–0.076 for the others), consistent with the EDL literature: the Dirichlet evidence head trades calibration sharpness for ranking quality and explicit-uncertainty modelling. The high ECE does *not* degrade AURC — quite the opposite.

**Table 12.** LW-CCSD Pareto frontier on EDL. Val UQ-only AF recall at  $c_0 = 0.50$  is 0.313, so floors  $\geq 0.35$  are infeasible. Every feasible operating point sits above UQ-only on test AURC — LW-CCSD does not improve EDL's selective ranking.

| Val AF floor     | $w^*$ (NSR/AF/Other)   | Test AURC | $\Delta$ vs UQ | Test AF@0.5 | $\Delta$ AF |
|------------------|------------------------|-----------|----------------|-------------|-------------|
| 0.20             | 0.0 / 0.5 / 0.4        | 0.1777    | −3.02 %        | 0.331       | −0.068      |
| 0.25             | 0.0 / 0.4 / 0.4        | 0.1770    | −2.65 %        | 0.367       | −0.032      |
| 0.28             | 0.0 / 0.4 / 0.4        | 0.1770    | −2.65 %        | 0.367       | −0.032      |
| <b>0.30</b>      | <b>0.0 / 0.3 / 0.4</b> | 0.1764    | −2.28 %        | 0.386       | −0.013      |
| UQ-only baseline | —                      | 0.1725    | —              | 0.399       | 0.000       |

**Mechanism — why LW-CCSD does not help EDL.** Spectral SNR provides cross-regime information that the model's confidence does not have access to: a noisy waveform produces a low SNR independently of what the classifier thinks. For deterministic, MC Dropout, and ensemble confidences this signal is genuinely orthogonal to the model output, which is why LW-CCSD recovers margin on all three. EDL is different: under the EDL training objective, an input that lacks a clean cardiac rhythm produces *low evidence on every class*, hence low total  $\alpha$ , hence high Dirichlet uncertainty  $u = K/S$ . EDL has *learned in-method* exactly the cross-regime ranking that SNR would supply externally. Mixing the two ranks is therefore double-counting the same content, and the

rank-noise component of the externally-computed SNR rank now reduces selective quality rather than adding to it.

This is a falsifiable mechanism prediction. Any UQ method that conditions on input signal quality directly — SNGP via its distance-aware feature norm, evidential variants, or learned-extractor models that propagate uncertainty from the rPPG stage forward — should similarly admit no LW-CCSD margin. The remaining three families (post-hoc softmax confidence, stochastic-pass disagreement, ensemble disagreement) all leave SNR-content unmodelled and therefore admit margin. **Section 5.13 tests this prediction with SNGP and refutes it.**

**Deployment update.** The recommendation chain across compute budgets now reads:

- **Smallest budget:** deterministic + LW-CCSD — test AURC 0.1998. Lightweight single-pass inference plus the free post-hoc deferral rule.
- **Standard budget:** single-pass EDL — test AURC 0.1725. Same inference cost as deterministic, one additional training pass with the EDL loss. Best AURC of all four methods and best test accuracy.
- **Maximum budget:** clean ensemble + LW-CCSD — test AURC 0.1928. Five-model inference plus deferral.

EDL at the standard budget dominates both the lightweight and the maximum configurations on AURC, at single-pass inference cost. For clinical-screen deployment the simplest defensible choice is therefore EDL alone — no auxiliary feature, no per-class weights, no ensemble.

### 5.13 SNGP — falsifying the input-conditional-UQ mechanism

We add SNGP (Liu *et al.* 2020) as a fifth UQ source. SNGP replaces the softmax head with a Random Fourier Features projection followed by a Bayesian Gaussian-process layer, and applies spectral normalisation (coefficient 0.95) to every Conv1d and Linear layer in the backbone. After standard CE training, a diagonal precision matrix is accumulated over a full training-set pass and inverted to yield a per-logit variance; at inference, the mean-field correction  $\text{softmax}(\mu / \sqrt{1 + (\pi/8) \sigma^2})$  produces calibrated probabilities. The backbone is spectral-norm-Lipschitz, so the feature map is distance-preserving and the GP variance grows on inputs far from the training distribution — exactly the “distance-aware” UQ that Section 5.12 hypothesised would absorb signal-quality information.

**Table 13.** SNGP on CinC test set ( $n = 6,750$ ). Single checkpoint, `data_seed = 42`, RFF  $D = 1024$ , ridge  $10^{-3}$ , spectral-norm coefficient 0.95.

| Method                     | Test Acc | ECE ↓ | Brier ↓ | UQ-only AURC |
|----------------------------|----------|-------|---------|--------------|
| Deterministic              | 0.686    | —     | 0.440   | 0.2367       |
| MC Dropout ( $T = 30$ )    | 0.715    | 0.076 | 0.418   | 0.1980       |
| Clean Ensemble ( $M = 5$ ) | 0.692    | 0.052 | 0.440   | 0.2066       |
| <b>SNGP</b>                | 0.729    | 0.029 | 0.393   | 0.2044       |
| EDL                        | 0.739    | 0.137 | 0.426   | 0.1725       |

SNGP has the *best test ECE of all five methods* (0.029, a 44 % relative improvement over the clean ensemble at the same single-pass inference cost) and the second-best test accuracy (0.729). On AURC it sits in the middle of the classical-UQ range. The headline question is whether LW-CCSD still adds margin.

**Table 14.** LW-CCSD Pareto frontier on SNGP. Val UQ-only AF recall at  $c_0 = 0.50$  is 0.085, so the floor sweep starts at 0.03.

| Val AF floor     | $w^*$ (NSR/AF/Other)   | Test AURC | $\Delta$ vs UQ | Test AF@0.5 | $\Delta$ AF |
|------------------|------------------------|-----------|----------------|-------------|-------------|
| 0.03             | 0.0 / 0.4 / 1.0        | 0.1979    | +3.16 %        | 0.052       | -0.047      |
| 0.05             | 0.0 / 0.2 / 1.0        | 0.1973    | +3.47 %        | 0.070       | -0.029      |
| <b>0.06</b>      | <b>0.0 / 0.1 / 1.0</b> | 0.1969    | +3.69 %        | 0.075       | -0.023      |
| 0.08             | 0.0 / 0.0 / 0.4        | 0.2019    | +1.24 %        | 0.098       | +0.000      |
| UQ-only baseline | —                      | 0.2044    | —              | 0.098       | 0.000       |

**SNGP admits a positive LW-CCSD margin of +3.7 %** at AF cost just -0.023, in the same range as MC Dropout (+4.1 %) and ensembles (+6.7 %). The Section 5.12 mechanism prediction is refuted: distance-aware UQ does *not* imply no-LW-CCSD-margin. EDL's negative margin is specific to EDL, not a generic property of input-conditional uncertainty.

**Why EDL is unique and SNGP is not.** Both methods are input-aware, but through different mechanisms. EDL's evidence collapses on inputs that lack a *confident-classifiable signal* — this is operationally identical to a signal-quality measurement, because a noisy rPPG signal lacks rhythm template, harmonic structure, and consistent beat morphology, and therefore produces low evidence on every class. SNGP's variance grows on inputs *far from the training distribution in feature space*. Signal quality and feature-space distance are correlated but distinct: a clean signal from an under-represented record can be far in feature space, and a noisy signal from a well-represented record can be close. SNR adds information about signal quality that the GP variance does not capture, and that is precisely the information LW-CCSD's external SQI rank provides.

The revised mechanism statement is therefore narrower: EDL's no-LW-CCSD-margin behaviour stems from a specific property of the EDL training objective — evidence collapses on inputs that lack a confident-classifiable signal, which is operationally identical to a signal-quality measurement. This is *not* a property of input-conditional UQ in general. The classification of UQ sources is finer than “input-conditional vs. not”: it is “evidence-on-noisy-signal-collapses” vs. “feature-space-distance-tracks” vs. “stochastic-disagreement”, and only the first family is redundant with external SQI.

**Deployment update.** The recommendation chain across compute budgets becomes:

- **Smallest budget:** deterministic + LW-CCSD — test AURC 0.1998. Lightweight single-pass plus deferral.
- **Standard budget (AURC-first):** single-pass EDL — test AURC 0.1725.
- **Standard budget (calibration-first):** single-pass SNGP + LW-CCSD — test AURC 0.1969, test ECE 0.029 (best of all five). Recommended when reliability diagrams are part of the deployment contract.
- **Maximum budget:** clean ensemble + LW-CCSD — test AURC 0.1928.

Adding SNGP gives the practitioner a calibration-first choice that EDL cannot provide — EDL has the worst ECE of all five methods (0.137 vs SNGP's 0.029). For a clinical-screen system where regulators inspect calibration plots, SNGP + LW-CCSD is the defensible choice.

## 5.14 EDL ensemble — variance characterisation and mechanism confirmation

The Section 5.12 EDL result is from a single checkpoint. Two natural follow-up questions: (a) how stable is EDL across initialisation seeds? and (b) does the no-LW-CCSD-margin property survive ensembling? We train four additional EDL members ( $\text{model\_seed} \in \{2, 3, 4, 5\}$ , shared  $\text{data\_seed} = 42$ ), then form a 5-member EDL ensemble by averaging Dirichlet concentrations across members before computing predictive probabilities and uncertainty.

**Table 15.** EDL ensemble on CinC test set ( $n = 6,750$ ). Per-member statistics characterise the seed-to-seed variance; the  $M = 5$  row is the ensemble.

| Configuration                            | Test Acc               | ECE ↓                | Brier ↓              | UQ-only AURC           |
|------------------------------------------|------------------------|----------------------|----------------------|------------------------|
| EDL member $m=1$ (Section 5.12)          | 0.7390                 | 0.138                | 0.426                | 0.1725                 |
| EDL member $m=2$                         | 0.7356                 | 0.140                | 0.432                | 0.1685                 |
| EDL member $m=3$                         | 0.7434                 | 0.139                | 0.423                | 0.1655                 |
| EDL member $m=4$                         | 0.7418                 | 0.135                | 0.423                | 0.1679                 |
| EDL member $m=5$                         | 0.7430                 | 0.140                | 0.425                | 0.1664                 |
| Per-member mean $\pm$ std                | 0.7405 $\pm$<br>0.0033 | 0.138 $\pm$<br>0.002 | 0.426 $\pm$<br>0.003 | 0.1681 $\pm$<br>0.0027 |
| <b>EDL ensemble (<math>M = 5</math>)</b> | 0.7468                 | 0.144                | 0.422                | 0.1640                 |

Three findings:

**EDL is variance-stable across seeds.** Per-member AURC standard deviation is 0.0027 on a mean of 0.1681 — 1.6 % relative spread. The Section 5.12 result (member  $m=1$ , AURC 0.1725) sits at the upper end of the per-member distribution but well within the typical seed-to-seed range. The EDL headline is reproducible across initialisations.

**EDL ensemble is the strongest configuration studied.** Test AURC 0.1640 — 4.9 % relative improvement over best single EDL (0.1725) and 20.6 % relative improvement over the clean softmax ensemble at the same  $M = 5$  inference budget (0.2066). Test accuracy 0.7468 (best of any configuration). Brier 0.422 (best of any configuration). ECE 0.144 (slightly worse than worst single-member ECE, reflecting Dirichlet sharpening under averaging). For an AURC-first deployment with five-pass inference budget, EDL ensemble dominates all alternatives.

**Table 16.** LW-CCSD Pareto on the EDL ensemble. Val UQ-only AF recall at  $c_0 = 0.50$  is 0.298, so floors  $\geq 0.35$  are infeasible.

| Val AF floor     | $w^*$ (NSR/AF/Other)   | Test AURC | $\Delta$ vs UQ | Test AF@0.5 | $\Delta$ AF |
|------------------|------------------------|-----------|----------------|-------------|-------------|
| 0.20             | 0.0 / 0.4 / 0.3        | 0.1688    | -2.91 %        | 0.347       | -0.036      |
| 0.25             | 0.0 / 0.4 / 0.3        | 0.1688    | -2.91 %        | 0.347       | -0.036      |
| 0.28             | 0.0 / 0.4 / 0.3        | 0.1688    | -2.91 %        | 0.347       | -0.036      |
| <b>0.30</b>      | <b>0.0 / 0.3 / 0.3</b> | 0.1679    | -2.40 %        | 0.372       | -0.011      |
| UQ-only baseline | —                      | 0.1640    | —              | 0.383       | 0.000       |

**LW-CCSD remains structurally negative on the EDL ensemble.** Every feasible operating point produces negative  $\Delta$  AURC, ranging from -2.91 % at floor 0.20 to -2.40 % at the best safe floor (0.30, AF cost -0.011). This confirms the Section 5.12 mechanism is structural to the EDL training objective rather than a property of any one initialisation: ensembling EDL members averages their evidence heads but does not change the fact that each member's evidence collapses on noisy signals. The redundancy with external SNR therefore persists at the ensemble level.

#### Final deployment chain.

- **Smallest budget:** deterministic + LW-CCSD — test AURC 0.1998. Single-pass.
- **Standard budget (AURC-first, single pass):** single-pass EDL — test AURC 0.1725.
- **Standard budget (calibration-first, single pass):** SNGP + LW-CCSD — test AURC 0.1969, test ECE 0.029.
- **Maximum AURC (M = 5 inference):** EDL ensemble — test AURC **0.1640**, test acc **0.747**, test Brier **0.422** — the strongest configuration studied.
- **Maximum calibration (M = 5 inference):** clean softmax ensemble + LW-CCSD — test AURC 0.1928, test ECE 0.052.

EDL ensemble is the new recommended choice when the deployment can afford the M = 5 inference budget and AURC is the primary objective. The EDL mechanism makes its own LW-CCSD redundant at every scale.

### 5.15 EDL under conformal coverage — robustness of the negative margin

Section 5.12 establishes a negative LW-CCSD margin on single-checkpoint EDL using empirical-floor optimisation. Section 5.14 confirms the margin survives ensembling. A reviewer may still ask: is the negative margin robust to the conformal coverage machinery? We replicate the Section 5.6 per-class, Bonferroni, and Holm step-down conformal procedures on the EDL val predictions at family-wise (or per-class)  $\alpha = 0.10$ . Table 17 reports the best safe operating point for each mode.

**Table 17.** EDL LW-CCSD under empirical, per-class conformal, Bonferroni joint, and Holm step-down joint feasibility tests. Single EDL checkpoint, CinC test set, constraint coverage 0.50. Family-wise (or per-class)  $\alpha = 0.10$ . Every conformal mode produces a negative test  $\Delta$  AURC — the Section 5.12 finding is robust to the strongest probabilistic guarantee.



| Mode                                                                | Floor       | $\mathbf{w}^*$ (NSR/<br>AF/Other) | Test<br>AURC | $\Delta$ vs<br>UQ-only | Test<br>AF@0.5 | $\Delta$ AF |
|---------------------------------------------------------------------|-------------|-----------------------------------|--------------|------------------------|----------------|-------------|
| Empirical floor (Section 5.12)                                      | 0.30        | 0.0 / 0.3 / 0.4                   | 0.1764       | -2.28 %                | 0.386          | -0.013      |
| <b>Per-class conformal, <math>\alpha = 0.10</math></b>              | <b>0.28</b> | <b>0.0 / 0.2 / 0.4</b>            | 0.1759       | -2.00 %                | 0.394          | -0.005      |
| Bonferroni joint, family-wise $\alpha = 0.10$                       | 0.25        | 0.0 / 0.4 / 0.4                   | 0.1770       | -2.65 %                | 0.367          | -0.032      |
| <b>Holm step-down joint, family-wise <math>\alpha = 0.10</math></b> | <b>0.28</b> | <b>0.0 / 0.2 / 0.4</b>            | 0.1759       | -2.00 %                | 0.394          | -0.005      |
| UQ-only baseline (no LW-CCSD)                                       | —           | —                                 | 0.1725       | —                      | 0.399          | 0.000       |

Three findings.

**The negative margin survives every conformal mode.** Empirical -2.28 %, per-class conformal -2.00 %, Bonferroni -2.65 %, Holm -2.00 %. There is no conformal LCB tightening that flips the EDL frontier positive.

**Per-class and Holm produce the identical optimum on EDL.** Both at floor 0.28,  $\mathbf{w}^* = (0, 0.2, 0.4)$ , AURC 0.1759, AF cost -0.005. The EDL optimisation landscape near the AF-only axis is flat enough that the per-class  $\rightarrow$  Holm LCB tightening does not shift  $\mathbf{w}^*$ . On the deterministic baseline Holm strictly dominates per-class on the joint statement (Section 5.6); on EDL the two procedures coincide.

**Bonferroni's conservatism replicates.** Bonferroni picks a stricter feasible floor (0.25 vs 0.28), with AURC 0.0011 worse and AF cost six times larger. The Section 5.6 result that Bonferroni is conservative for  $C = 3$  holds on EDL exactly as on the deterministic baseline.

The headline EDL claim therefore reads, in its strongest form: EDL admits negative LW-CCSD margin under empirical optimisation (Section 5.12), under ensembling (Section 5.14), and under per-class conformal, Bonferroni joint, and Holm step-down joint coverage at family-wise  $\alpha = 0.10$  (this section). The redundancy with external SNR is not a feature of any single optimisation or feasibility test — it is a structural property of EDL training.

## 6 Discussion

### 6.1 Why the Method Works

LW-CCSD succeeds because spectral SNR carries deferral-relevant information that model confidence does not, but only for some predicted classes. Predictions of NSR or Other rhythms on noisy windows are typically over-confident: the classifier learned features tied to rhythm regularity, which are corrupted by camera motion, lighting flicker, and partial face occlusion in ways the per-window confidence score cannot detect. SNR exposes this corruption directly. Predictions of AF, on the other hand, are correctly less confident on noisy windows (because the AF-defining irregularity raises uncertainty in the same direction as motion noise) but

*also* less confident on clean windows (because regularity is the NSR signature). Weighting SNR on AF predictions therefore double-counts the irregularity penalty and rejects positives. The learned per-class weight resolves this: the optimiser discovers a small or zero weight on the AF class and larger weights on NSR / Other, precisely where SNR adds orthogonal information.

## 6.2 Deployment Implications

LW-CCSD applied to a single-pass deterministic classifier achieves test AURC 0.1998 at AF-recall cost  $-0.081$  (operating point: val floor 0.55). An unaugmented five-model deep ensemble (clean methodology, Section 5.11) on the same data achieves test AURC 0.2066 — worse, at five times the inference compute. The lightweight model plus the free post-hoc deferral rule outperforms ensembling. For clinical-screen deployment where compute and latency budgets are tight, this suggests LW-CCSD is a viable substitute for ensembling rather than an add-on to it.

The cross-UQ pattern also has a practical implication: when investing in stronger UQ (MC Dropout at  $T=30$ , ensembles at  $M=5$ ), the marginal value of adding SNR-based deferral shrinks. A deployed system should therefore make the UQ-method choice and the SQI-deferral choice jointly — they are partial substitutes, not independent additions.

## 6.3 Limitations

The main benchmark uses synthetic rPPG derived from ECG, not real face-video rPPG. The synthesis preserves rhythm structure (which the classifier ultimately relies on for AF detection) but abstracts away morphological details that real rPPG would also lack. We expect the qualitative trends to transfer to real face-video AF data, particularly the central failure mode of naïve SQI deferral on AF, which depends only on the spectral concentration of cardiac-band energy and not on synthesis details. Quantitative magnitudes (the exact size of the  $+15.6\%$  deterministic AURC gain, the exact slope of the Pareto frontier) may shift on real data. Replication on OBF [4] or MAHNOB-HCI is the natural next step pending data access.

The LW-CCSD optimiser uses a discrete 11-point grid. Generalisation noise from grid discreteness manifests as small non-monotonicities in the test-side Pareto curve. A continuous gradient-free optimiser (Nelder–Mead, CMA-ES) on val AURC subject to constraint penalties would smooth this and is a natural refinement. The conformal feasibility check formulated in Section 5.6 transfers unchanged to the continuous setting.

## 6.4 Generality of the Pattern

The core failure mode — aggregate-metric improvement that comes from systematically rejecting the minority class because the class-defining signal collides with the auxiliary deferral feature — is not specific to rPPG-AF screening. It appears whenever the auxiliary feature is correlated with class identity in ways the aggregate metric does not capture. The fix — learn per-class weights subject to per-class recall constraints — is correspondingly general. LW-CCSD as formulated here applies directly to any classification task with a continuous auxiliary quality feature and a per-class safety floor, and is a candidate methodology for the broader literature on selective prediction in clinical AI.

## 7 Conclusion

---

We introduced LW-CCSD, a post-hoc class-conditional deferral procedure that learns per-predicted-class signal-quality weights subject to a configurable safety floor. On a 45,064-segment synthetic-rPPG benchmark, LW-CCSD recovers most of the aggregate AURC gain of naïve signal-quality deferral while preserving AF recall, and applied to a lightweight single-pass classifier it outperforms an unaugmented five-model deep ensemble. The method is model-agnostic, requires no retraining, and generalises across three uncertainty quantification methods. We release the full pipeline and CinC-derived synth-rPPG substrate under MIT licence; replication on real face-video AF data is a natural next step pending OBF / MAHNOB-HCI access.

## Acknowledgments

---

This work uses public datasets — PhysioNet/CinC 2017 AF Challenge and the MIT-BIH Arrhythmia Database — whose maintainers are gratefully acknowledged.

## Data and Code Availability

---

Open-source pipeline including all scripts, configurations, trained checkpoints, and per-method evaluation artefacts is available at [github.com/ShahnawazKakarh/rppg-selective-arrhythmia](https://github.com/ShahnawazKakarh/rppg-selective-arrhythmia) under MIT licence. The CinC-derived synthetic-rPPG cache is reproducible from the released code in approximately 20 minutes of CPU time on a recent laptop.

## Conflict of Interest Statement

---

The author declares no competing interests.

## References

---

1. G. de Haan and V. Jeanne, “Robust pulse rate from chrominance-based rPPG,” *IEEE Transactions on Biomedical Engineering*, vol. 60, no. 10, pp. 2878–2886, 2013.
2. W. Wang, A. C. den Brinker, S. Stuijk and G. de Haan, “Algorithmic principles of remote PPG,” *IEEE Transactions on Biomedical Engineering*, vol. 64, no. 7, pp. 1479–1491, 2017.
3. Z. Yu, W. Peng, X. Li, X. Hong and G. Zhao, “Remote heart rate measurement from highly compressed facial videos: an end-to-end deep learning solution with video enhancement,” *Proc. IEEE/CVF ICCV*, 2019.
4. X. Li, I. Alikhani, J. Shi, T. Seppänen, J. Junntila, K. Majamaa-Voltti, M. Tulppo and G. Zhao, “The OBF database: a large face video database for remote physiological signal measurement and atrial fibrillation detection,” *Proc. IEEE FG*, 2018.
5. B. P. Yan, W. H. S. Lai, C. K. Y. Chan et al., “Detection of atrial fibrillation from facial videos using consumer-grade cameras,” *Scientific Reports*, vol. 12, art. 13176, 2022.

6. Y. Gal and Z. Ghahramani, “Dropout as a Bayesian approximation: representing model uncertainty in deep learning,” *Proc. ICML*, 2016.
7. B. Lakshminarayanan, A. Pritzel and C. Blundell, “Simple and scalable predictive uncertainty estimation using deep ensembles,” *NeurIPS*, 2017.
8. M. Sensoy, L. Kaplan and M. Kandemir, “Evidential deep learning to quantify classification uncertainty,” *NeurIPS*, 2018.
9. J. Z. Liu, Z. Lin, S. Padhy, D. Tran, T. Bedrax-Weiss and B. Lakshminarayanan, “Simple and principled uncertainty estimation with deterministic deep learning via distance awareness,” *NeurIPS*, 2020.
10. A. N. Angelopoulos and S. Bates, “A gentle introduction to conformal prediction and distribution-free uncertainty quantification,” *arXiv:2107.07511*, 2021.
11. Y. Geifman and R. El-Yaniv, “Selective classification for deep neural networks,” *NeurIPS*, 2017.
12. M. P. Naeini, G. F. Cooper and M. Hauskrecht, “Obtaining well-calibrated probabilities using Bayesian binning,” *AAAI*, 2015.
13. G. D. Clifford, C. Liu, B. Moody, L. H. Lehman, I. Silva, Q. Li, A. E. W. Johnson and R. G. Mark, “AF classification from a short single lead ECG recording: the PhysioNet/Computing in Cardiology Challenge 2017,” *Computing in Cardiology (CinC)*, 2017.
14. G. B. Moody and R. G. Mark, “The impact of the MIT-BIH arrhythmia database,” *IEEE Engineering in Medicine and Biology Magazine*, vol. 20, no. 3, pp. 45–50, 2001.