Residual-limb FEA run report

synthetic_human_T75

run id `synthetic_human_T75` created 2026-10-15T15:24:10Z

Job state: CONVERGED. Solver: FEBio 4.13.0.32ae206ff. Load model: resolved_contact. **Numerical verification only: this report does not establish clinical accuracy, socket grip or tissue safety.** Geometry: **SYNTHETIC** (no patient data).

Warnings and labelled assumptions

- Socket geometry is a PROVISIONAL parametric model generated from configuration values; no verified current socket CAD was supplied (V6 excluded).
- No verified RevoFit rated strand tension supplied: rated-tension cases (25/50/75/100%) are NOT run.
- Strand tension 75 N is an EXAMPLE value, not a verified rating.
- Material 'skin' uses assumed (unsourced) parameters: k.
- Material 'silicone_pad' uses assumed (unsourced) parameters: c1, c2, k.
- Material 'distal_cushion' uses assumed (unsourced) parameters: c1, c2, k.
- Each petal hinge is a frictionless revolute joint (penalty 1e4 N/mm, 1e7 N mm/rad). A radial stabiliser spring k = 0.05 N/mm per petal is NUMERICAL STABILISATION; its force and energy are reported.
- Cable span forces are applied to the rigid petals as fixed-direction resultant force and moment about each petal's centre of mass (directions do not follow petal rotation).

1 Inputs and provenance

input	path	sha256 (prefix)
config	/home/claude/residual-limb-fea/configs/synthetic_human.yaml	a133ad6196904481...
material_set	/home/claude/residual-limb-fea/configs/materials/human_tissue.yaml	f2b663785c96bfac...

Repository commit: `cce4b5c5c261fbe16793ff4d303bd86b74a2e321` (dirty worktree: True). Solver input `solver/model.feb` sha256 `8c3ee968fe0c49b02635...`. Execution command: `/usr/local/bin/febio4 -nosplash -silent -noconfig -i model.feb -dump model.dmp`.

1.1 Geometry audit

body	status	source unit	dims mm	vol mm3	closed	comp.	self-int.	d
skin	VALID_CLOSED_SURFACE	mm	100.7x103.5x199.6	1.49479e+06	True	1	0	
tibia	VALID_CLOSED_SURFACE	mm	66x52.44x133.7	71643	True	1	0	
fibula	VALID_CLOSED_SURFACE	mm	18x16.2x97.8	10555.8	True	1	0	

Anatomy roles (as configured): tibia: tibia (synthetic), fibula: fibula (synthetic).

SYNTHETIC geometry: not patient data, not anatomically measured.

body	fraction inside skin	min clearance mm	skin intersections
tibia	1	4	0
fibula	1	13.58	0

2 Model

Layer thicknesses are configurable geometric assumptions, NOT patient-specific segmentation. Skin thickness {"min": 0.8, "p01": 0.8, "median": 1.5, "max": 1.5} mm; fat thickness {"min": 0.8, "p01": 0.8, "median": 3.0, "max": 3.0} mm. 124 skin vertices had layer thickness reduced near bone. Minimum wedge scaled Jacobian 0.188.

id	block	element	material	region	formulation
0	skin	penta6	skin	skin	three-field-solid
1	fat	penta6	fat	fat	three-field-solid
2	proximal_cap	penta6	muscle	muscle (layers under artificial proximal cut)	three-field-solid
3	muscle	tet4	muscle	muscle	ut4-solid
4	bone_tibia	tet4	rigid_bone_tibia	bone:tibia	bone
5	bone_fibula	tet4	rigid_bone_fibula	bone:fibula	bone
6	petal1_pad	hex8	silicone_pad	socket:petal1:silicone pad	three-field-solid
7	petal1_shell	hex8	rigid_petal1	socket:petal1:rigid petal	rigid
8	petal2_pad	hex8	silicone_pad	socket:petal2:silicone pad	three-field-solid
9	petal2_shell	hex8	rigid_petal2	socket:petal2:rigid petal	rigid
10	petal3_pad	hex8	silicone_pad	socket:petal3:silicone pad	three-field-solid
11	petal3_shell	hex8	rigid_petal3	socket:petal3:rigid petal	rigid
12	petal4_pad	hex8	silicone_pad	socket:petal4:silicone pad	three-field-solid
13	petal4_shell	hex8	rigid_petal4	socket:petal4:rigid petal	rigid
14	petal5_pad	hex8	silicone_pad	socket:petal5:silicone pad	three-field-solid
15	petal5_shell	hex8	rigid_petal5	socket:petal5:rigid petal	rigid
16	petal6_pad	hex8	silicone_pad	socket:petal6:silicone pad	three-field-solid
17	petal6_shell	hex8	rigid_petal6	socket:petal6:rigid petal	rigid
18	distal_cushion	penta6	distal_cushion	socket:distal cushion	three-field-solid
19	distal_cup	penta6	rigid_cup	socket:rigid distal cup (+ puck/plate/adapter as support)	rigid

Strain-energy functions as implemented by FEBio 4.13 (checked against source and against an independent implementation for homogeneous deformations, Section ??). Isochoric invariants use $\tilde{\mathbf{C}} = J^{-2/3}\mathbf{C}$.

$$\text{HGO (skin):}\quad W = \tfrac{c}{2}(\tilde{I}_1 - 3) + \frac{k_1}{2k_2}\sum_{a=1,2}\left[e^{k_2\langle E_a\rangle^2} - 1\right] + \tfrac{k}{2}\left[\tfrac{J^2-1}{2} - \ln J\right], \quad E_a = \kappa(\tilde{I}_1 - 3) + (1 - 3\kappa)$$

$$\text{Ogden (fat, muscle):}\quad W = \sum_i \frac{c_i}{m_i^2}\left(\tilde{\lambda}_1^{m_i} + \tilde{\lambda}_2^{m_i} + \tilde{\lambda}_3^{m_i} - 3\right) + \tfrac{k}{2}(\ln J)^2$$

$$\text{Mooney–Rivlin (silicone, cushion):}\quad W = c_1(\tilde{I}_1 - 3) + c_2(\tilde{I}_2 - 3) + \tfrac{k}{2}(\ln J)^2$$

Fibre families lie at $\pm\gamma$ from local axis $\mathbf{e}_1$ in the $\mathbf{e}_1$–$\mathbf{e}_2$ plane and resist only tension ($E_a \geq 0$). FEBio's c equals ABAQUS $2C_{10}$; FEBio's HGO volumetric term equals ABAQUS GOH with $D = 2/k$. The sources' conventions and the conversions applied are listed per parameter in Table 2.

material	FEBio model	param	value (MPa/deg/-)	source	note
skin	Holzapfel-Gasser-Ogden	c	0.2014	NiAnnaidh2012	source mu; FEBio ground matrix W - 3), so c = mu (Abaqus C10 = m
skin	Holzapfel-Gasser-Ogden	k1	24.53	NiAnnaidh2012	source reports k1 = 243.6 in its c isation (anisotropic term scaled gives the ABAQUS value 24.53 ABAQUS value is used. FE
skin	Holzapfel-Gasser-Ogden	k2	0.1327	NiAnnaidh2012	
skin	Holzapfel-Gasser-Ogden	kappa	0.1404	NiAnnaidh2012	dispersion, 0 ¡= kappa ¡= 1/3
skin	Holzapfel-Gasser-Ogden	gamma	41	NiAnnaidh2012	angle of each fibre family from l (FEBio gamma). Mapping of Lar the lower leg to e1 is an ASSUM fiber_reference_axis
skin	Holzapfel-Gasser-Ogden	k	20.14	assumption	bulk modulus = 100 c (near-incor assumption). FEBio HGO uses U 1)/2 - ln J) (= ABAQUS GOH wit

material	FEBio model	param	value (MPa/deg/-)	source	note
fat	Ogden	c1	0.00522	Sengeh2016	source Psi = (c/mˆ2) sum(lˆˆm 2) == FEBio Ogden with c1=c2 m2=-m; small-strain shear modul
fat	Ogden	m1	4.79	Sengeh2016	
fat	Ogden	c2	0.00522	Sengeh2016	
fat	Ogden	m2	-4.79	Sengeh2016	
fat	Ogden	k	0.522	Sengeh2016	source constrained bulk = 100 c w (ln J)ˆ2, identical to FEBio press
muscle	Ogden	c1	0.0052	Sengeh2016	
muscle	Ogden	m1	4.78	Sengeh2016	
muscle	Ogden	c2	0.0052	Sengeh2016	
muscle	Ogden	m2	-4.78	Sengeh2016	
muscle	Ogden	k	0.52	Sengeh2016	
bone_deformable	neo-Hookean	E	1.7e+04	ReillyBurstein1975	human cortical bone, longitudinal the WHOLE bone volume (cortica not distinguished) - simplification
bone_deformable	neo-Hookean	v	0.3	ReillyBurstein1975	
silicone_pad	Mooney-Rivlin	c1	0.05	PriorPackageAssumption	ASSUMED: mu = 100 kPa -¿ c1 = ply the actual silicone's test data.
silicone_pad	Mooney-Rivlin	c2	0	assumption	
silicone_pad	Mooney-Rivlin	k	10	assumption	near-incompressible bulk modulus
distal_cushion	Mooney-Rivlin	c1	0.01	assumption	ASSUMED soft gel cushion, mu Supply measured data.
distal_cushion	Mooney-Rivlin	c2	0	assumption	
distal_cushion	Mooney-Rivlin	k	2	assumption	


References: [NiAnnaidh2012] Ni Annaidh A, Bruyere K, Destrade M, Gilchrist MD, Maurini C, Ottenio M, Saccomandi G. Automated estimation of collagen fibre dispersion in the dermis and its contribution to the anisotropic behaviour of skin. Ann Biomed Eng. 2012;40(8):1666-78. doi:10.1007/s10439-012-0542-3. [Sengeh2016] Sengeh DM, Moerman KM, Petron A, Herr H. Multi-material 3-D viscoelastic model of a transtibial residuum from in-vivo indentation and MRI data. J Mech Behav Biomed Mater. 2016;59:379-392. doi:10.1016/j.jmbbm.2016.02.020. [ReillyBurstein1975] Reilly DT, Burstein AH. The elastic and ultimate properties of compact bone tissue. J Biomech. 1975;8(6):393-405. doi:10.1016/0021-9290(75)90075-5. [PriorPackageAssumption] Supplied handoff package 03_Previous_Tissue_Analysis (silicone mu = 100 kPa listed as an assumed material; no measurement)..

2.1 Socket (provisional parametric model)

PROVISIONAL parametric socket (not verified design geometry).

3 Loading

Applied strand tension 75.0 N (basis: example). Rated tension: None. Output levels: [18.75, 37.5, 56.25, 75.0] N. PROVISIONAL default single-row lace generated from the parametric petals

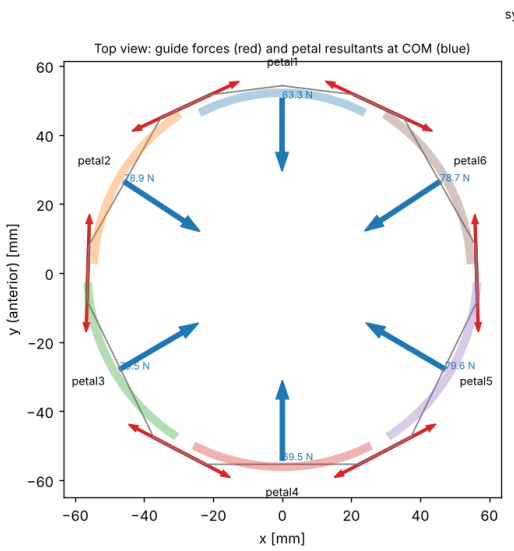

Lace tension 75.0 N (example); guide friction mu_g = 0.0

body	Fx N	Fy N	Fz N	Mx Nmm	My Nmm	Mz Nmm
petal1	-0.05	-63.35	0	701.9	-0.6	-7.2
petal2	65.91	-43.36	0	486.8	740	-188.9
petal3	68.56	40.21	0	-451	769	218.2
petal4	-0	69.53	0	-1652.8	-0.1	-4.3
petal5	-68.71	40.2	0	-450.9	-770.7	-220.1
petal6	-65.7	-43.23	0	485.1	-737.2	184.9
SUM F	-1.42e-14	-7.11e-15	0.00e+00			
SUM M@O				-9.09e-13	1.19e-12	0.00e+00

Figure 1: Lace route, guide forces and petal resultants (free-body check: sums must vanish).

4 Solver and convergence

Tolerances: dtol=0.01, etol=0.001, rtol=0.001; Newton with auto (max_ups=10); PARDISO; automatic time stepping with must points; max retries 10. Retries in log: 0; negative-Jacobian events: 0.

step	time	converged	iterations	final residual	final energy norm
1	0.02	yes	3	0.9354	0.003771
2	0.03291	yes	3	0.0007649	1.816e-05
3	0.04346	yes	2	0.0008547	8.976e-05
4	0.05	yes	2	0.0001712	1.591e-05
5	0.05795	yes	1	0.0002393	4.327e-05
6	0.0659	yes	1	0.0006157	7.63e-05
7	0.07385	yes	1	0.001038	9.225e-05
8	0.1	yes	2	0.033	0.0006205
9	0.1309	yes	2	0.04145	0.000135
10	0.15	yes	2	0.01543	0.0001784
11	0.1693	yes	2	0.03312	5.09e-05
12	0.1857	yes	2	0.08602	0.0003582
13	0.199	yes	2	0.04596	0.0001591
14	0.2	yes	4	0.008493	1.425e-06
15	0.2065	yes	2	0.002262	9.273e-05
16	0.2125	yes	1	0.05165	0.0002696
17	0.2424	yes	2	0.0512	0.0001245
18	0.25	yes	2	0.0142	0.0001983
19	0.2731	yes	1	0.06667	0.0002988
20	0.3	yes	1	0.08614	0.0002936
21	0.35	yes	2	0.1203	0.0005762
22	0.4	yes	2	0.04112	0.002734
23	0.45	yes	1	0.1713	0.001193
24	0.5	yes	1	0.02785	0.002206
25	0.55	yes	2	0.003768	0.0004974
26	0.6	yes	1	0.1041	0.003585
27	0.65	yes	1	0.05572	0.00314
28	0.7	yes	1	0.2139	0.001353
29	0.75	yes	1	0.1058	0.0006972
30	0.8	yes	1	0.1664	0.002454
31	0.85	yes	2	0.5014	0.004299
32	0.9	yes	1	0.2174	0.00331
33	0.95	yes	1	1.064	0.002581
34	1	yes	1	1.042	0.002735
1	1.02	yes	2	0.01022	0.001173
2	1.038	yes	2	0.009071	0.0009467

step	time	converged	iterations	final residual	final energy norm
3	1.053	yes	1	0.01007	9.341e-05
4	1.081	yes	1	0.04313	0.001143
5	1.1	yes	2	0.06953	0.002815
6	1.124	yes	1	0.02381	0.00057
7	1.16	yes	1	0.2487	0.0004394
8	1.2	yes	1	0.06012	0.0003378
9	1.3	yes	1	6.65	0.004431
10	1.4	yes	1	0.2527	0.003898
11	1.5	yes	1	0.2669	0.007533
12	1.6	yes	1	0.1411	0.0003358
13	1.7	yes	1	0.5701	0.003064
14	1.8	yes	1	0.3311	0.002816
15	1.9	yes	1	0.299	0.00451
16	2	yes	1	0.2972	0.002778

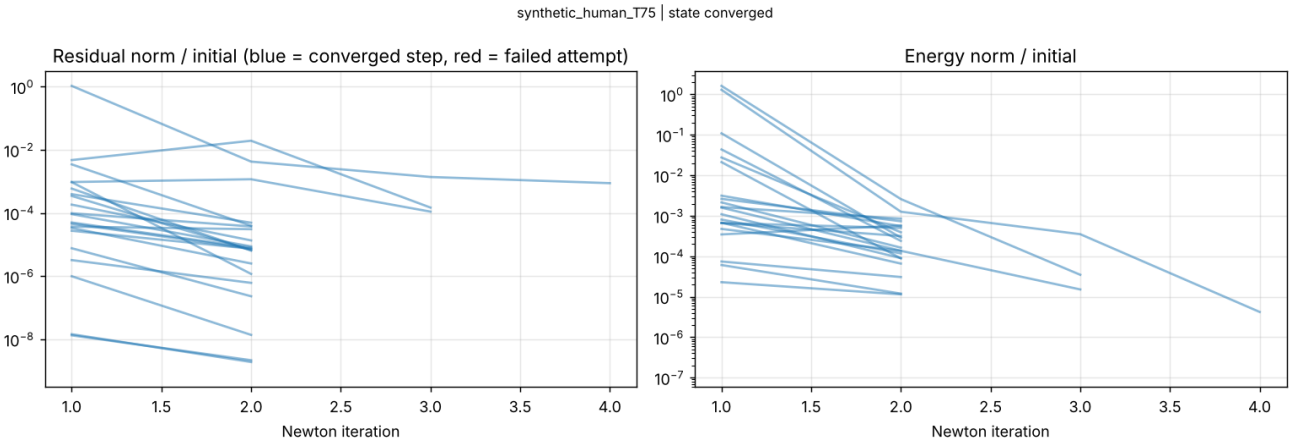


Figure 2: Newton convergence history.

5 Results (actual FEBio fields)

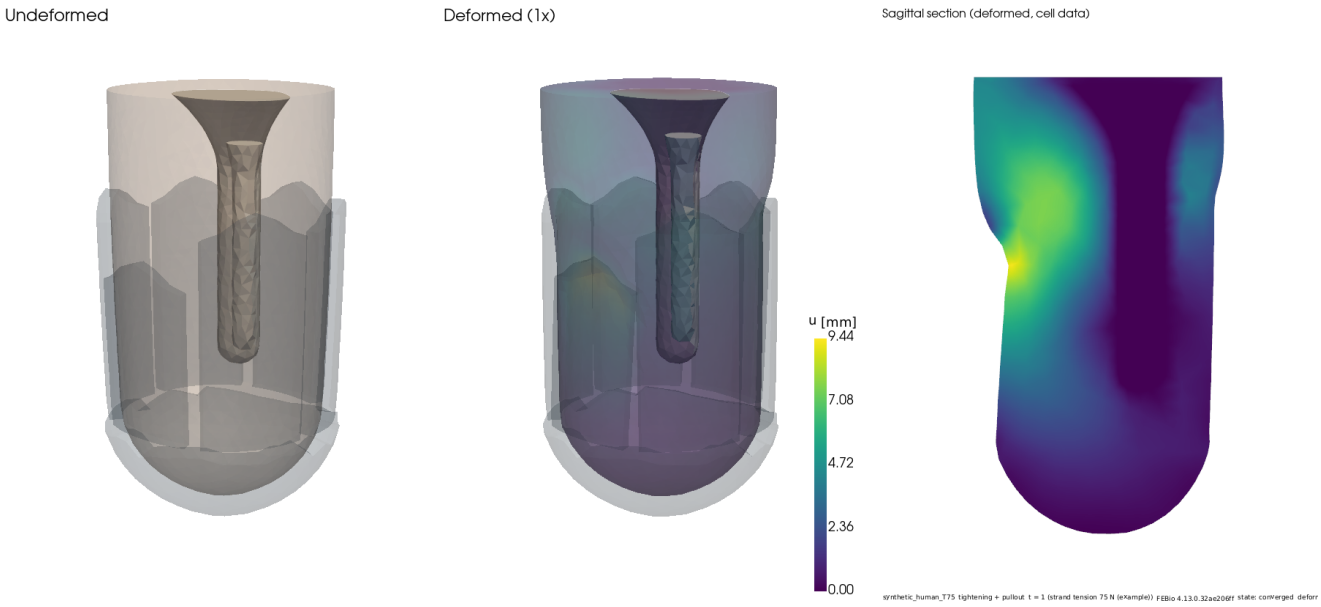


Figure 3: Full limb, undeformed and deformed at 1× (true scale), with sagittal section.

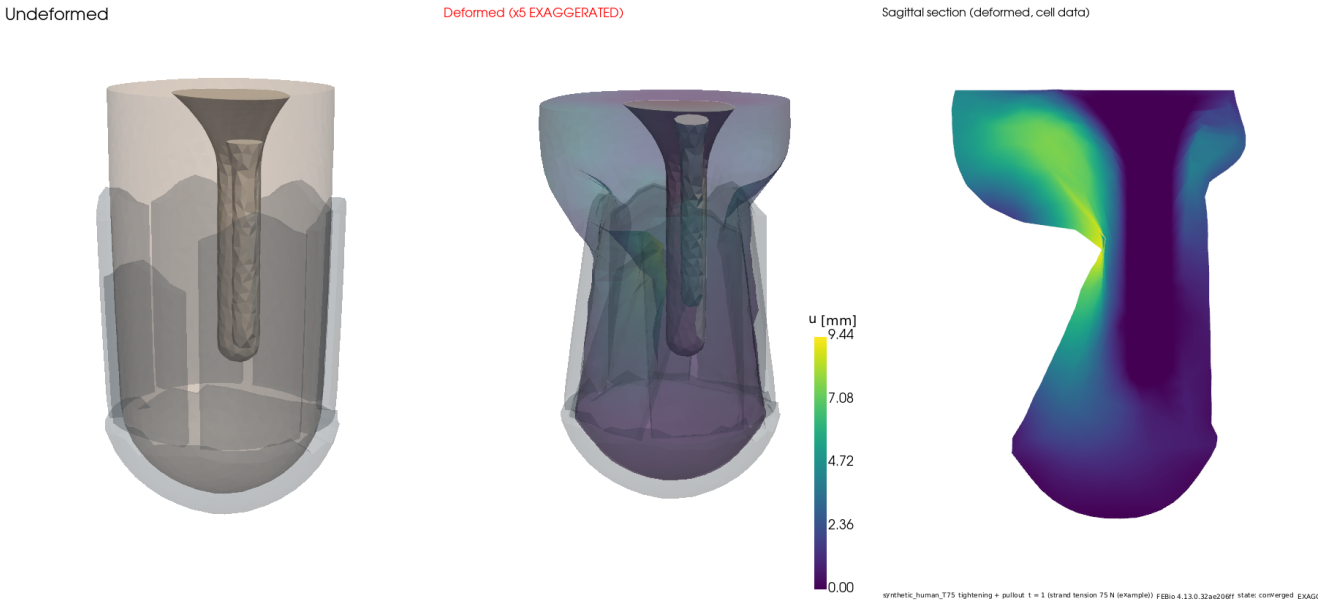


Figure 4: **EXAGGERATED** deformation (labelled scale) for visual inspection only.

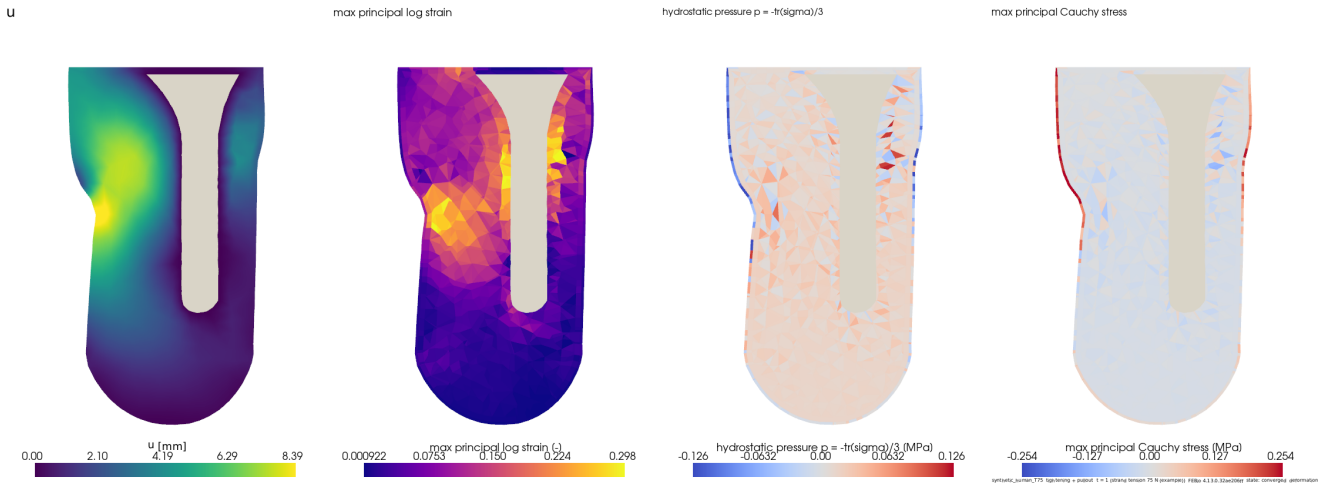


Figure 5: Sections through the deformed limb: displacement, maximum principal log strain, hydrostatic pressure, maximum principal Cauchy stress (cell data, no smoothing). Peak values may be mesh-dependent and are not injury predictions.

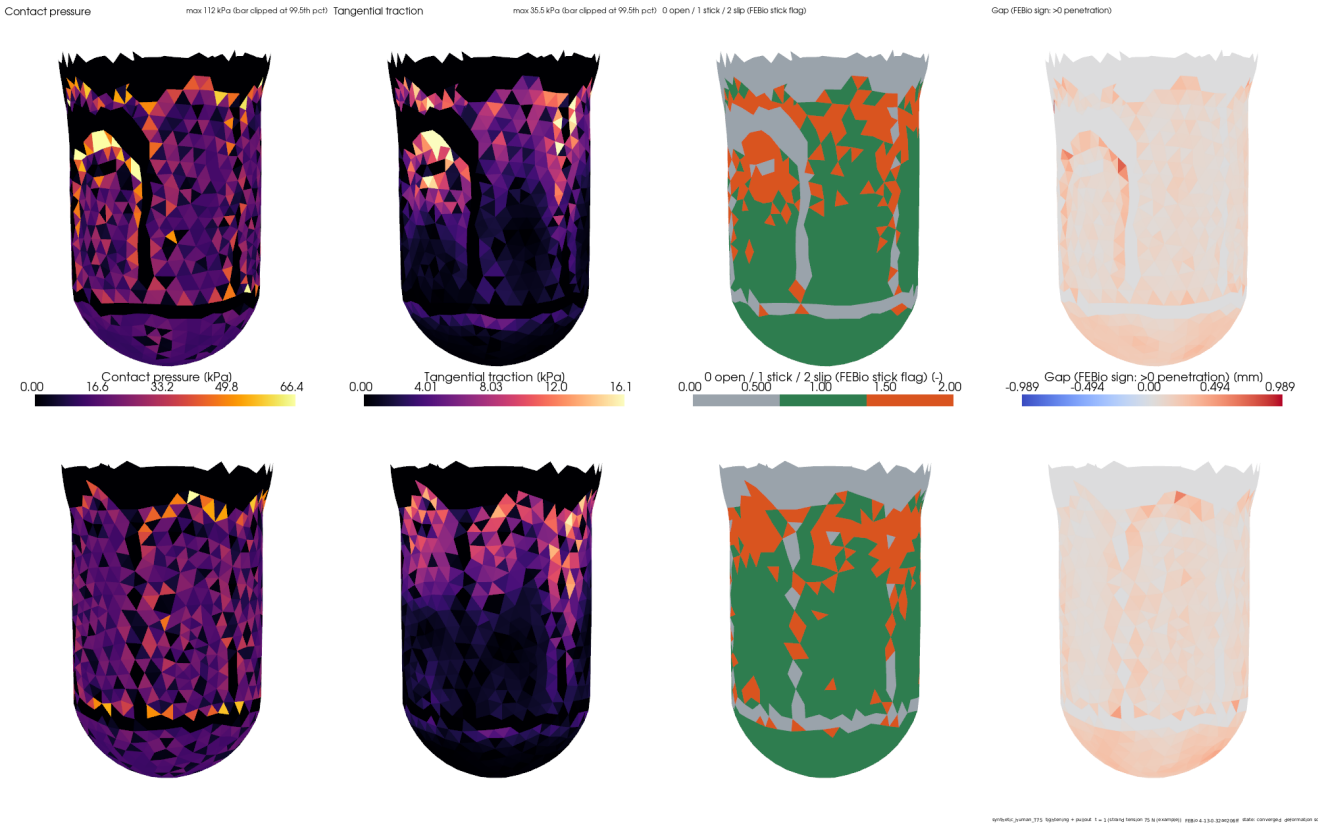


Figure 6: Skin contact pressure, tangential traction, derived stick/slip status and gap.

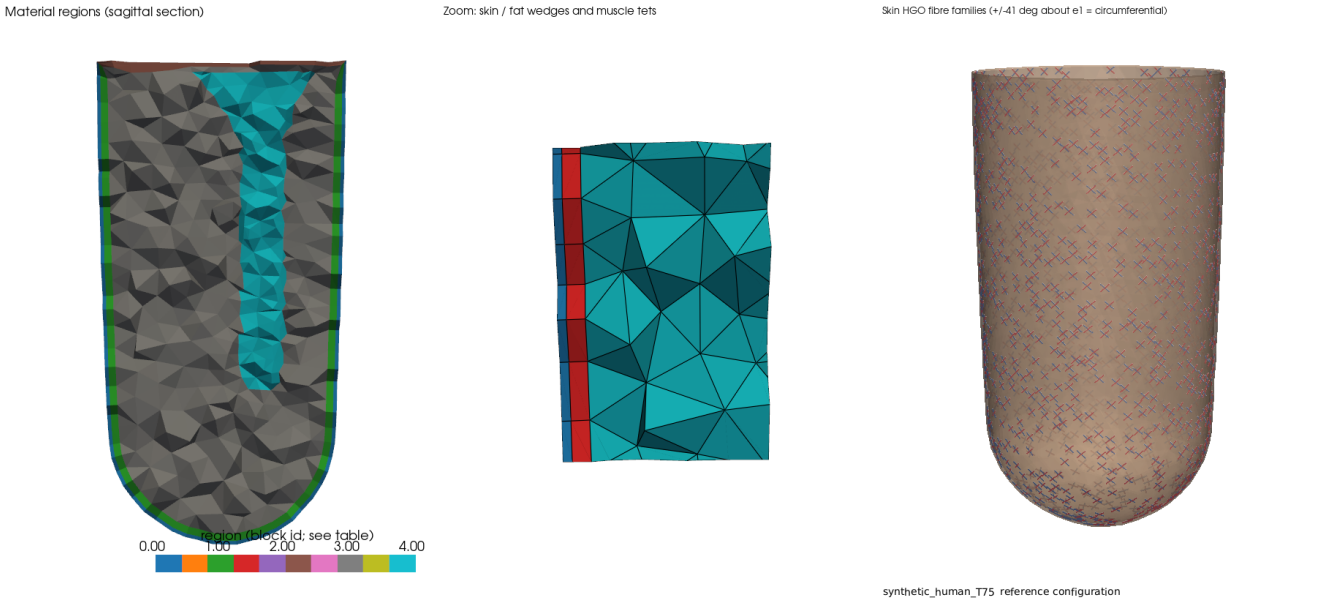


Figure 7: Material regions and skin fibre orientation.

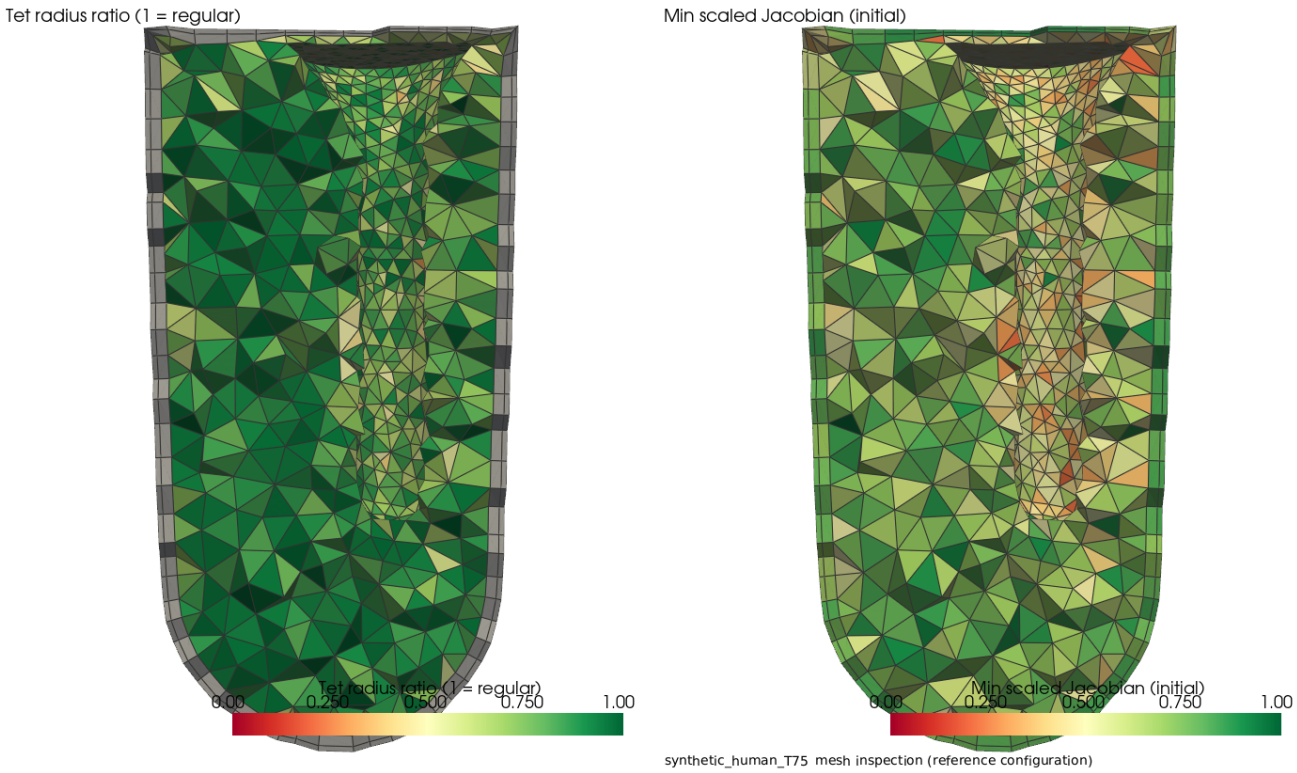


Figure 8: Mesh element quality.

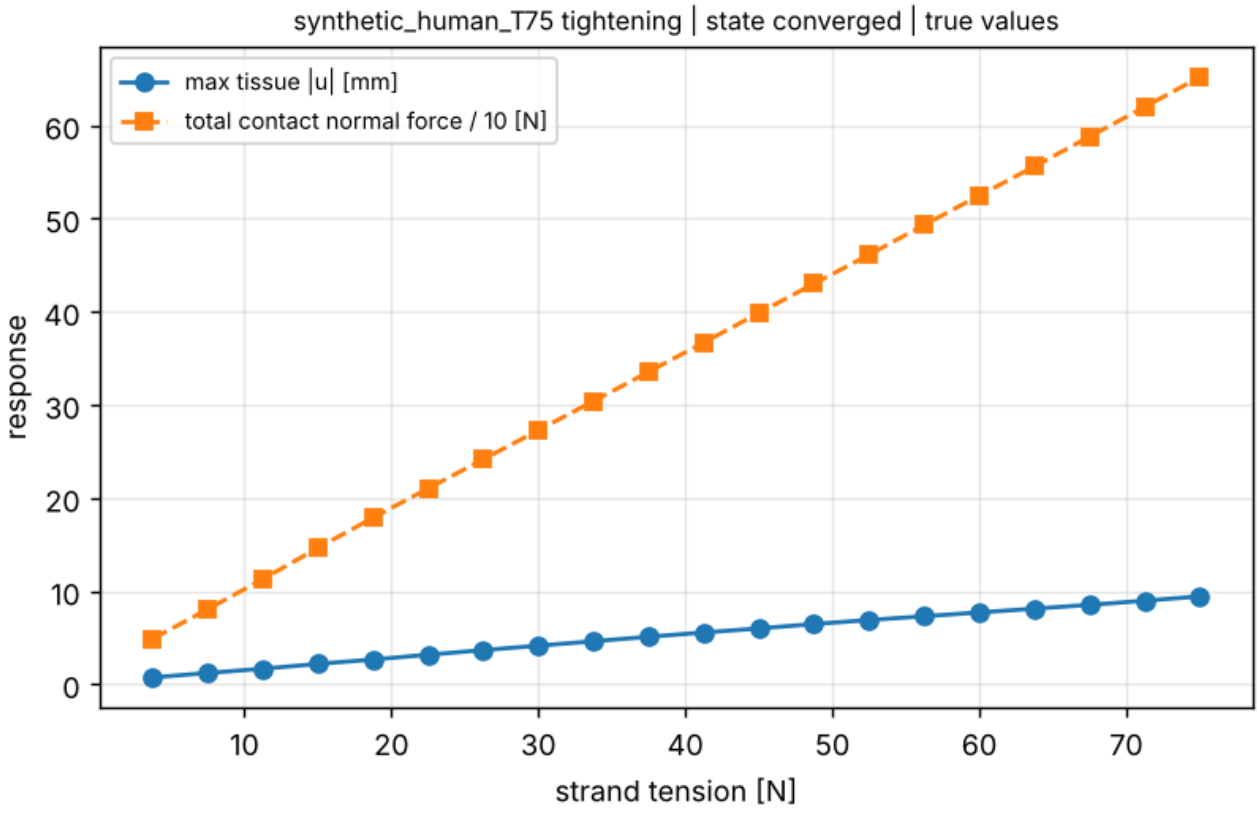


Figure 9: Force–displacement / load–response curves.

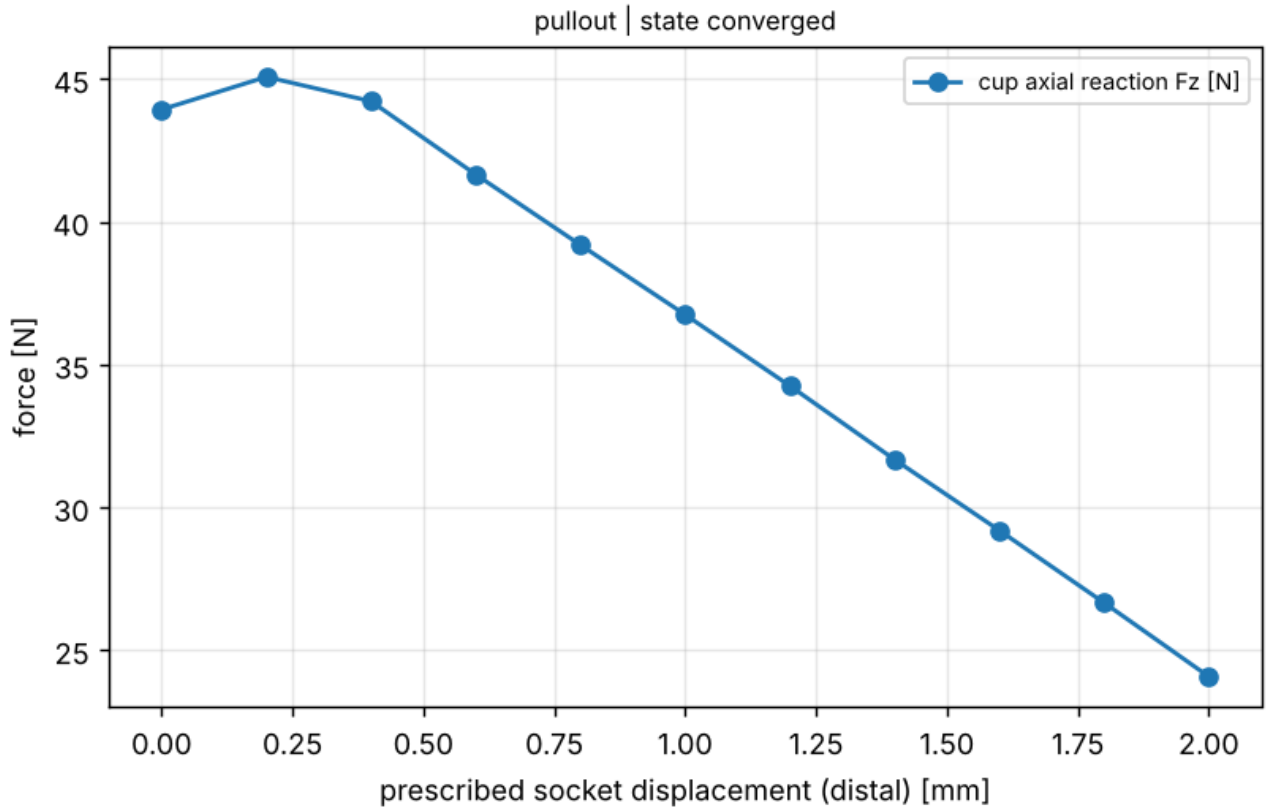


Figure 10: Pull-out: reaction versus relative socket displacement.

t	max —u— tissue mm	min J	inverted	contact N	max p kPa	slip area frac.	force imbalance
0.05	0.74	0.9826	0	48.9	10.61	0.4753	0.000154
0.1	1.214	0.9702	0	80.56	13.75	0.4292	0.004488
0.15	1.673	0.9585	0	113	18.91	0.4053	0.002228
0.2	2.186	0.9459	0	146.4	24.23	0.3578	6.352e-08
0.25	2.664	0.9343	0	178.9	29.5	0.3335	1.852e-05
0.3	3.175	0.9246	0	210.3	35.45	0.3246	9.61e-05
0.35	3.67	0.9157	0	241.5	42.76	0.3292	1.134e-05
0.4	4.146	0.9072	0	272.8	49.65	0.3208	3.989e-05
0.45	4.621	0.8984	0	304	56.59	0.3132	0.0001699
0.5	5.103	0.8876	0	335.4	64.67	0.2995	0.0001881
0.55	5.561	0.8774	0	367	71.64	0.2892	1.85e-06
0.6	5.999	0.8673	0	398.6	77.94	0.2746	0.0004983
0.65	6.47	0.8575	0	430.1	84.94	0.2711	0.0001175
0.7	6.903	0.8482	0	461.2	91.7	0.2593	0.0002405
0.75	7.306	0.8389	0	493.2	98.1	0.249	4.051e-05
0.8	7.715	0.8297	0	524.7	104.3	0.2471	3.684e-05
0.85	8.123	0.8206	0	556	111.8	0.2332	5.836e-05
0.9	8.528	0.8121	0	588	99.4	0.2237	4.91e-05
0.95	8.972	0.804	0	619.8	113.1	0.2198	1.709e-06
1	9.437	0.7953	0	652	112	0.2145	8.778e-05
1.1	9.755	0.7857	0	660.3	148.8	0.1798	5.827e-06
1.2	9.887	0.7794	0	661.6	138.3	0.1616	3.955e-06
1.3	10.08	0.7748	0	660.9	127.1	0.1687	0.0001475
1.4	10.11	0.7708	0	659.2	135.6	0.1672	2.653e-06
1.5	10.13	0.7669	0	657.3	136.6	0.1661	3.434e-05
1.6	10.13	0.7627	0	655.1	137.2	0.1674	7.766e-06
1.7	10.12	0.759	0	653	137.7	0.1741	4.486e-05
1.8	10.12	0.7552	0	650.8	137.6	0.1777	9.247e-06
1.9	10.19	0.7512	0	648.8	126	0.1762	3.558e-06

t	max —u— tissue mm	min J	inverted	contact N	max p kPa	slip area frac.	force imbalance
2	10.22	0.7471	0	646.8	140.6	0.1731	2.082e-05

Petal free bodies at t = 1 (force magnitudes, N). Pad contact force is the facet-averaged traction on the skin zone times the deformed facet area (an approximate post-processed integral); the global reaction balance in the table above is the exact check.

petal	—cable—	—hinge—	—pad contact—	—stabiliser—	—residual—	residual/cable
petal1	63.3	13	74.1	0.0633	0.267	0.00422
petal2	78.9	12.2	87	0.175	0.125	0.00158
petal3	79.5	11.5	87.4	0.192	0.256	0.00322
petal4	69.5	20.7	87.9	0.422	0.258	0.00371
petal5	79.6	10.2	85.5	0.161	0.0335	0.000421
petal6	78.7	12.3	85.6	0.182	0.0531	0.000676

block	max —u—	max log e	min log e	max p MPa	min p MPa	max vM MPa	min J
skin	10.22	0.1794	-0.1815	0.1573	-0.3318	0.5843	0.9922
fat	10.22	0.2863	-0.2837	0.03743	-0.007994	0.008024	0.9356
proximal_cap	4.403	0.2033	-0.2206	0.03708	-0.03746	0.004312	0.9385
muscle	9.508	0.3949	-0.479	0.2029	-0.09444	0.01604	0.7471
petal1_pad	2.856	0.06984	-0.07983	0.04257	-0.005695	0.02726	0.9972
petal2_pad	4.933	0.06928	-0.08165	0.04332	-0.0006859	0.02778	0.9957
petal3_pad	5.216	0.0753	-0.1038	0.0518	-0.004717	0.03346	0.9946
petal4_pad	10.45	0.1393	-0.1574	0.1147	-0.01002	0.0533	0.9905
petal5_pad	4.611	0.069	-0.1105	0.04835	-0.0003392	0.03384	0.9949
petal6_pad	4.945	0.07266	-0.09954	0.04722	-0.005397	0.03176	0.9963
distal_cushion	2.134	0.1388	-0.151	0.0227	-0.008104	0.01003	0.99

6 Limitations

- Numerical verification is separate from experimental or clinical validation; no validation data were supplied.
- Tissue layers are geometric assumptions; material parameters come from literature on other subjects/sites (see table) or are labelled assumptions.
- The socket is a provisional parametric model; cable routing is provisional unless the configuration supplies verified routing.
- Quasi-static, no viscoelasticity, no perfusion, no active muscle, no skin adhesion or liner; friction is Coulomb with a screening coefficient.
- A converged state does not establish grip; pull-out is evaluated only through the resolved contact tractions and relative motion of this model.