


Mean Allan deviation

Run 20260910_170948 | Arithmetic mean across 9 channel pairs

13.78 ms: 41.385 μrad^2

118 s: 23.3154 μrad^2

Tail slope: -0.166

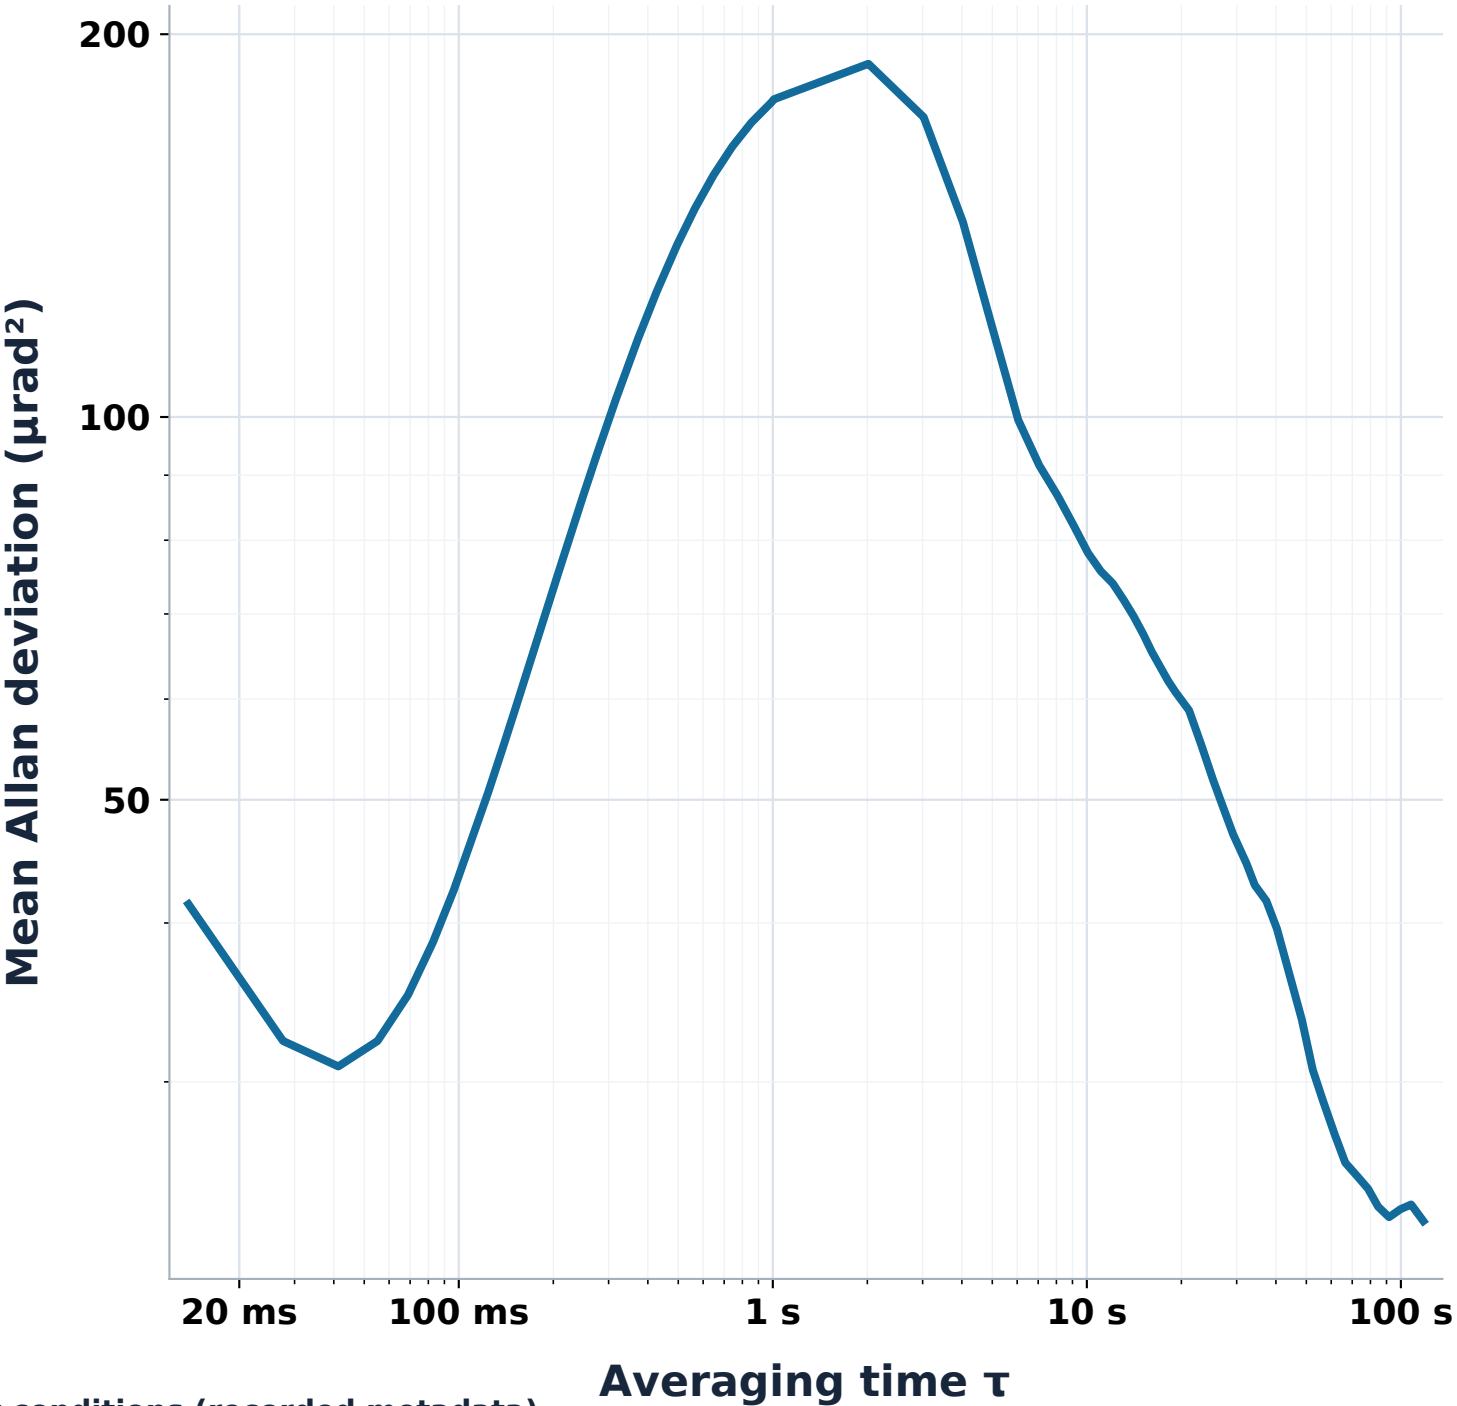

Measurement conditions (recorded metadata)

Vacuum sanity check | 780 nm | 294 K | OPO enabled | Si detector

High-pass + band-pass filters | Power-detector attenuation: 40 dB | Duration: 20 min 07 s

Delay scan: 15-35 mm at 2 mm/s | Recorded powers (1 / 2): 0.24 / 0.31 mW

Equal-weight mean of the nine individual Allan deviations at each averaging time; no smoothing or detrending.

Ranges joined near 1 s: nominal frame timing below the join; saved profile-timed, binned results above it.

Tail slope fits the final eight mean-curve points. This delay-scan record does not identify a stationary noise process.