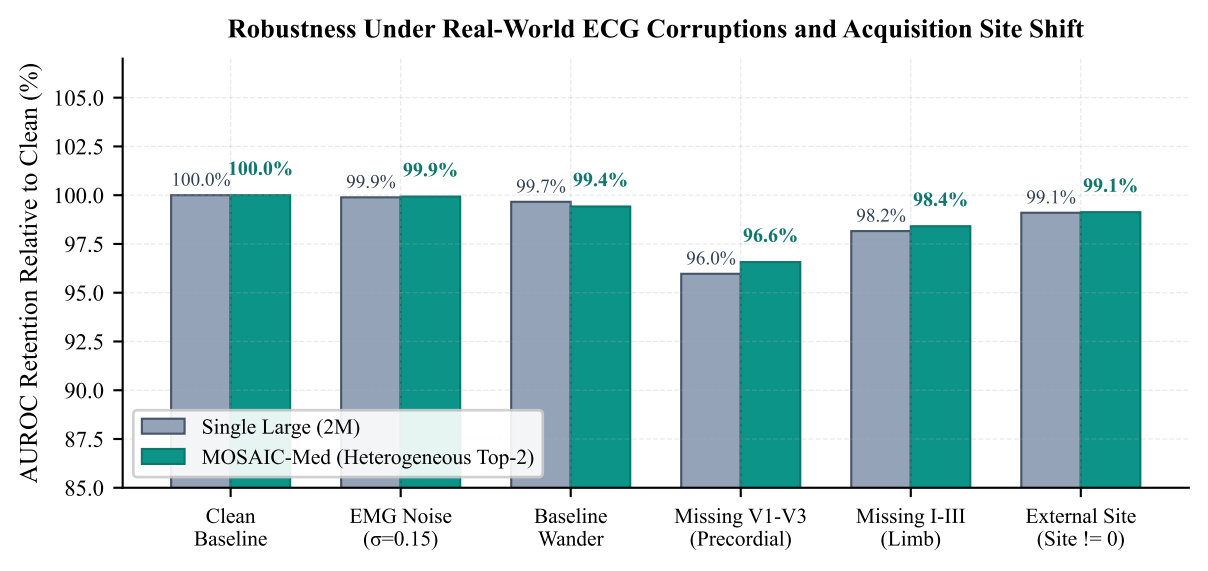
Robustness Under Real-World ECG Corruptions and Acquisition Site Shift
AUROC Retention Relative to Clean (%)
105.0
102.5
100.0
97.5
95.0
92.5
90.0
87.5
85.0
100.0%
100.0%
99.9%
99.9%
99.7%
99.4%
96.0%
96.6%
98.2%
98.4%
99.1%
99.1%
Single Large (2M)
MOSAIC-Med (Heterogeneous Top-2)
Clean Baseline
EMG Noise (σ=0.15)
Baseline Wander
Missing V1-V3 (Precordial)
Missing I-III (Limb)
External Site (Site != 0)